

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092019\
 Data File : PD054804.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Sep 2019 16:31
 Operator : SG\AJ
 Sample : K4890-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AS3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 23:52:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.297	3.965	4834232	6305468	7.157	7.730
27) SA Decachlor...	7.978	9.003	16538710	19066418	18.767	18.542
Target Compounds						
10) B trans-Chl...	0.000	6.047	0	2552360	N.D.	2.308


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092019\
Data File : PD054804.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Sep 2019 16:31
Operator : SG\AJ
Sample : K4890-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AS3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 23:52:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

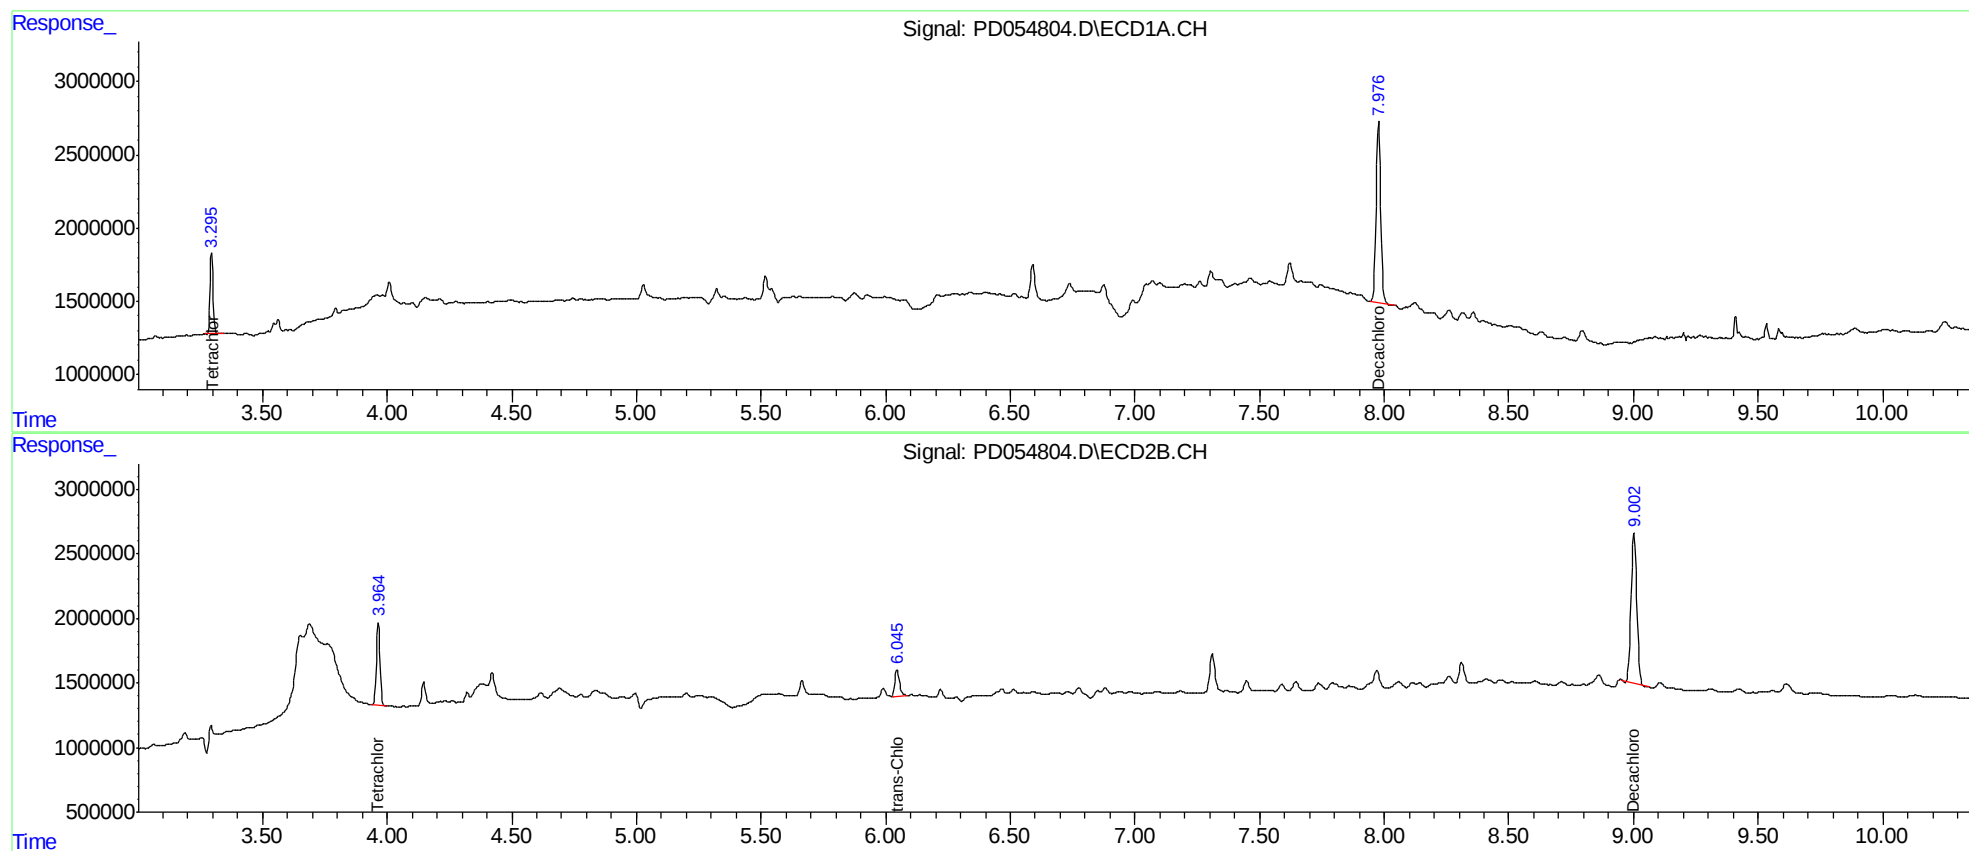


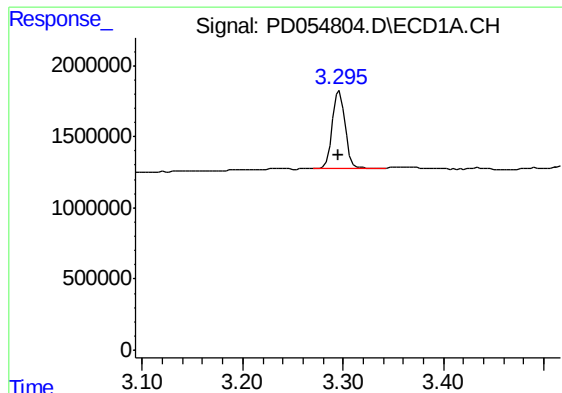

#1 Tetrachloro-m-xylene


R.T.: 3.297 min
Delta R.T.: 0.002 min
Response: 4834232
Conc: 7.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS3

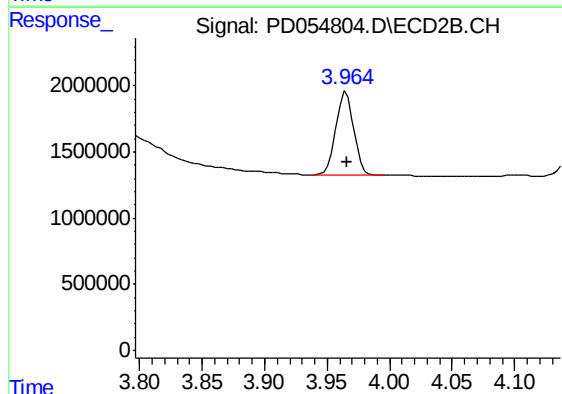


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 6305468
Conc: 7.73 ng/ml

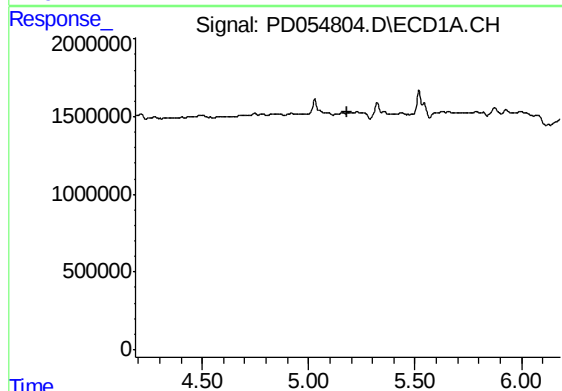


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

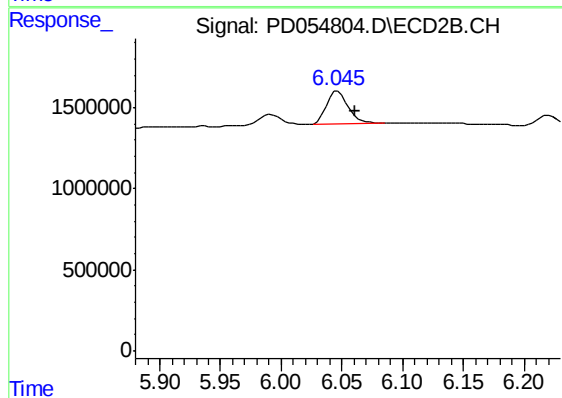

#10 trans-Chlordane


R.T.: 6.047 min
Delta R.T.: -0.015 min
Response: 2552360
Conc: 2.31 ng/ml

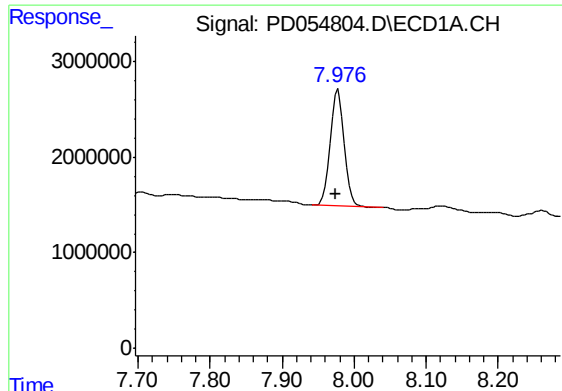

#27 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: 0.003 min
Response: 16538710
Conc: 18.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS3

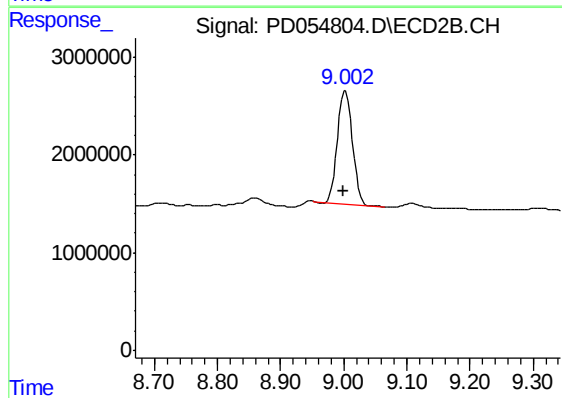

#27 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: 0.002 min
Response: 19066418
Conc: 18.54 ng/ml