

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 12:10
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1084

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 14:58:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 20 14:57:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.011	4589403	39437160	5.305	5.486
27)	SA Decachlor...	8.232	9.081	17154496	48248512	11.682	10.956
Target Compounds							
2)	A alpha-BHC	3.931	4.406	5769457	50206735	4.916	5.215
3)	MA gamma-BHC...	4.215	4.692	6433468	49911157	5.333	5.425
4)	MA Heptachlor	4.512	5.196	6744193	46415250	5.311	5.486
9)	A Endosulfan I	5.540	6.248	6305536	35586473	5.319	5.396
13)	MA Dieldrin	5.783	6.506	12977114	73887260	10.143	10.724
14)	MA Endrin	6.041	6.725	11940804	63125621	9.950	12.211
16)	A 4,4'-DDD	6.162	6.848	10483870	59404243	9.838	10.679
17)	MA 4,4'-DDT	6.402	7.146	11429692	57122450	9.897	10.388
20)	A Methoxychlor	6.948	7.605	37039631	151.2E6	53.491	57.820


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 12:10
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 14:58:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 20 14:57:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

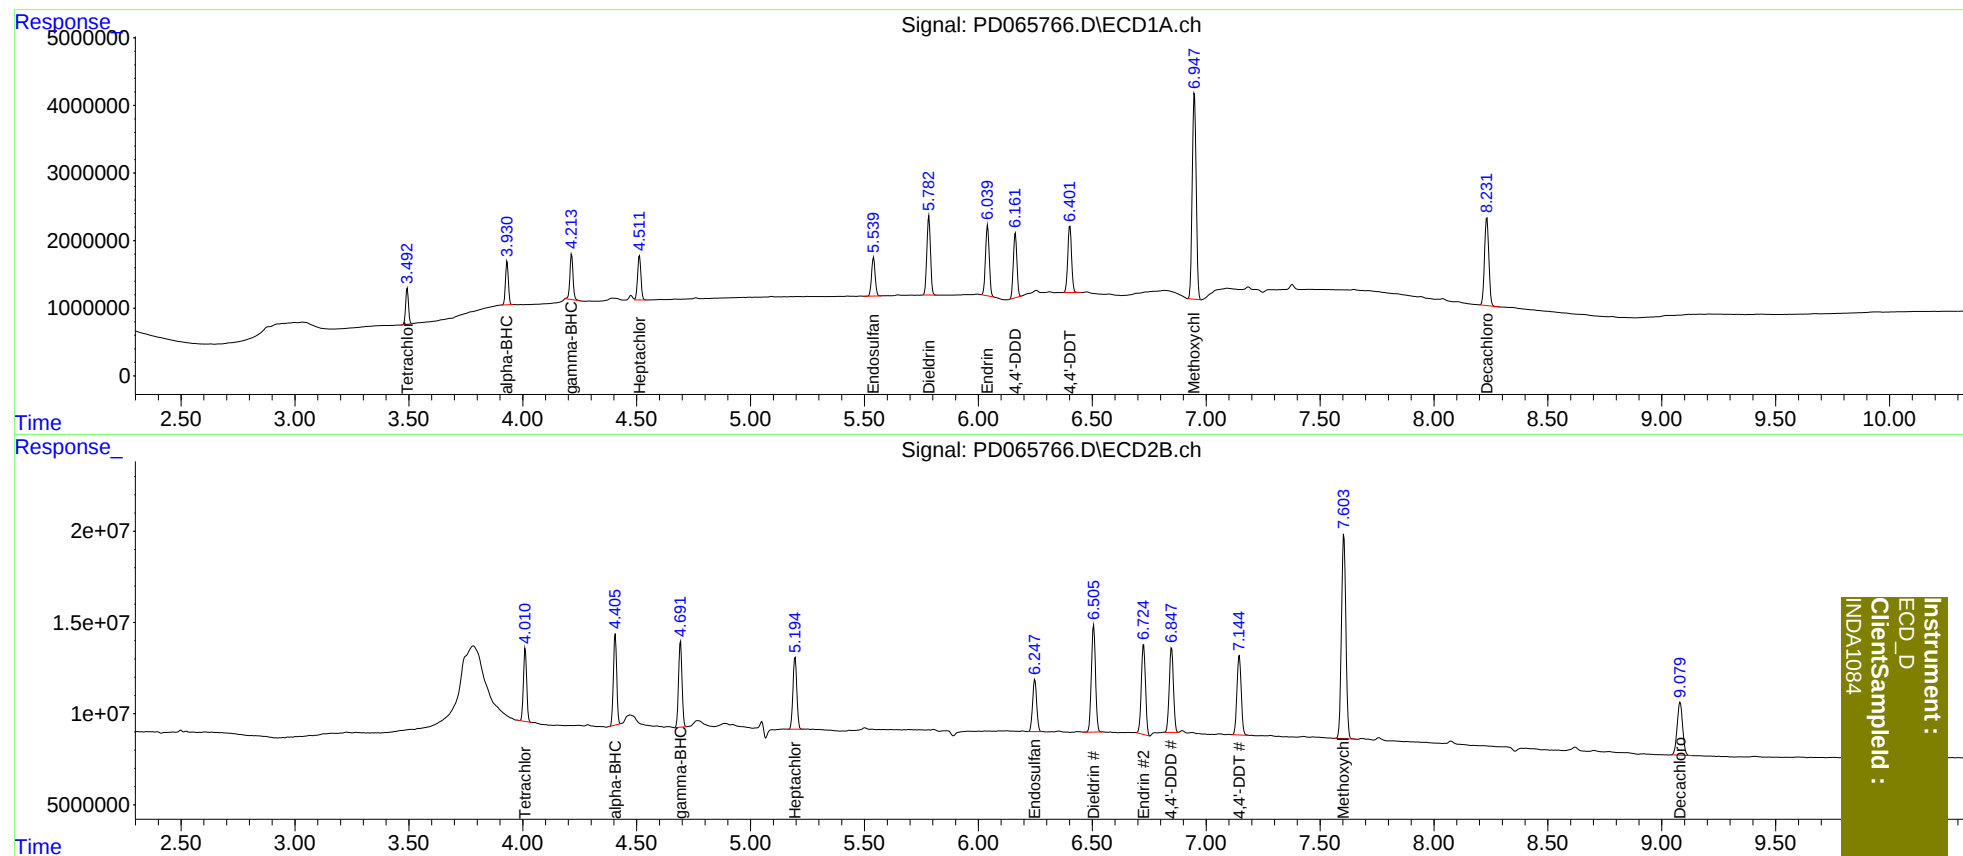


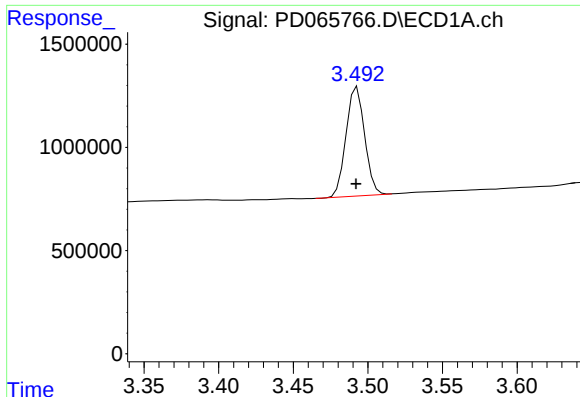

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 4589403
Conc: 5.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

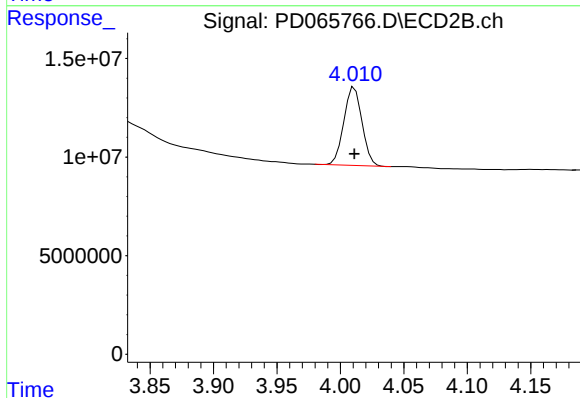


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 39437160
Conc: 5.49 ng/ml

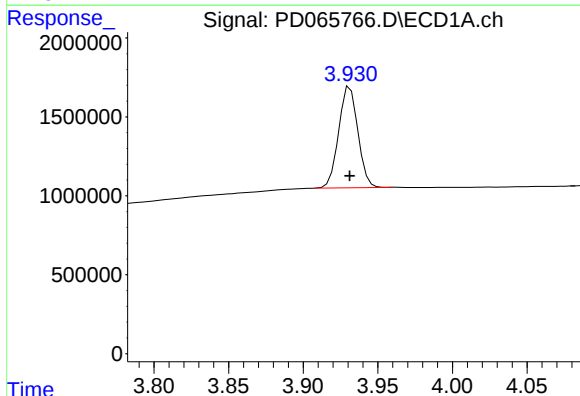


#2 alpha-BHC

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 5769457
Conc: 4.92 ng/ml

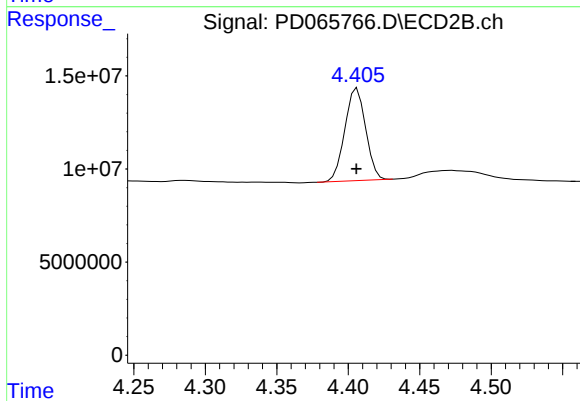

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 50206735
Conc: 5.22 ng/ml

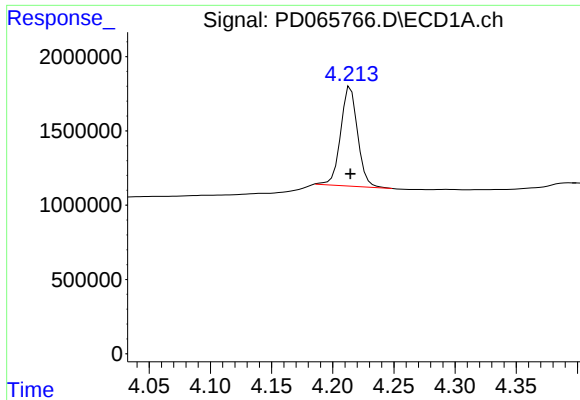

#3 gamma-BHC (Lindane)


R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 6433468
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

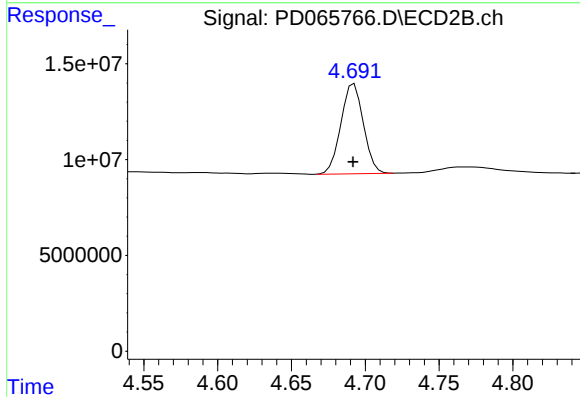


#3 gamma-BHC (Lindane)

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 49911157
Conc: 5.42 ng/ml

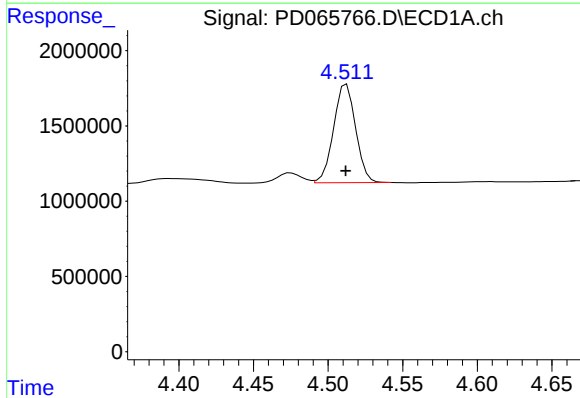


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 6744193
Conc: 5.31 ng/ml

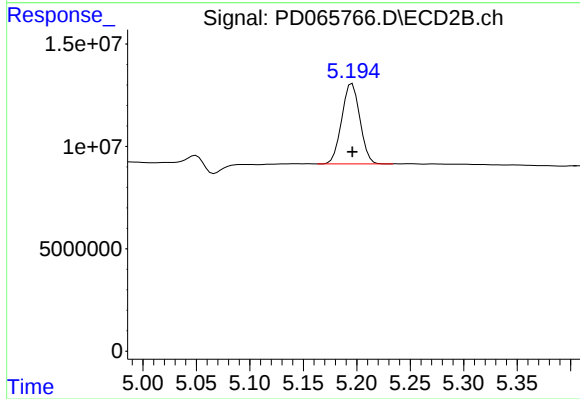

#4 Heptachlor


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 46415250
Conc: 5.49 ng/ml

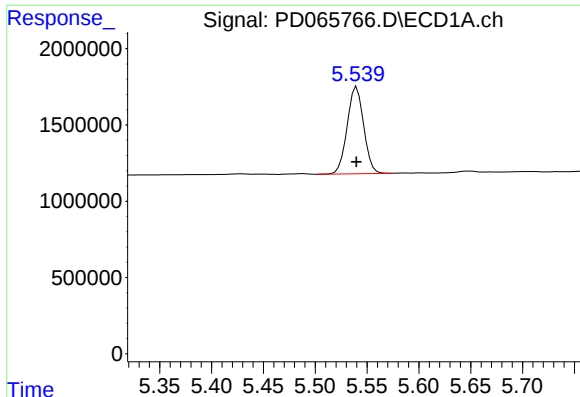

#9 Endosulfan I


R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 6305536
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

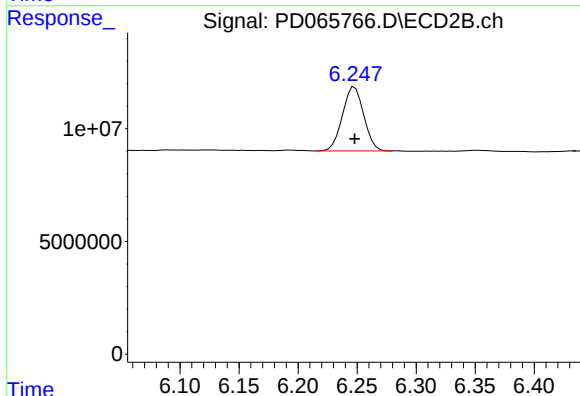


#9 Endosulfan I

R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 35586473
Conc: 5.40 ng/ml

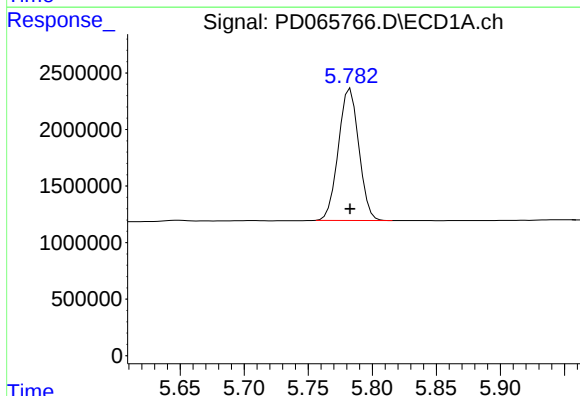


#13 Dieldrin

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 12977114
Conc: 10.14 ng/ml

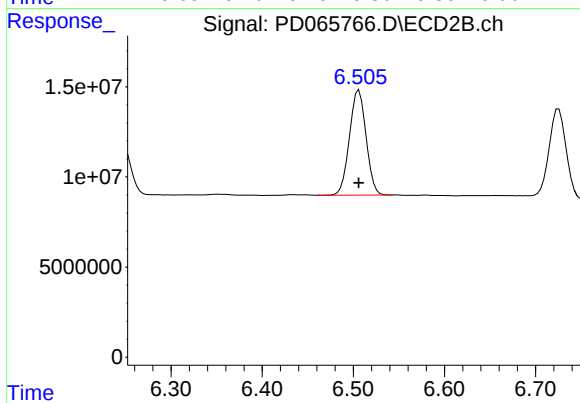

#13 Dieldrin


R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 73887260
Conc: 10.72 ng/ml

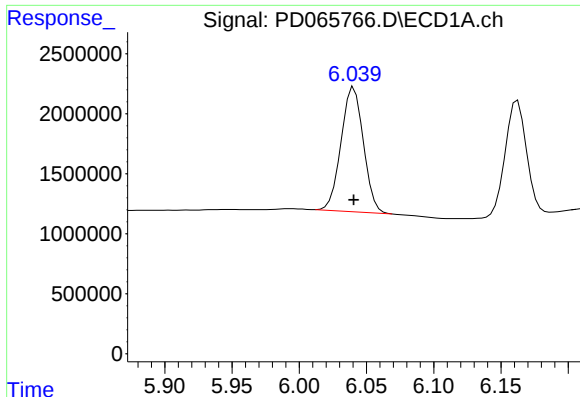

#14 Endrin


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 11940804
Conc: 9.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

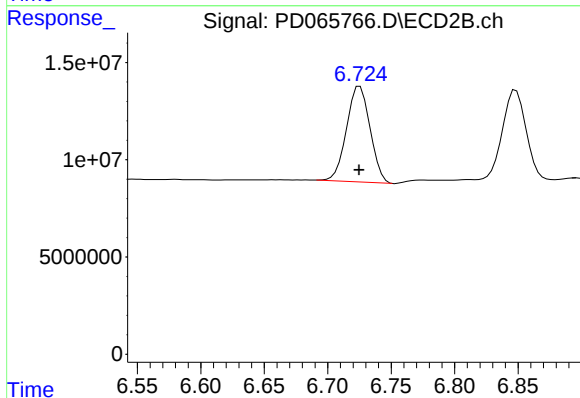


#14 Endrin

R.T.: 6.725 min
Delta R.T.: 0.000 min
Response: 63125621
Conc: 12.21 ng/ml

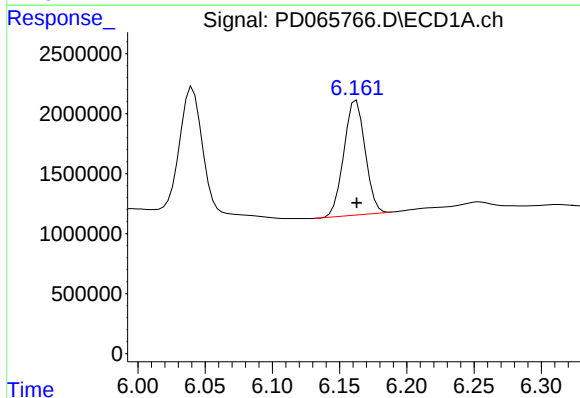


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 10483870
Conc: 9.84 ng/ml

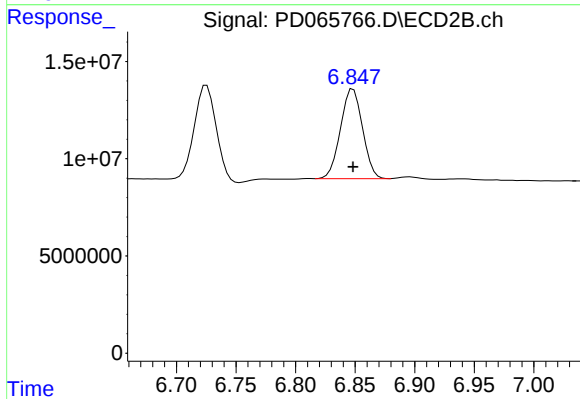

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 59404243
Conc: 10.68 ng/ml

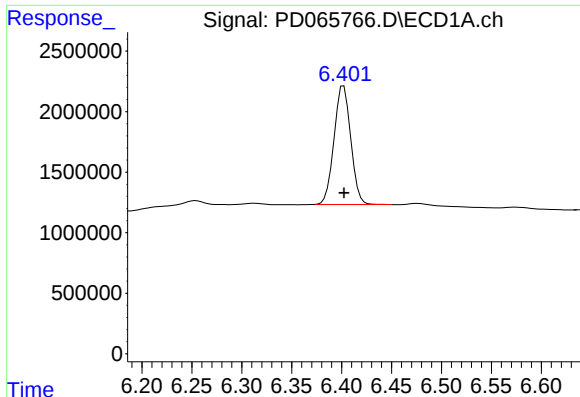

#17 4,4'-DDT


R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 11429692
Conc: 9.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

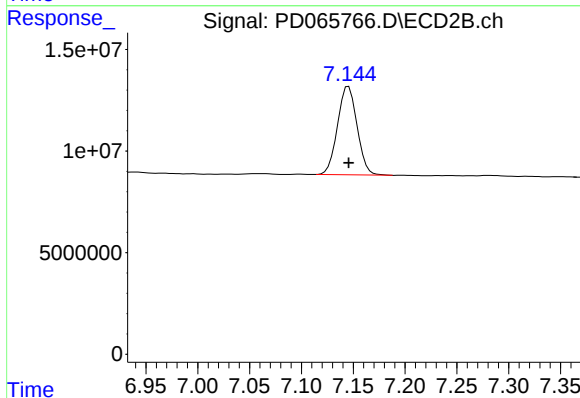


#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 57122450
Conc: 10.39 ng/ml

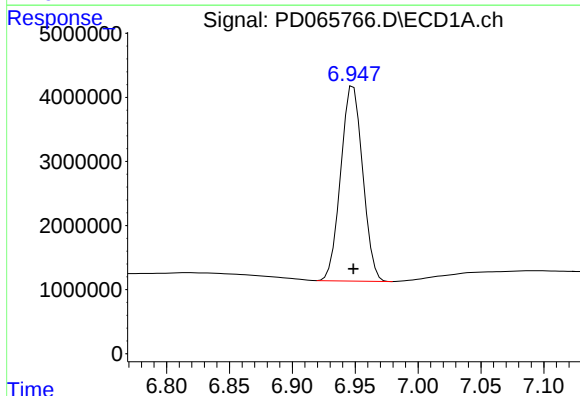


#20 Methoxychlor

R.T.: 6.948 min
Delta R.T.: 0.000 min
Response: 37039631
Conc: 53.49 ng/ml

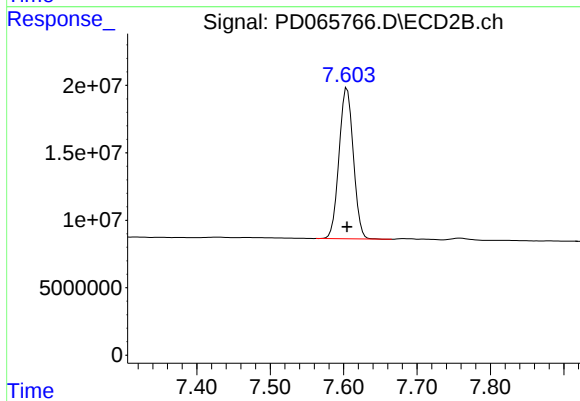

#20 Methoxychlor


R.T.: 7.605 min
Delta R.T.: 0.000 min
Response: 151232528
Conc: 57.82 ng/ml

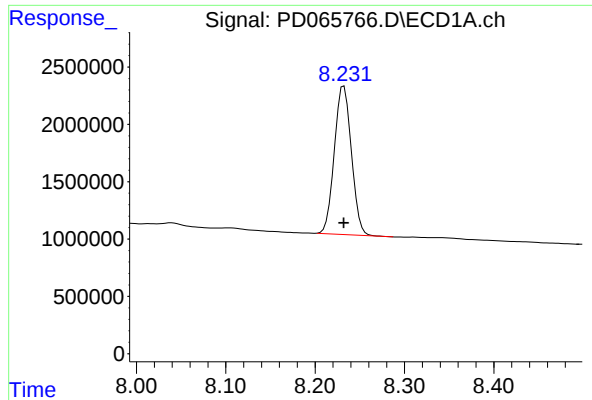

#27 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: 0.000 min
Response: 17154496
Conc: 11.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1084

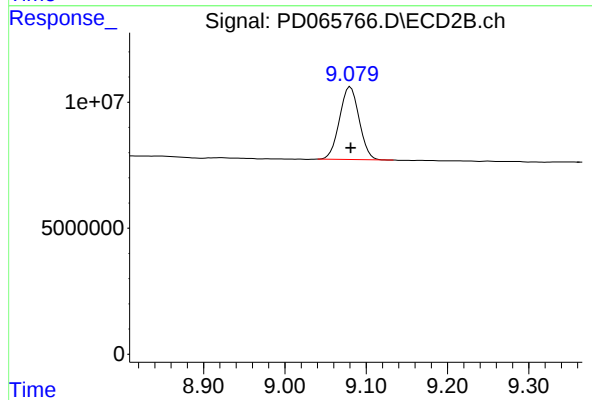

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 48248512
Conc: 10.96 ng/ml