

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 12:38
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 14:58:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 20 14:57:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	8927934	74944885	10.321	10.425
27)	SA Decachlor...	8.233	9.081	31228684	92216672	21.266	20.939
Target Compounds							
2)	A alpha-BHC	3.932	4.407	11458195	97710455	9.763	10.150
3)	MA gamma-BHC...	4.215	4.693	12069089	94856543	10.004	10.310
4)	MA Heptachlor	4.513	5.196	12946039	88663899	10.195	10.479
9)	A Endosulfan I	5.540	6.249	12200272	68468305	10.292	10.381
13)	MA Dieldrin	5.783	6.507	25331097	141.7E6	19.800	20.564
14)	MA Endrin	6.041	6.726	23163263	119.1E6	19.301	23.029
16)	A 4,4'-DDD	6.163	6.848	20857918	114.8E6	19.574	20.634
17)	MA 4,4'-DDT	6.403	7.145	22630556	111.2E6	19.597	20.222
20)	A Methoxychlor	6.949	7.605	70955045	282.1E6	102.470	107.849


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 12:38
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 14:58:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 20 14:57:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

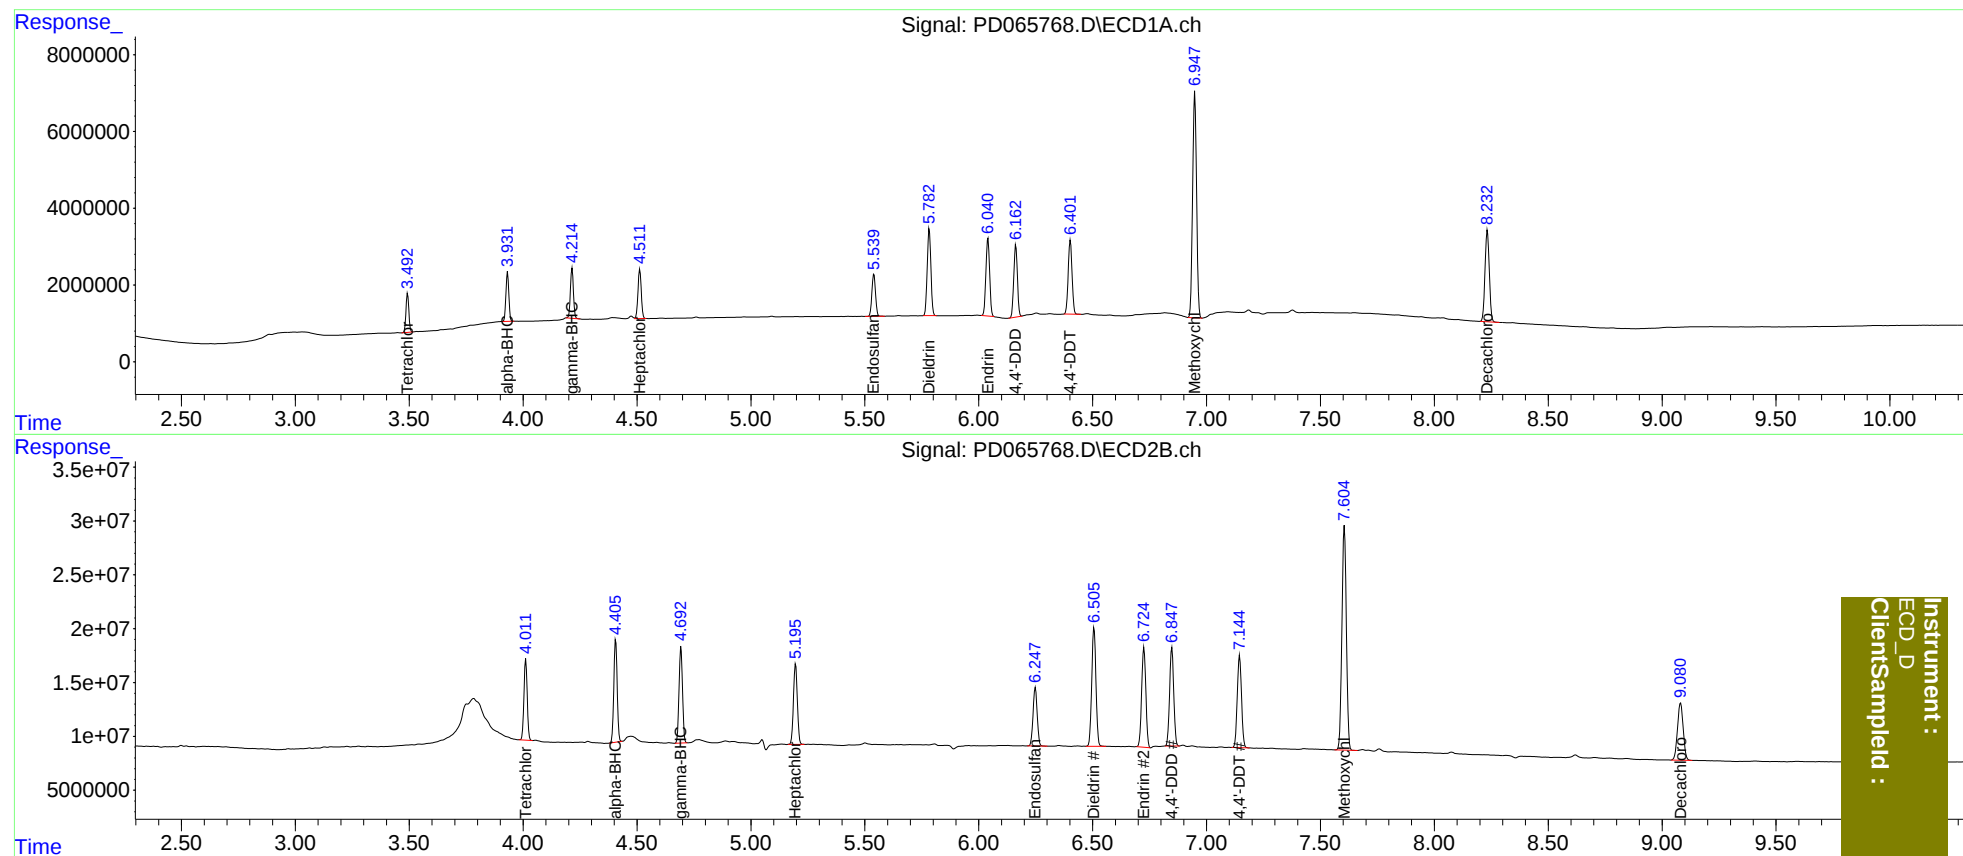


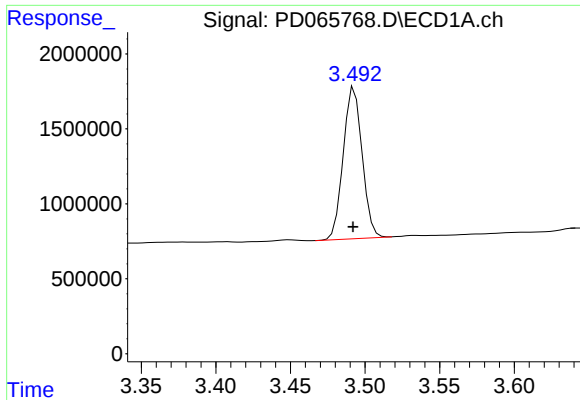

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 8927934
Conc: 10.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

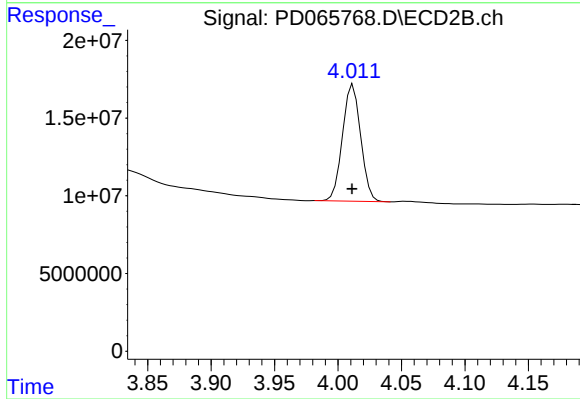


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 74944885
Conc: 10.42 ng/ml

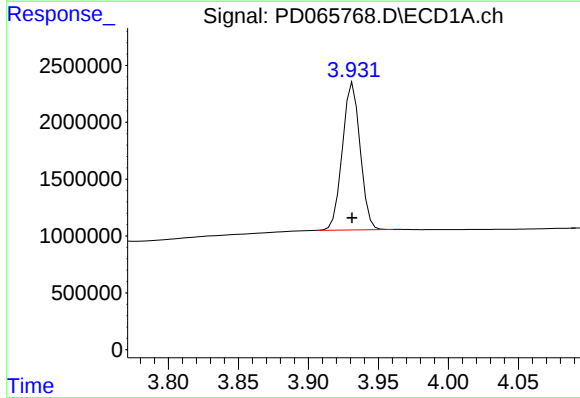


#2 alpha-BHC

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 11458195
Conc: 9.76 ng/ml

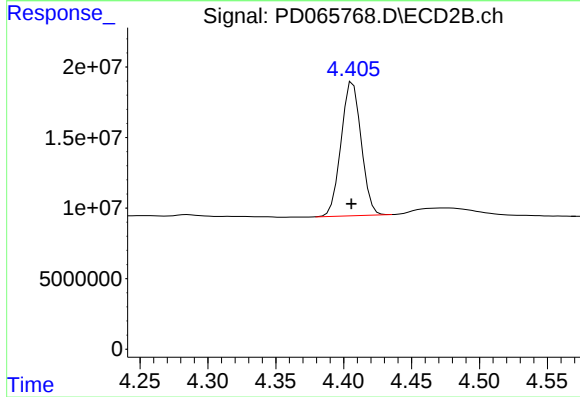

#2 alpha-BHC


R.T.: 4.407 min
Delta R.T.: 0.001 min
Response: 97710455
Conc: 10.15 ng/ml

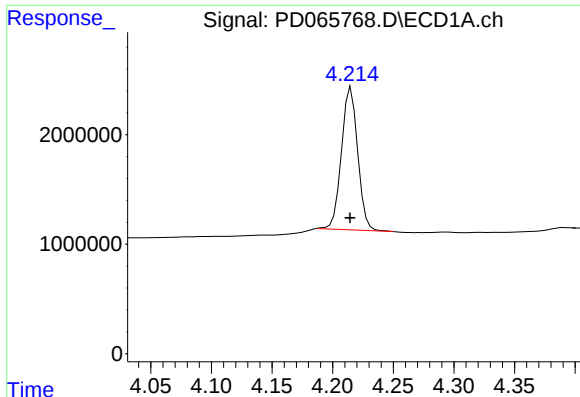

#3 gamma-BHC (Lindane)


R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 12069089
Conc: 10.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

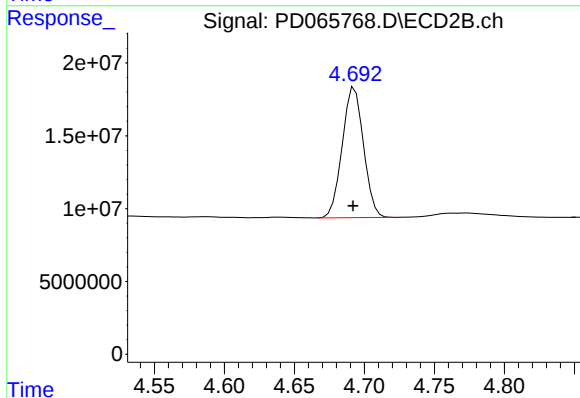


#3 gamma-BHC (Lindane)

R.T.: 4.693 min
Delta R.T.: 0.001 min
Response: 94856543
Conc: 10.31 ng/ml

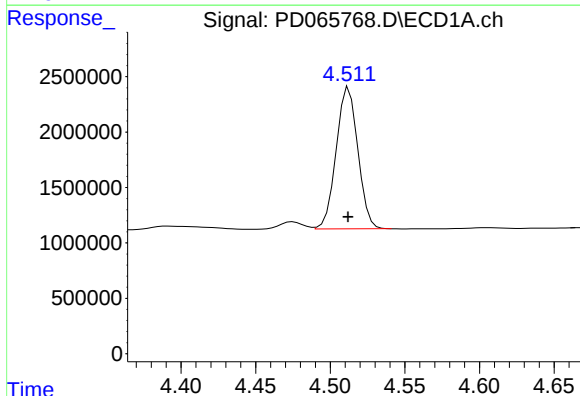


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 12946039
Conc: 10.19 ng/ml

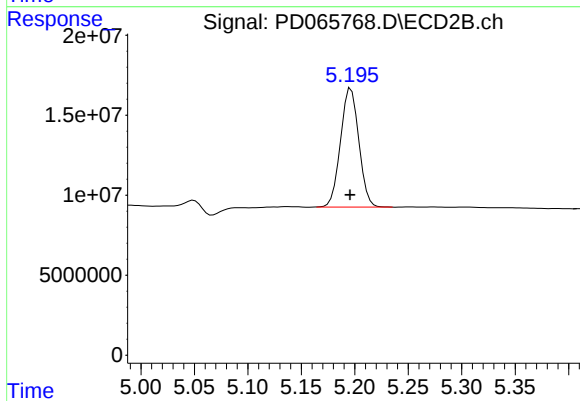

#4 Heptachlor


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 88663899
Conc: 10.48 ng/ml

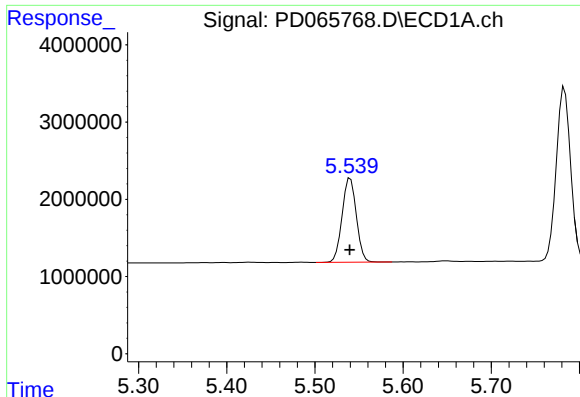

#9 Endosulfan I


R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 12200272
Conc: 10.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

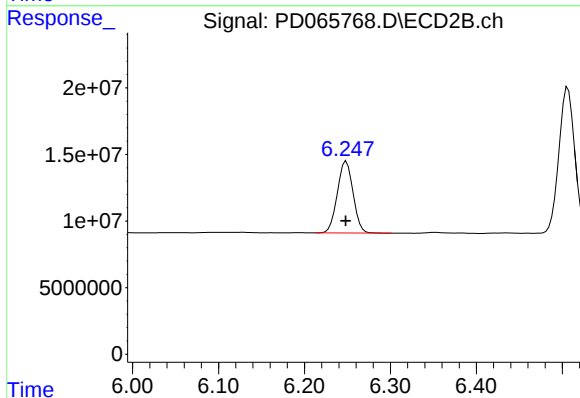


#9 Endosulfan I

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 68468305
Conc: 10.38 ng/ml

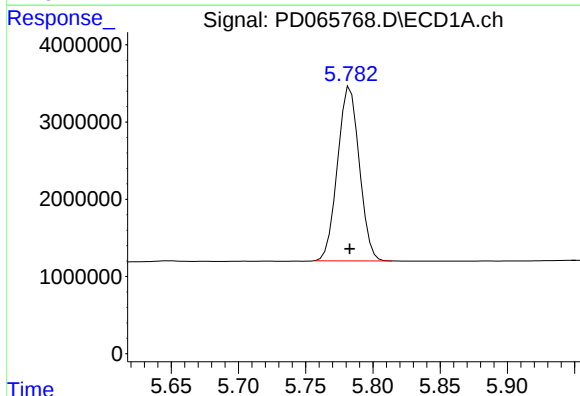


#13 Dieldrin

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 25331097
Conc: 19.80 ng/ml

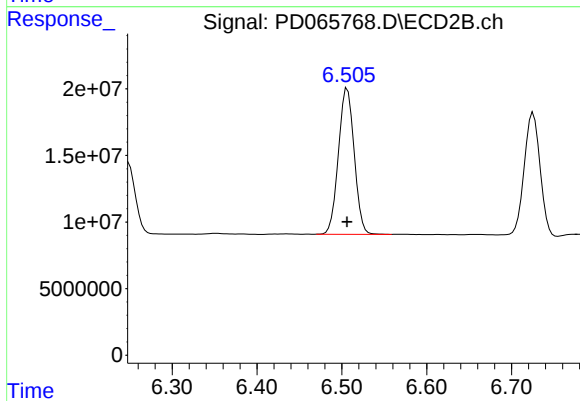

#13 Dieldrin


R.T.: 6.507 min
Delta R.T.: 0.000 min
Response: 141682623
Conc: 20.56 ng/ml

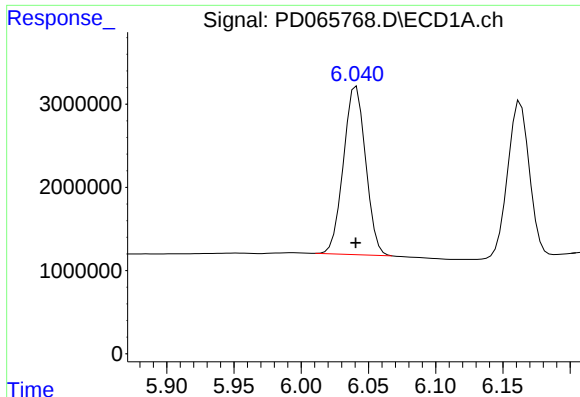

#14 Endrin


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 23163263
Conc: 19.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

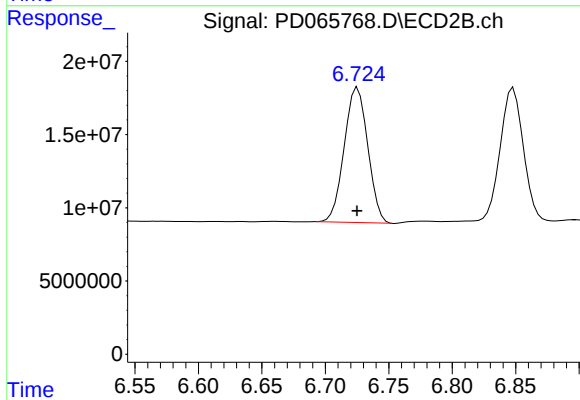


#14 Endrin

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 119053104
Conc: 23.03 ng/ml

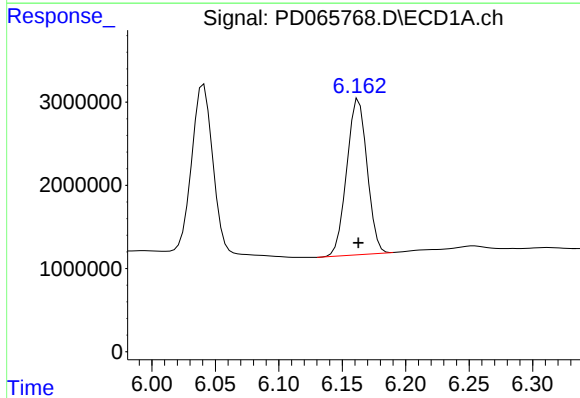


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 20857918
Conc: 19.57 ng/ml

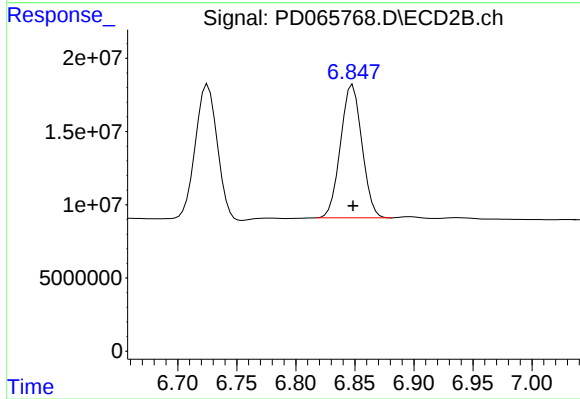

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 114785211
Conc: 20.63 ng/ml

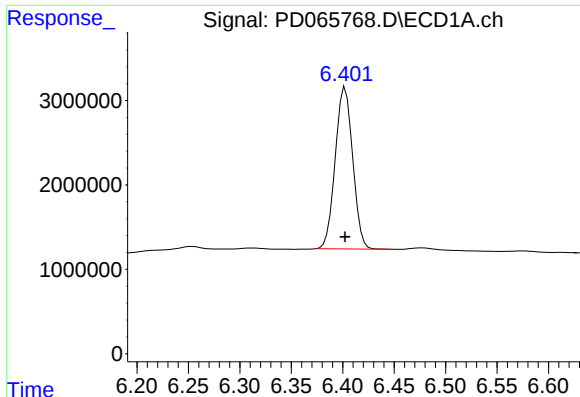

#17 4,4'-DDT


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 22630556
Conc: 19.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

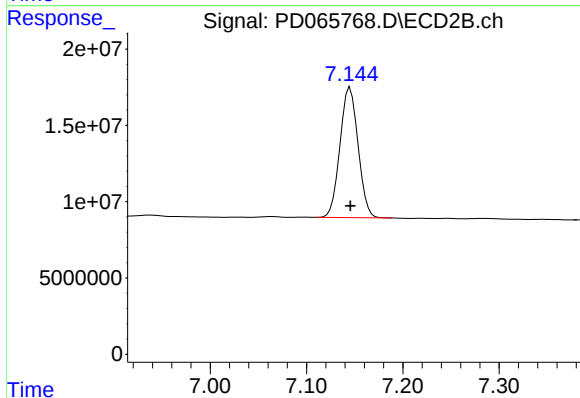


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 111201160
Conc: 20.22 ng/ml

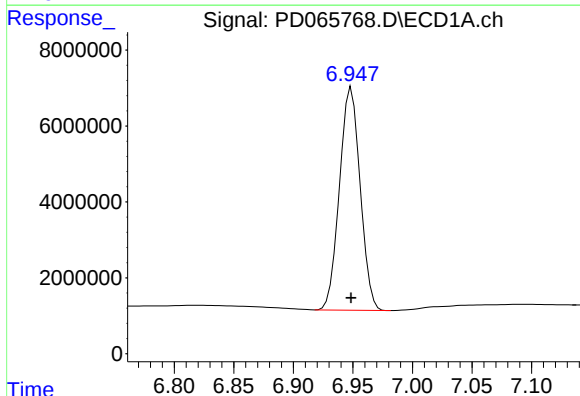


#20 Methoxychlor

R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 70955045
Conc: 102.47 ng/ml

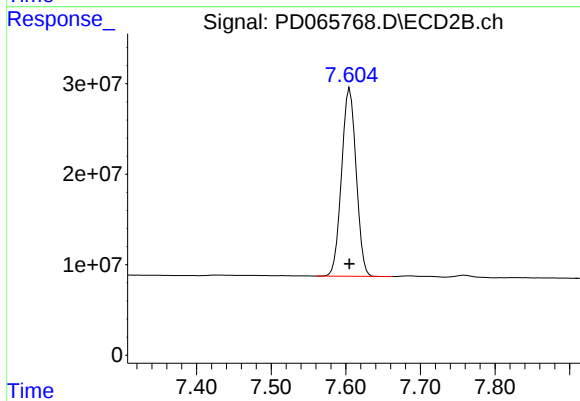

#20 Methoxychlor


R.T.: 7.605 min
Delta R.T.: 0.000 min
Response: 282085628
Conc: 107.85 ng/ml

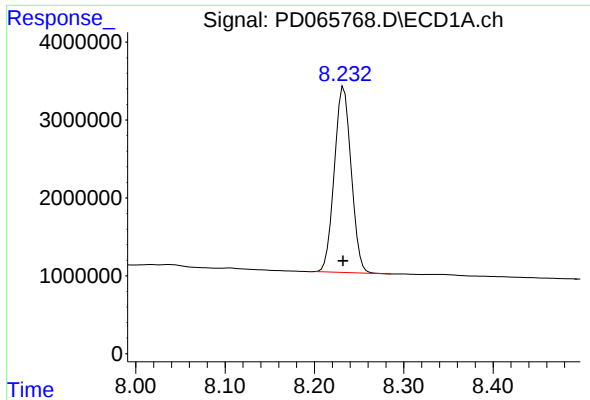

#27 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 31228684
Conc: 21.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

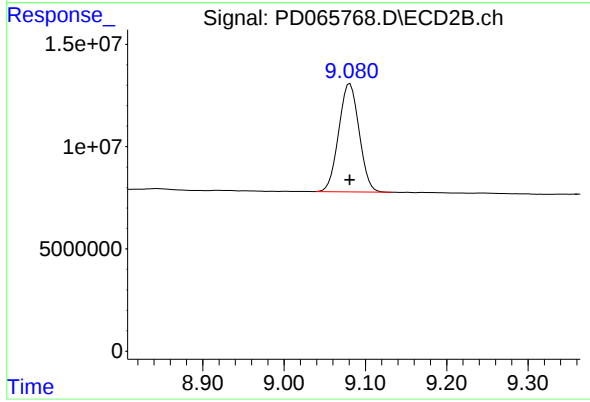

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 92216672
Conc: 20.94 ng/ml