

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 13:05
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3088

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 14:58:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 20 14:57:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	4.011	17300606	143.8E6	20.000	20.000
27)	SA Decachlor...	8.232	9.081	58738313	176.2E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.931	4.406	23473712	192.5E6	20.000	20.000
3)	MA gamma-BHC...	4.214	4.692	24127430	184.0E6	20.000	20.000
4)	MA Heptachlor	4.512	5.196	25397303	169.2E6	20.000	20.000
9)	A Endosulfan I	5.540	6.248	23707368	131.9E6	20.000	20.000
13)	MA Dieldrin	5.783	6.506	51174315	275.6E6	40.000	40.000
14)	MA Endrin	6.041	6.725	48003988	206.8E6	40.000	40.000
16)	A 4,4'-DDD	6.163	6.848	42624129	222.5E6	40.000	40.000
17)	MA 4,4'-DDT	6.402	7.146	46192857	220.0E6	40.000	40.000
20)	A Methoxychlor	6.948	7.605	138.5E6	523.1E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 13:05
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 14:58:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 20 14:57:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

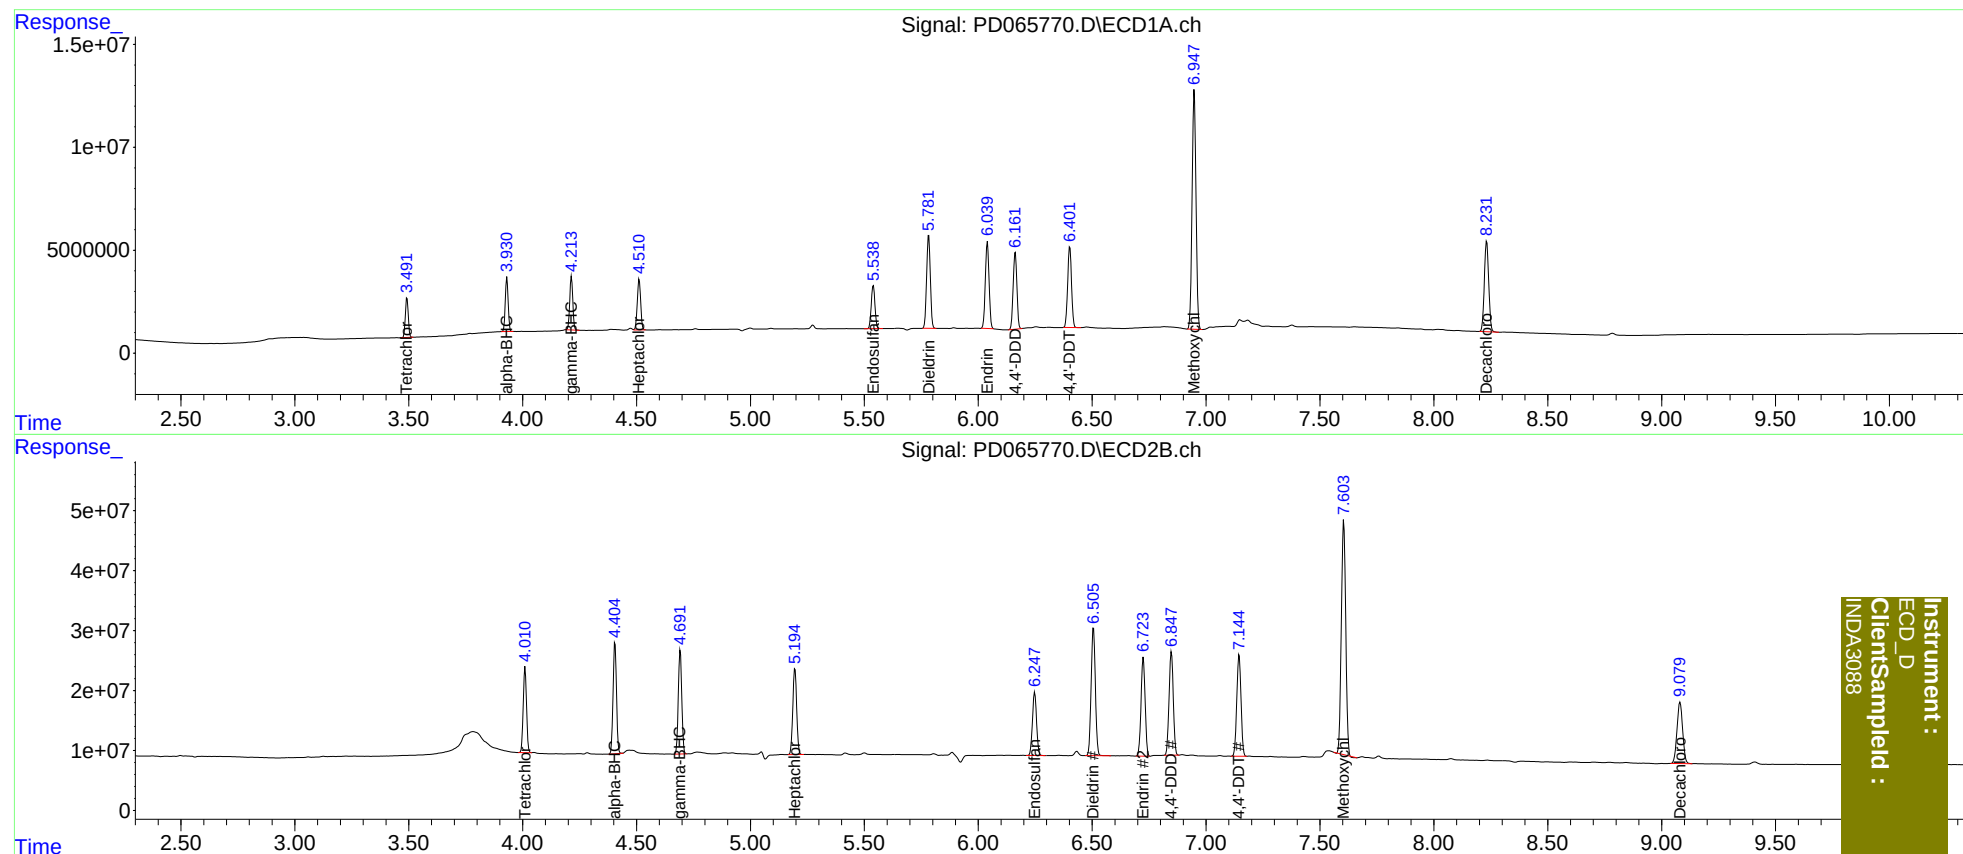


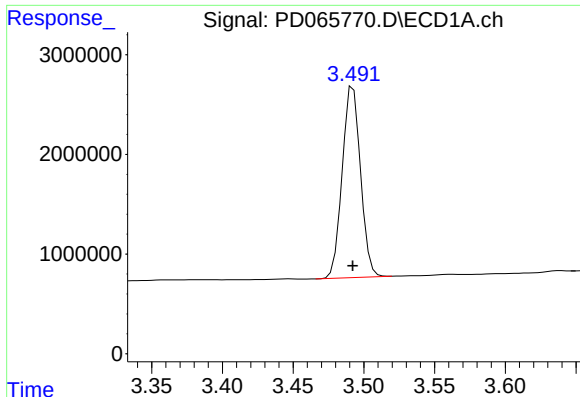

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 17300606
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

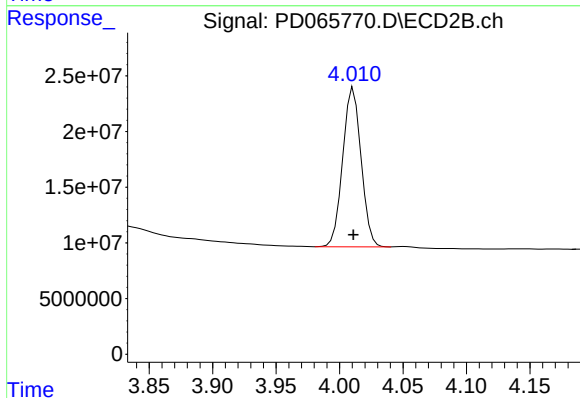


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 143779424
Conc: 20.00 ng/ml

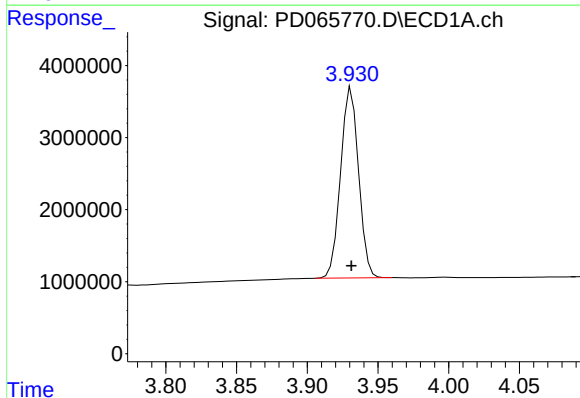


#2 alpha-BHC

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 23473712
Conc: 20.00 ng/ml

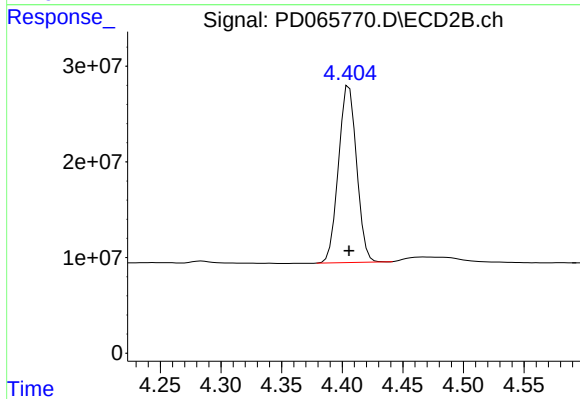

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 192534833
Conc: 20.00 ng/ml

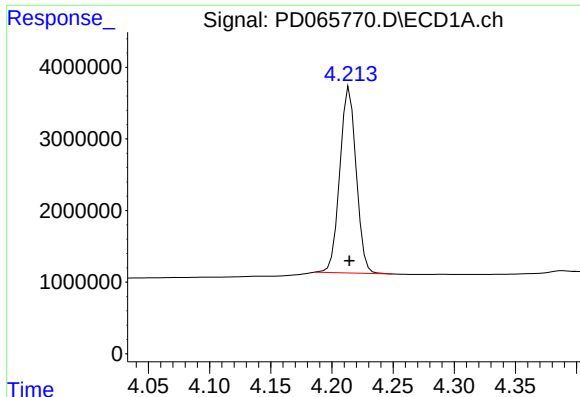

#3 gamma-BHC (Lindane)


R.T.: 4.214 min
Delta R.T.: 0.000 min
Response: 24127430
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

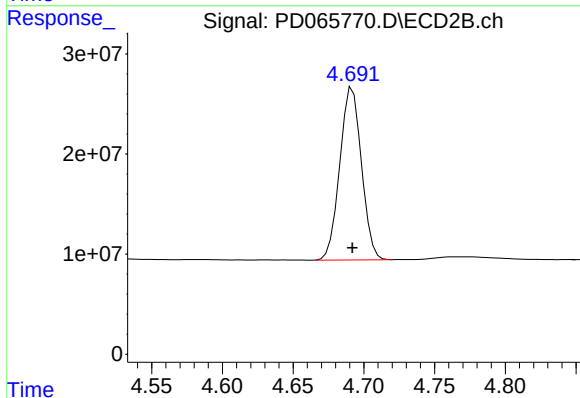


#3 gamma-BHC (Lindane)

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 184005384
Conc: 20.00 ng/ml

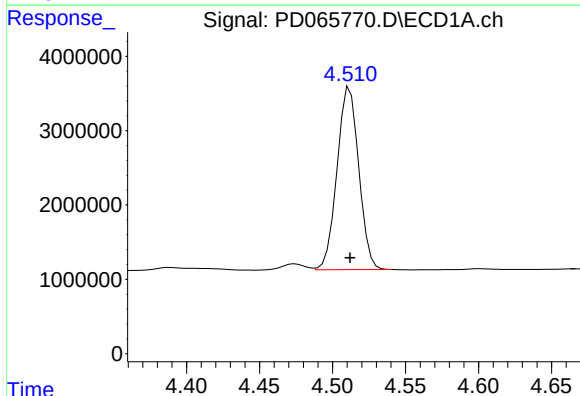


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 25397303
Conc: 20.00 ng/ml

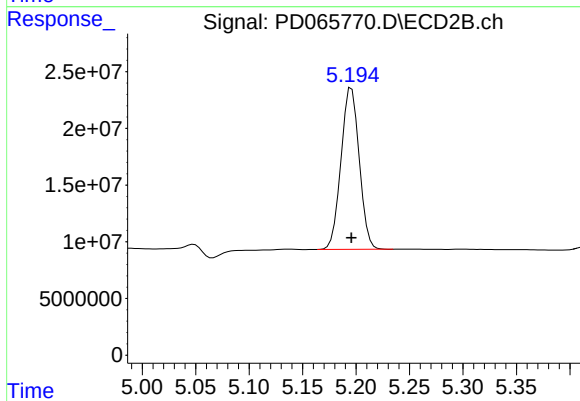

#4 Heptachlor


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 169227603
Conc: 20.00 ng/ml

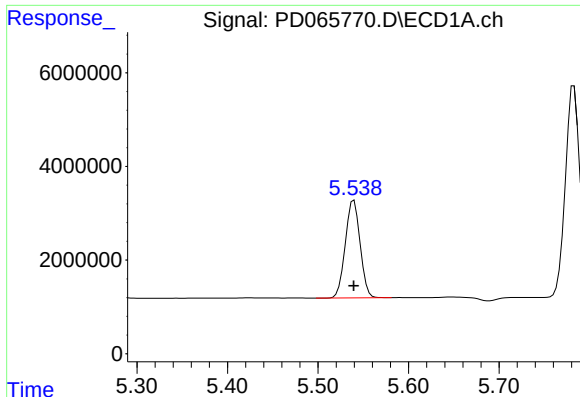

#9 Endosulfan I


R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 23707368
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

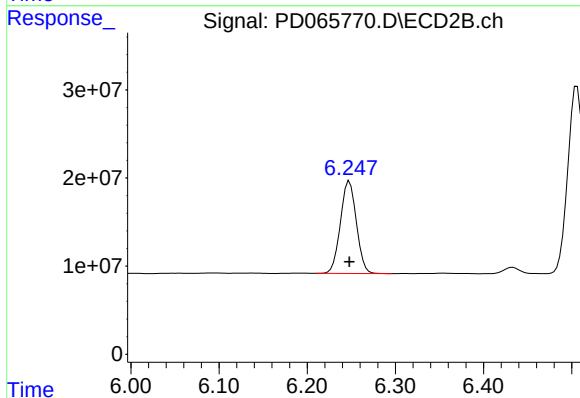


#9 Endosulfan I

R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 131909265
Conc: 20.00 ng/ml

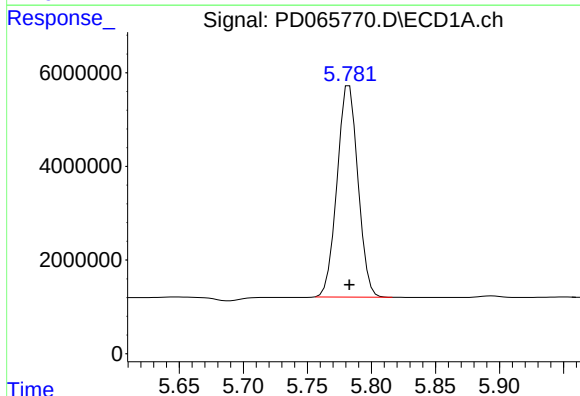


#13 Dieldrin

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 51174315
Conc: 40.00 ng/ml

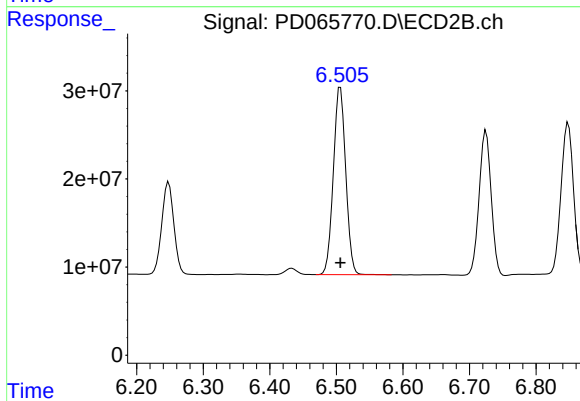

#13 Dieldrin


R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 275597422
Conc: 40.00 ng/ml

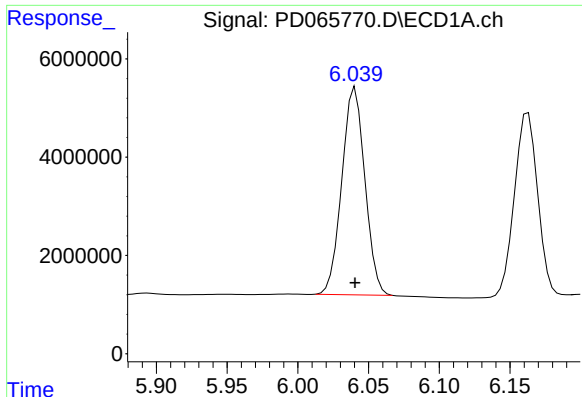

#14 Endrin


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 48003988
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

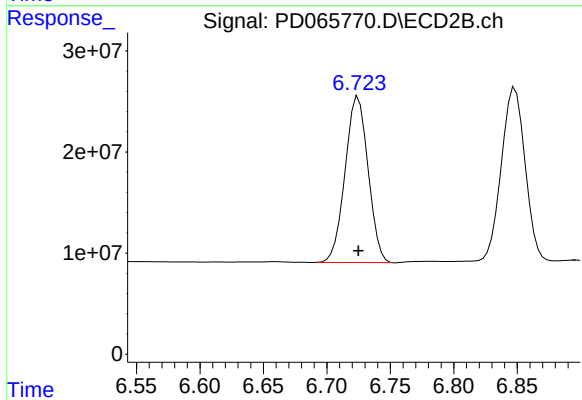


#14 Endrin

R.T.: 6.725 min
Delta R.T.: 0.000 min
Response: 206786693
Conc: 40.00 ng/ml

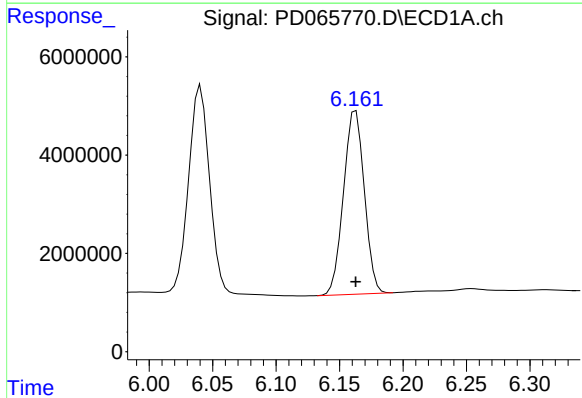


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 42624129
Conc: 40.00 ng/ml

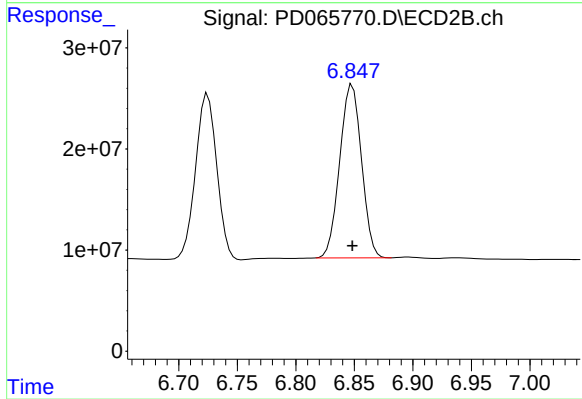

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 222515710
Conc: 40.00 ng/ml

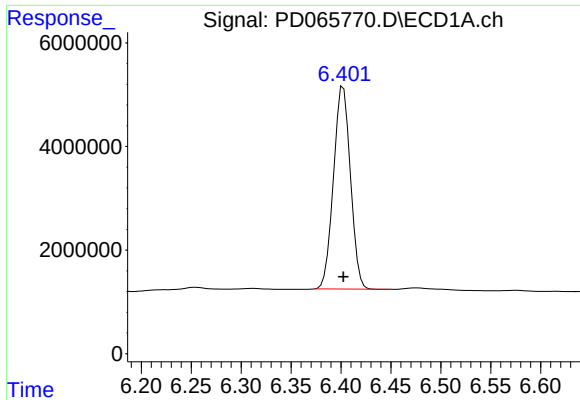

#17 4,4'-DDT


R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 46192857
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

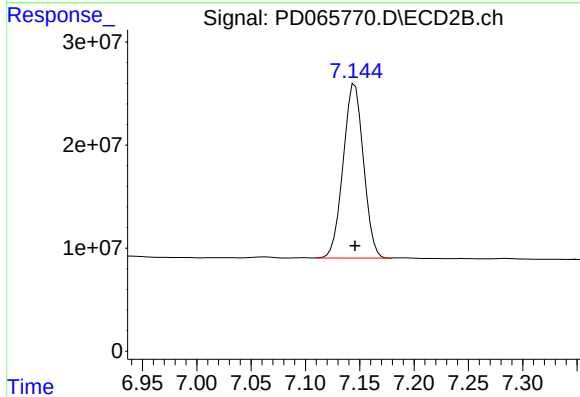


#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 219959489
Conc: 40.00 ng/ml

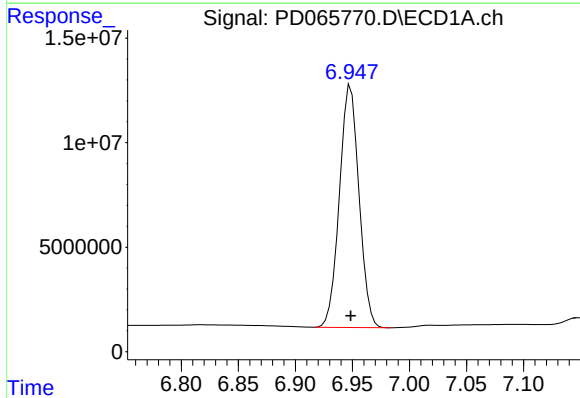


#20 Methoxychlor

R.T.: 6.948 min
Delta R.T.: 0.000 min
Response: 138489493
Conc: 200.00 ng/ml

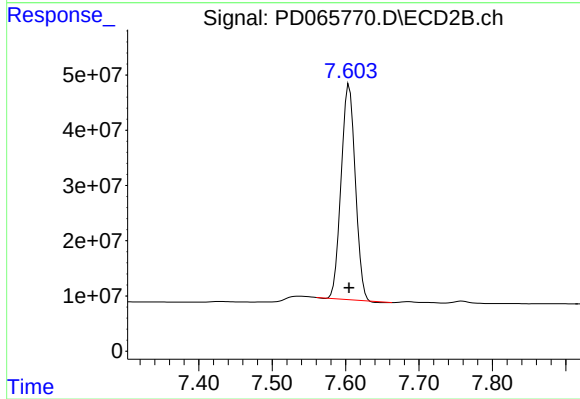

#20 Methoxychlor


R.T.: 7.605 min
Delta R.T.: 0.000 min
Response: 523114305
Conc: 200.00 ng/ml

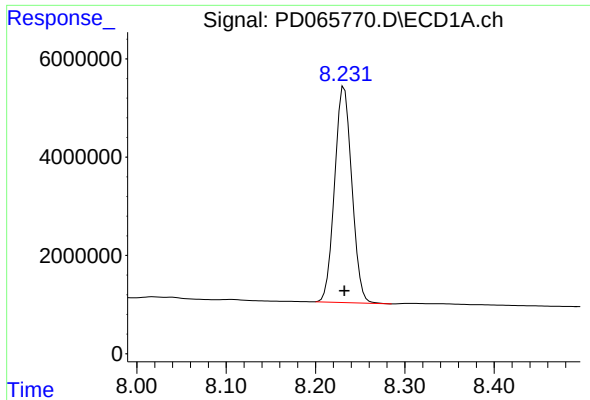

#27 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: 0.000 min
Response: 58738313
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3088

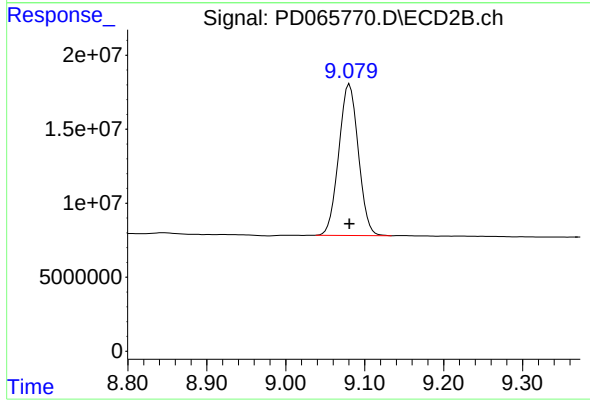

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 176159101
Conc: 40.00 ng/ml