

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 13:33
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4090

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 14:58:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 20 14:57:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	33602095	270.2E6	38.845	37.581
27)	SA Decachlor...	8.233	9.082	109.2E6	323.8E6	74.335	73.522
Target Compounds							
2)	A alpha-BHC	3.932	4.406	48217335	370.6E6	41.082	38.492
3)	MA gamma-BHC...	4.215	4.693	48080231	351.8E6	39.855	38.235
4)	MA Heptachlor	4.513	5.196	49756414	320.4E6	39.182	37.869
9)	A Endosulfan I	5.541	6.249	46375946	249.1E6	39.124	37.768
13)	MA Dieldrin	5.784	6.507	104.2E6	526.5E6	81.480	76.420
14)	MA Endrin	6.041	6.726	92868760	433.4E6	77.384	83.829
16)	A 4,4'-DDD	6.163	6.849	87001433	427.0E6	81.645	76.764
17)	MA 4,4'-DDT	6.403	7.146	94337460	423.2E6	81.690	76.958
20)	A Methoxychlor	6.949	7.606	265.5E6	961.5E6	383.387	367.624


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 13:33
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 14:58:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 20 14:57:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

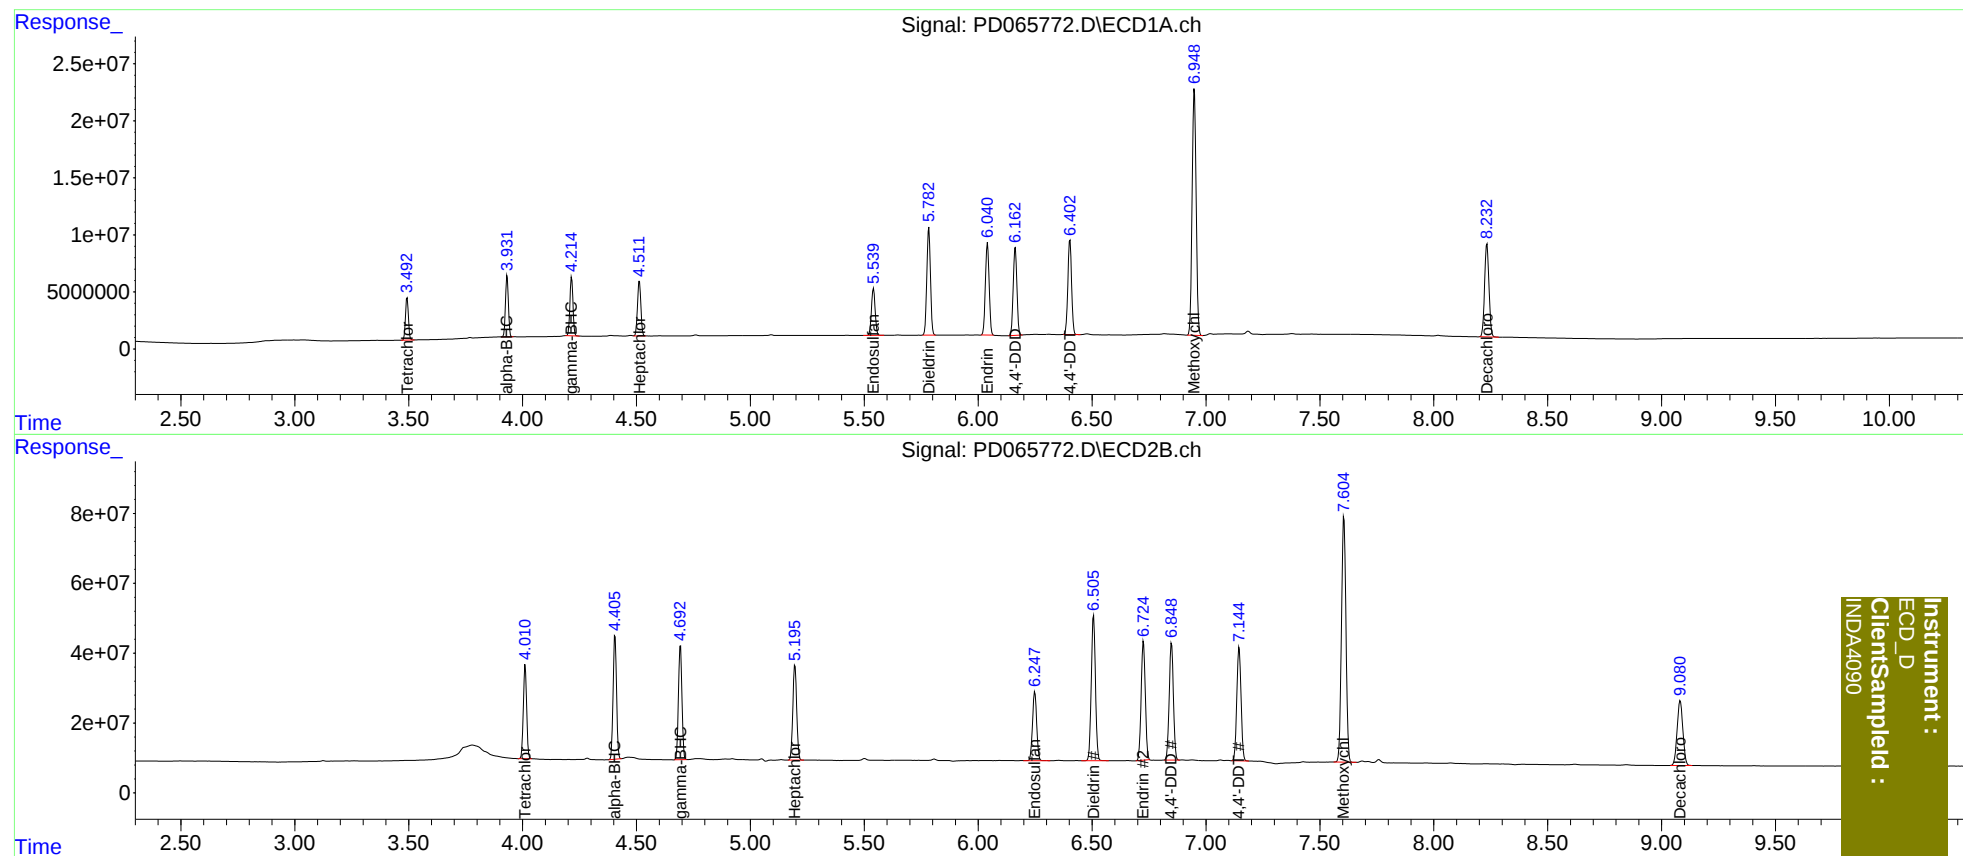


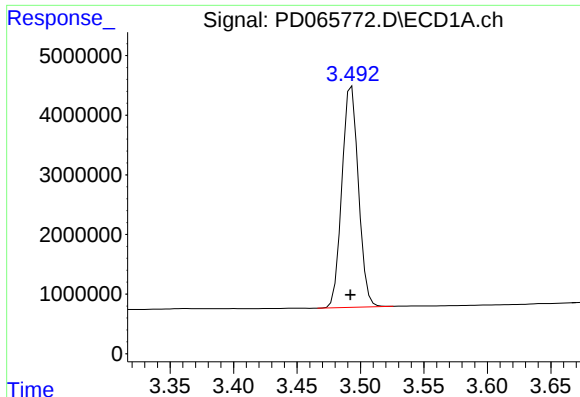

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.001 min
Response: 33602095
Conc: 38.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

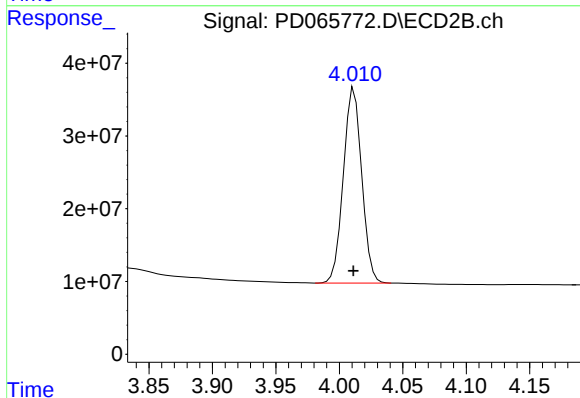


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 270169949
Conc: 37.58 ng/ml

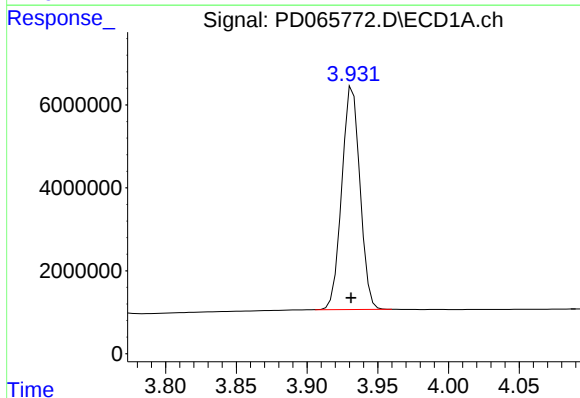


#2 alpha-BHC

R.T.: 3.932 min
Delta R.T.: 0.001 min
Response: 48217335
Conc: 41.08 ng/ml

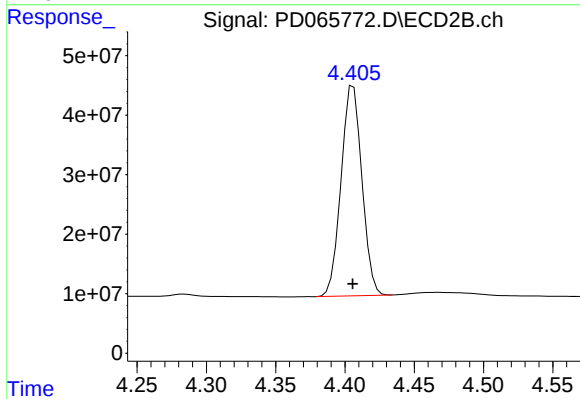

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 370551381
Conc: 38.49 ng/ml

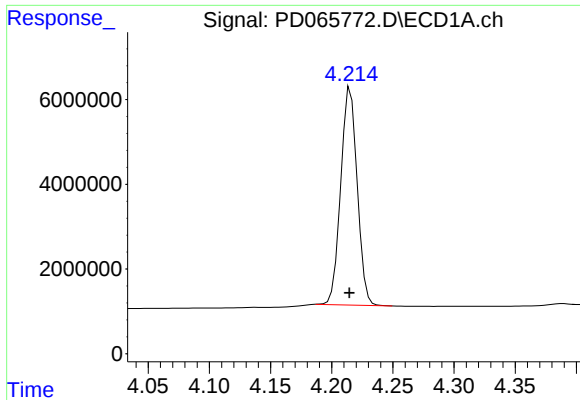

#3 gamma-BHC (Lindane)


R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 48080231
Conc: 39.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

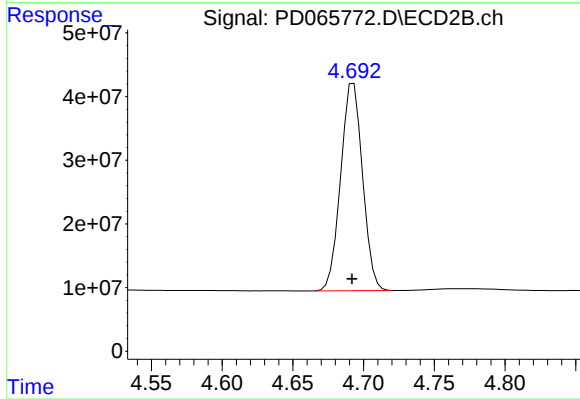


#3 gamma-BHC (Lindane)

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 351775829
Conc: 38.24 ng/ml

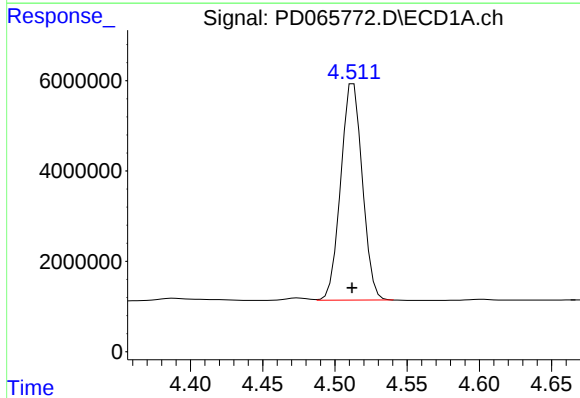


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 49756414
Conc: 39.18 ng/ml

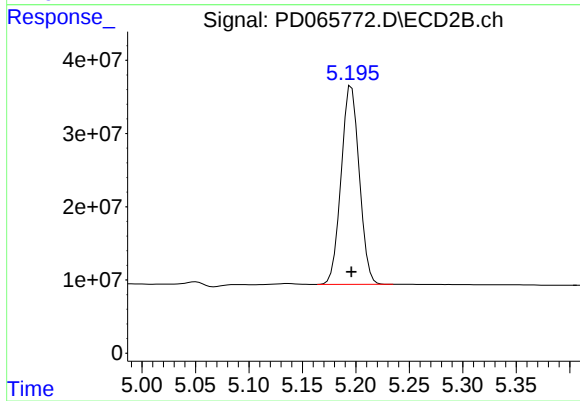

#4 Heptachlor


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 320427464
Conc: 37.87 ng/ml

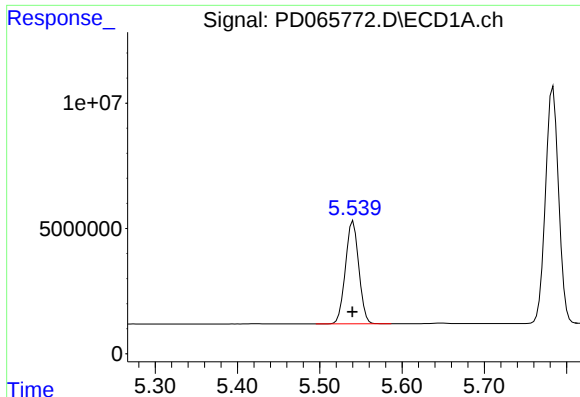

#9 Endosulfan I


R.T.: 5.541 min
Delta R.T.: 0.001 min
Response: 46375946
Conc: 39.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

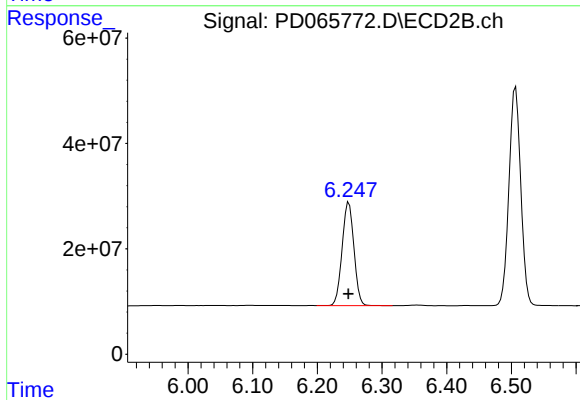


#9 Endosulfan I

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 249097325
Conc: 37.77 ng/ml

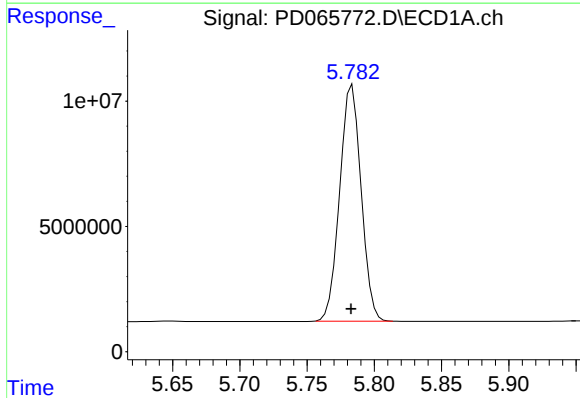


#13 Dieldrin

R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 104241570
Conc: 81.48 ng/ml

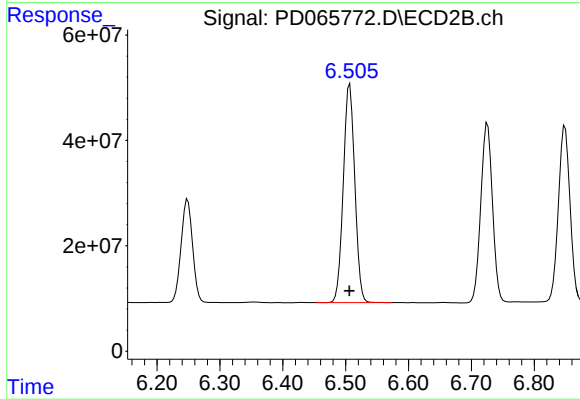

#13 Dieldrin


R.T.: 6.507 min
Delta R.T.: 0.000 min
Response: 526529872
Conc: 76.42 ng/ml

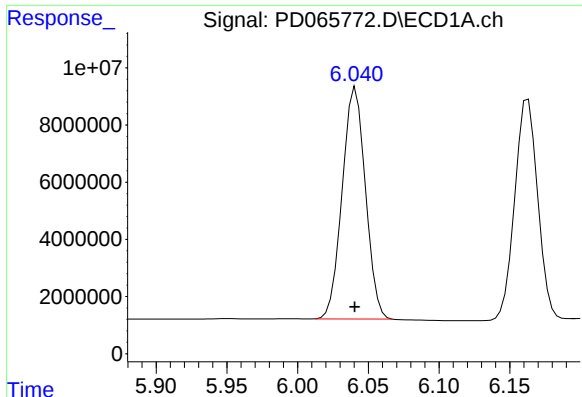

#14 Endrin


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 92868760
Conc: 77.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

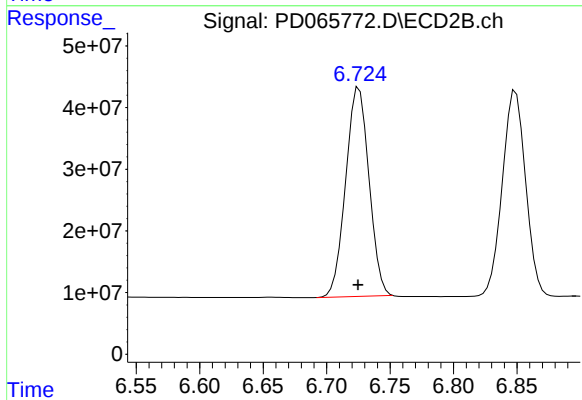


#14 Endrin

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 433369768
Conc: 83.83 ng/ml

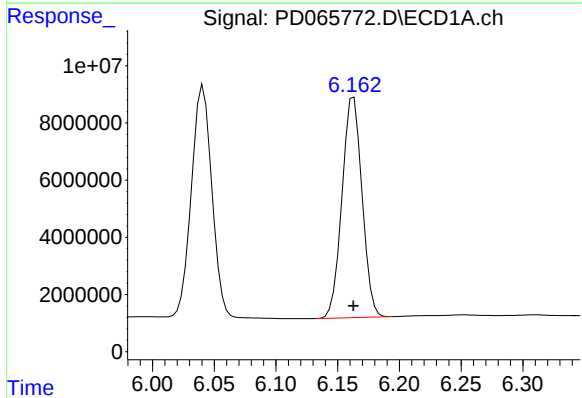


#16 4,4'-DDD

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 87001433
Conc: 81.65 ng/ml

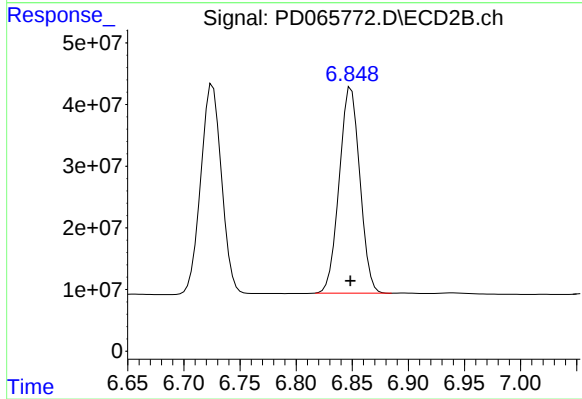

#16 4,4'-DDD


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 427027989
Conc: 76.76 ng/ml

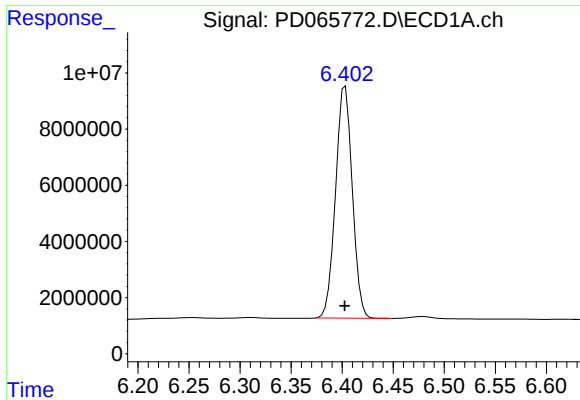

#17 4,4'-DDT


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 94337460
Conc: 81.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

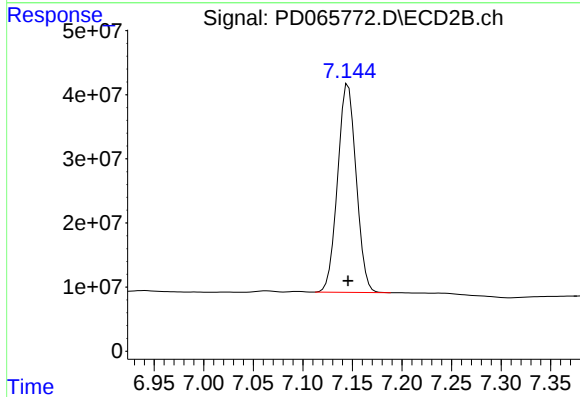


#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 423188707
Conc: 76.96 ng/ml

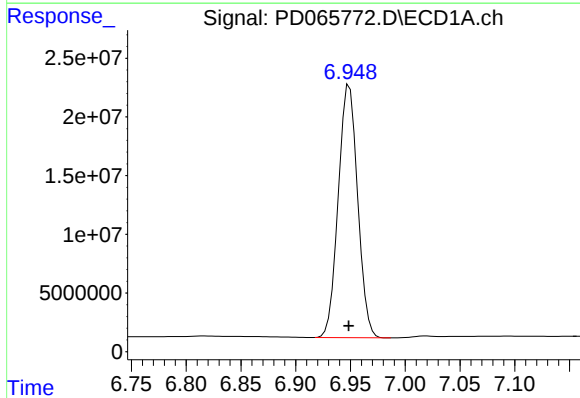


#20 Methoxychlor

R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 265475052
Conc: 383.39 ng/ml

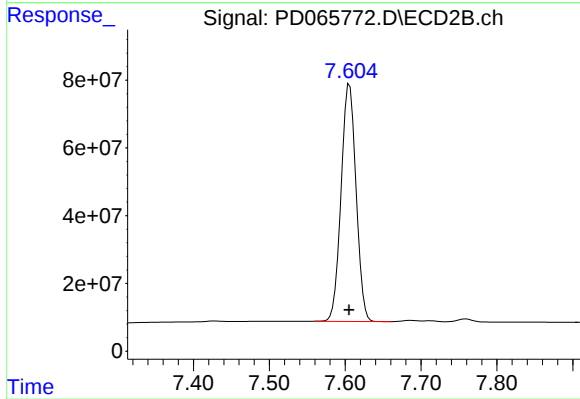

#20 Methoxychlor


R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 961546879
Conc: 367.62 ng/ml

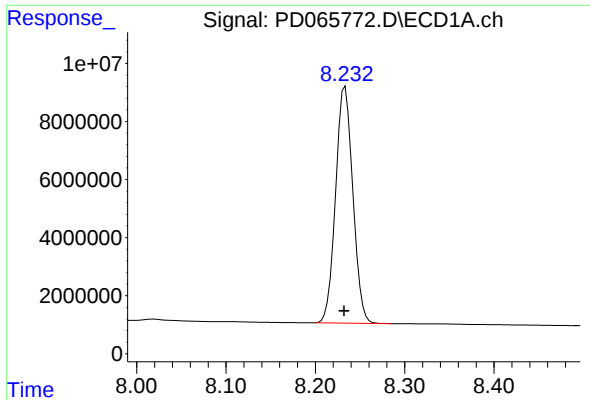

#27 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.001 min
Response: 109158244
Conc: 74.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4090

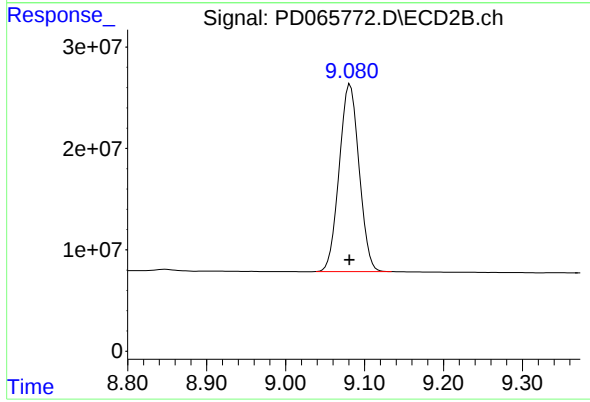

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.001 min
Response: 323788665
Conc: 73.52 ng/ml