

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 14:00
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5092

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 14:58:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 20 14:57:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.011	64936062	498.4E6	75.068	69.324
27)	SA Decachlor...	8.233	9.080	205.4E6	597.7E6	139.857	135.725
Target Compounds							
2)	A alpha-BHC	3.932	4.406	98866155	706.6E6	84.236	73.397
3)	MA gamma-BHC...	4.215	4.692	96790986	658.9E6	80.233	71.619
4)	MA Heptachlor	4.512	5.196	98463587	596.1E6	77.539	70.455
9)	A Endosulfan I	5.540	6.248	91321402	466.8E6	77.041	70.782
13)	MA Dieldrin	5.783	6.506	211.8E6	992.5E6	165.560	144.049
14)	MA Endrin	6.041	6.725	185.7E6	805.4E6	154.748	155.794
16)	A 4,4'-DDD	6.162	6.848	176.4E6	805.5E6	165.506	144.804
17)	MA 4,4'-DDT	6.402	7.145	190.4E6	798.6E6	164.886	145.222
20)	A Methoxychlor	6.948	7.604	506.1E6	1760.6E6	730.829	673.132


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 14:00
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 14:58:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 20 14:57:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

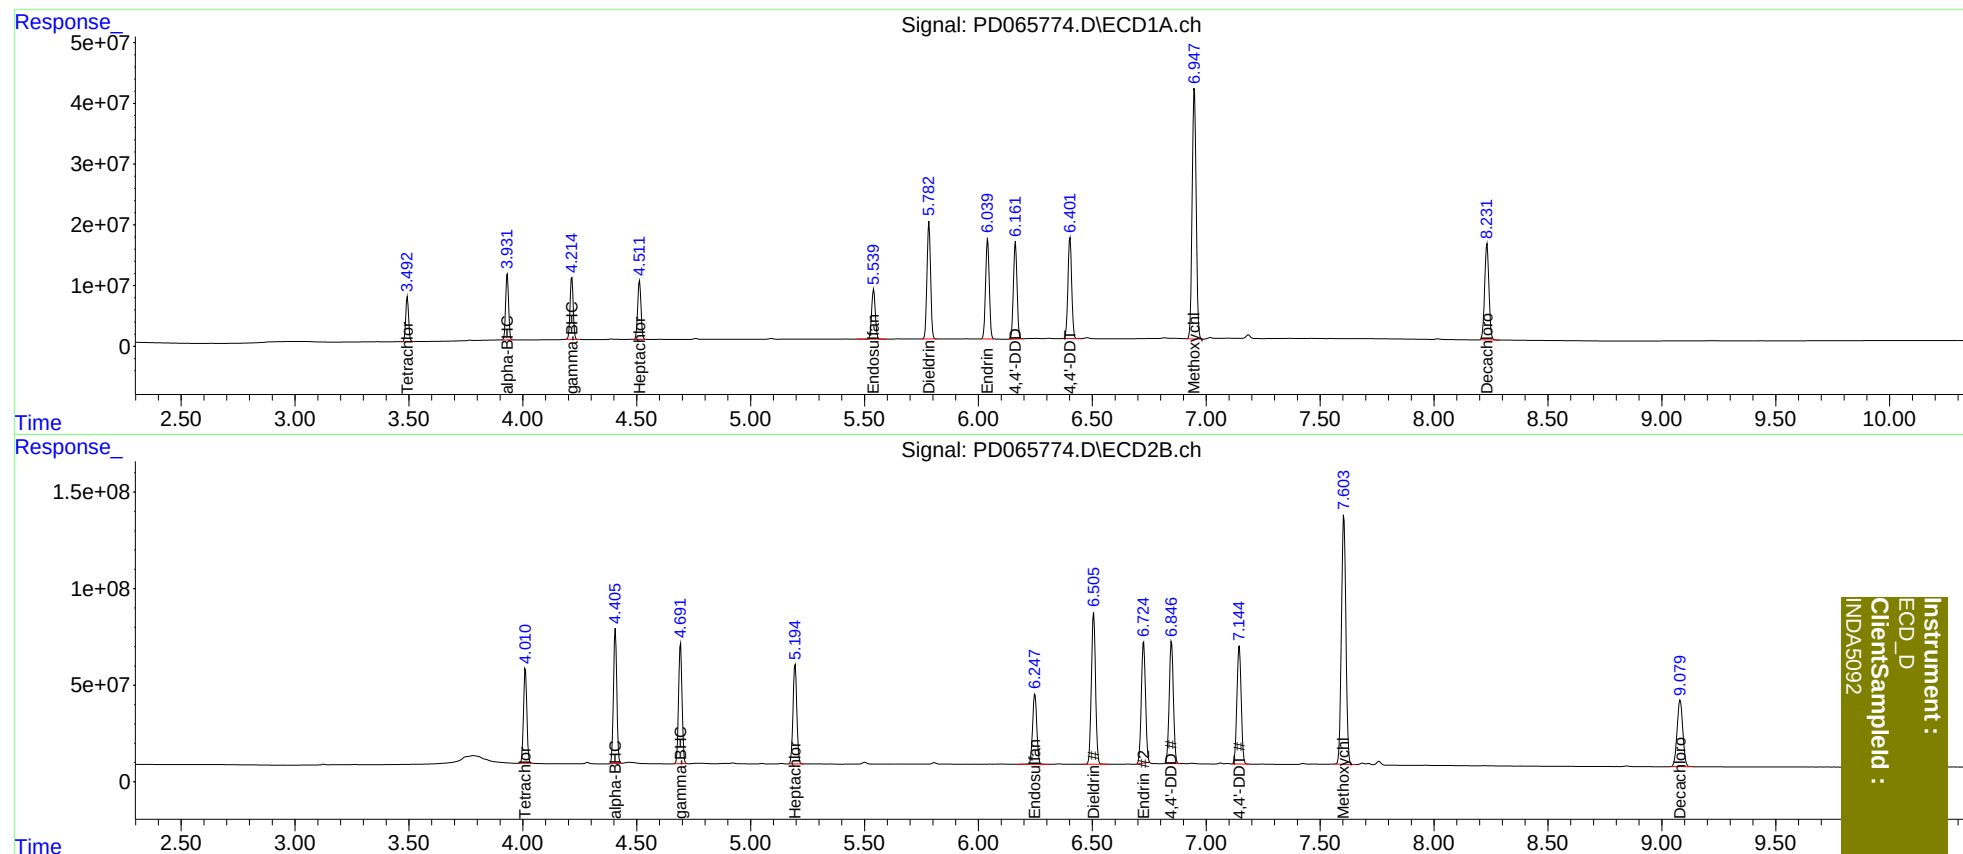


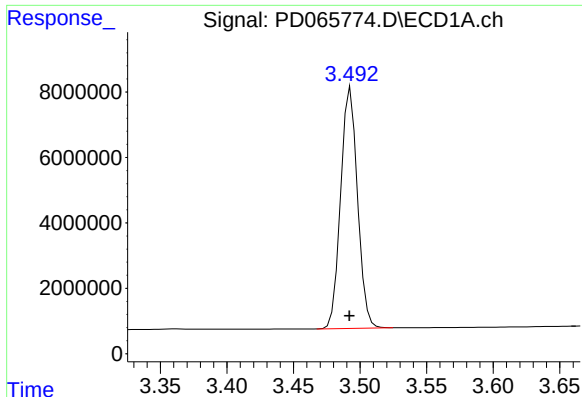

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 64936062
Conc: 75.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

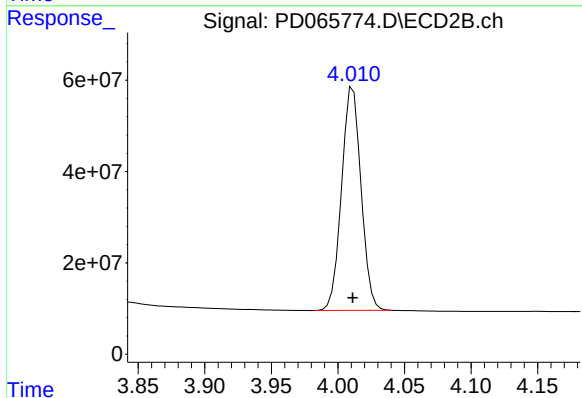


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 498364654
Conc: 69.32 ng/ml

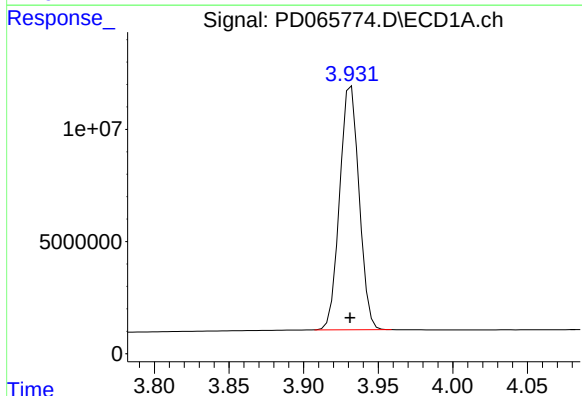


#2 alpha-BHC

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 98866155
Conc: 84.24 ng/ml

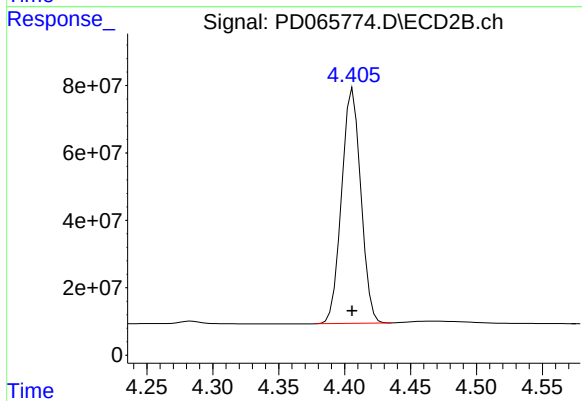

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 706570512
Conc: 73.40 ng/ml

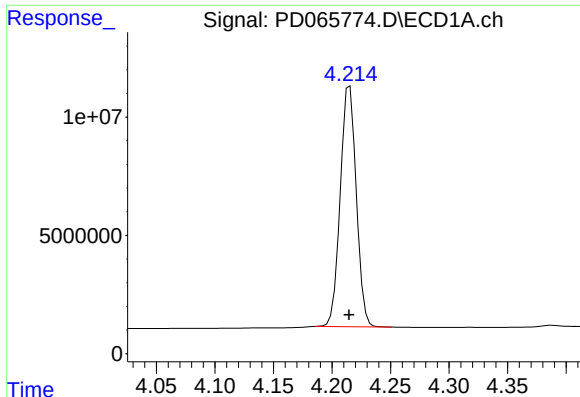

#3 gamma-BHC (Lindane)


R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 96790986
Conc: 80.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

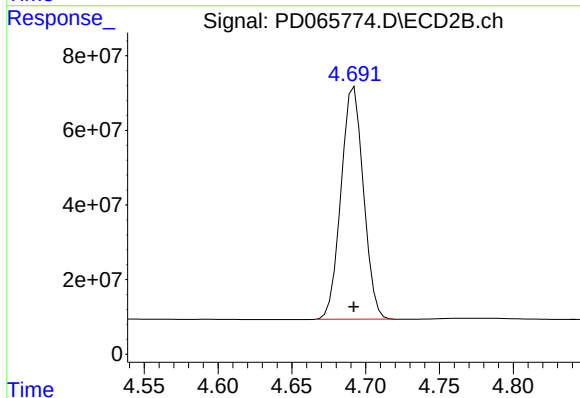


#3 gamma-BHC (Lindane)

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 658915090
Conc: 71.62 ng/ml

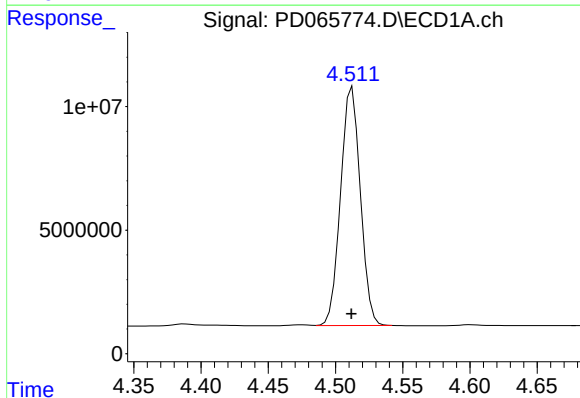


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 98463587
Conc: 77.54 ng/ml

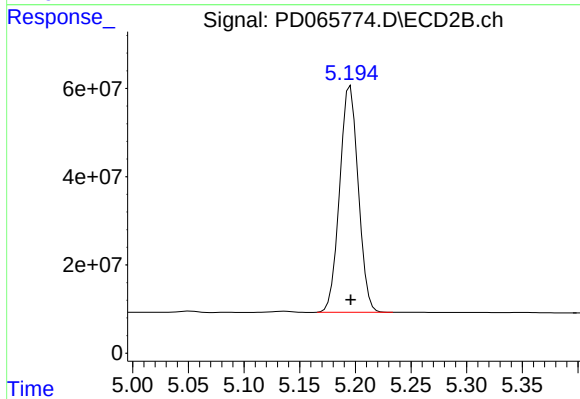

#4 Heptachlor


R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 596144212
Conc: 70.45 ng/ml

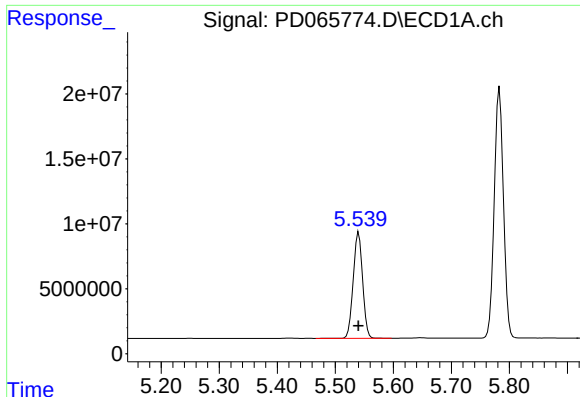

#9 Endosulfan I


R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 91321402
Conc: 77.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

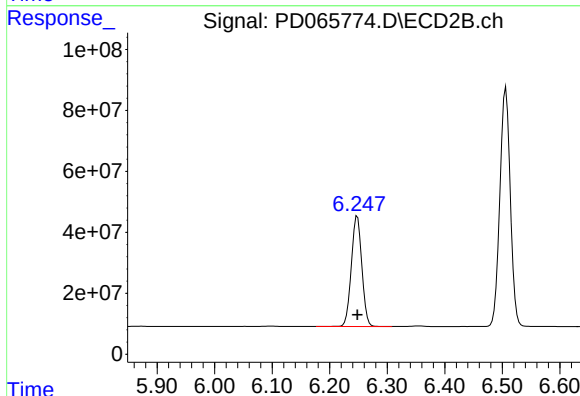


#9 Endosulfan I

R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 466840597
Conc: 70.78 ng/ml

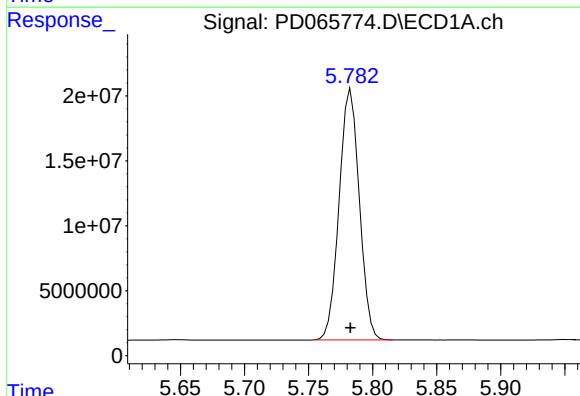


#13 Dieldrin

R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 211810871
Conc: 165.56 ng/ml

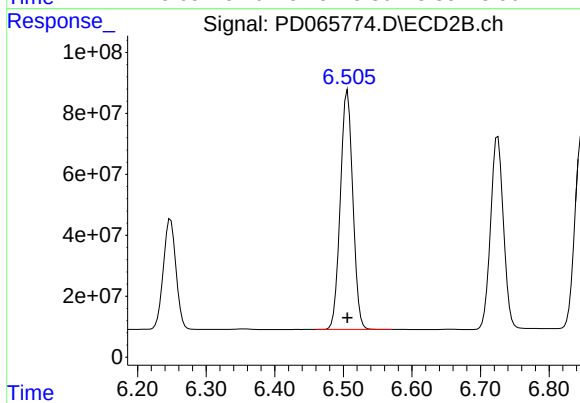

#13 Dieldrin


R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 992485179
Conc: 144.05 ng/ml

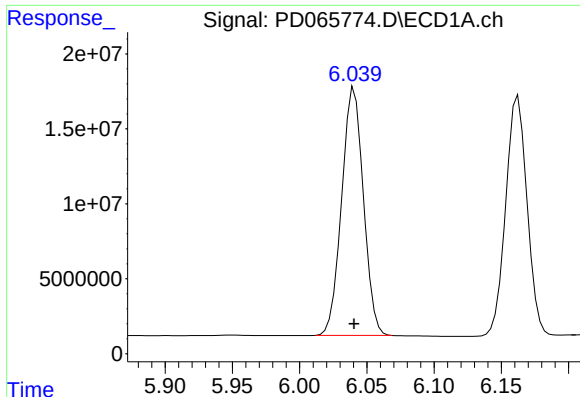

#14 Endrin


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 185712532
Conc: 154.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

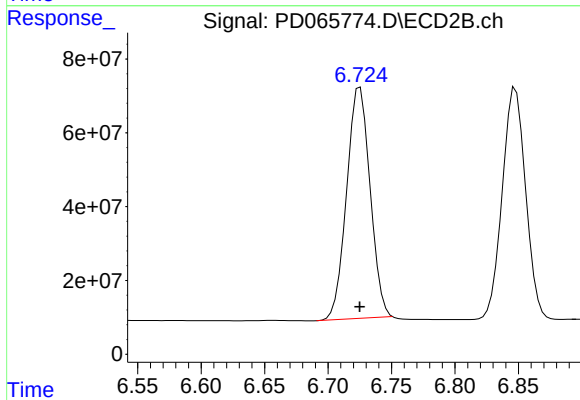


#14 Endrin

R.T.: 6.725 min
Delta R.T.: 0.000 min
Response: 805400977
Conc: 155.79 ng/ml

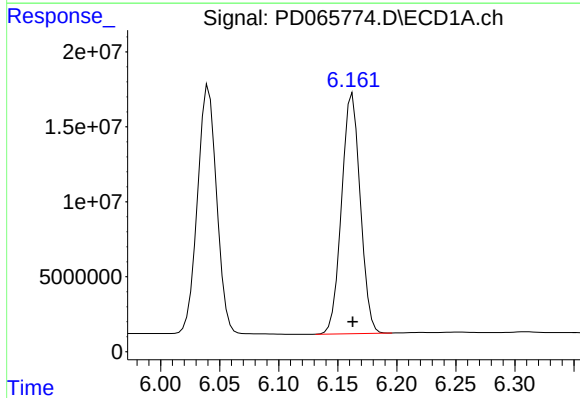


#16 4,4'-DDD

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 176363749
Conc: 165.51 ng/ml

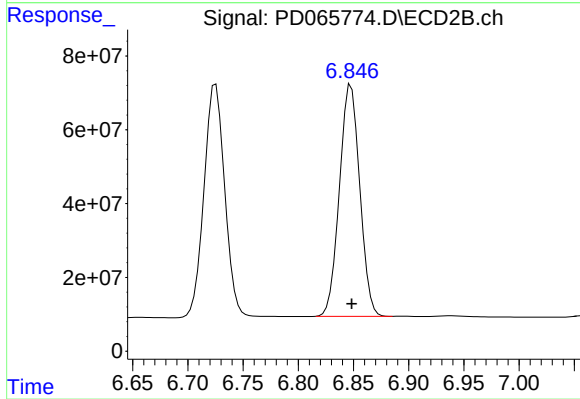

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 805526945
Conc: 144.80 ng/ml

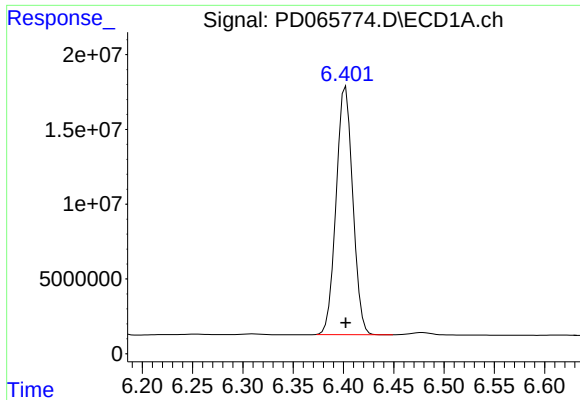

#17 4,4'-DDT


R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 190413858
Conc: 164.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

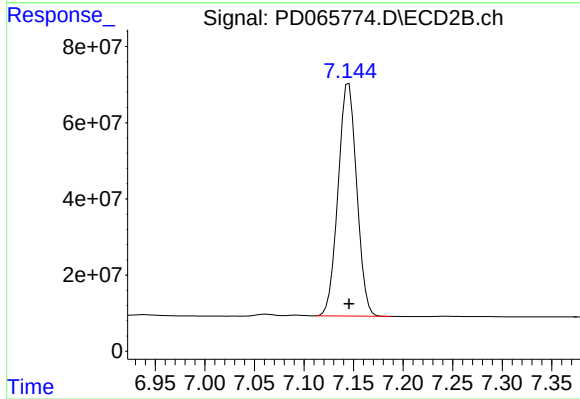


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 798571365
Conc: 145.22 ng/ml

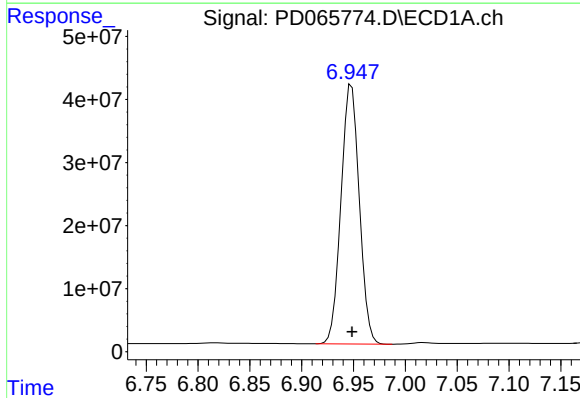


#20 Methoxychlor

R.T.: 6.948 min
Delta R.T.: 0.000 min
Response: 506060714
Conc: 730.83 ng/ml

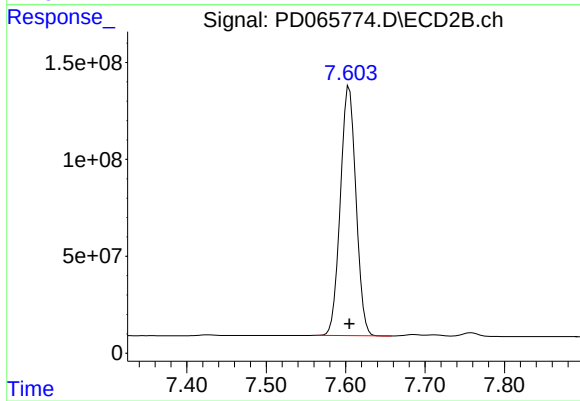

#20 Methoxychlor


R.T.: 7.604 min
Delta R.T.: 0.000 min
Response: 1760625454
Conc: 673.13 ng/ml

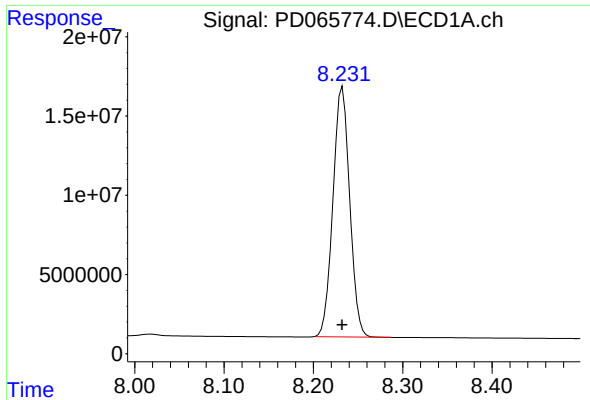

#27 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 205373536
Conc: 139.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5092

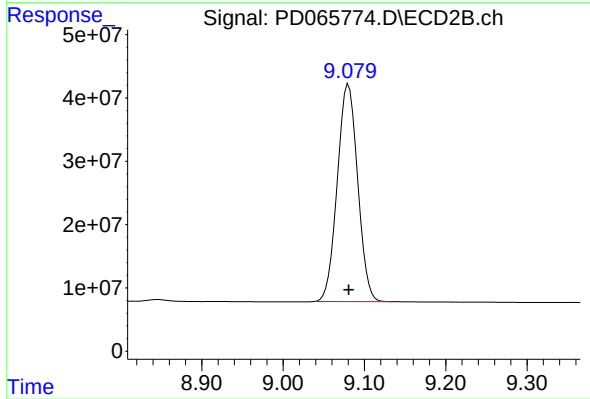

#27 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.000 min
Response: 597729966
Conc: 135.73 ng/ml