

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
 Data File : PD065759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 10:34
 Operator : AR\AJ
 Sample : RESC14
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC009

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 03:51:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	17547203	142.0E6	20.274	19.968
2)	SA Decachlor...	8.232	9.081	57220862	170.5E6	38.697	39.435
Target Compounds							
2)	A alpha-BHC	3.932	4.406	10800181	91752488	9.130	9.651
3)	MA gamma-BHC...	4.215	4.693	11280067	88722388	9.228	9.707
4)	MA Heptachlor	4.512	5.196	12170476	82467669	9.526	9.800
5)	MB Aldrin	4.760	5.501	13758643	91378199	11.069	11.359
6)	B beta-BHC	4.463	4.869	8060229	51126691	12.201	11.365
7)	B delta-BHC	4.667	5.086	13129386	96801218	10.504	10.672
8)	B Heptachlo...	5.202	5.891	13811899	77313914	11.098	11.306
9)	A Endosulfan I	5.540	6.248	11494679	64191767	9.631	9.839
10)	B trans-Chl...	5.426	6.124	14402083	79363044	11.055	11.135
11)	B cis-Chlor...	5.485	6.196	14417304	78436954	11.081	11.229
12)	B 4,4'-DDE	5.648	6.355	25258156	144.0E6	21.190	22.106
13)	MA Dieldrin	5.783	6.506	23777098	131.5E6	18.374	19.261
14)	MA Endrin	6.040	6.725	22064394	108.6E6	18.765	19.457
15)	B Endosulfa...	6.313	6.938	27400277	132.9E6	21.946	22.321
16)	A 4,4'-DDD	6.163	6.848	19579352	105.7E6	18.310	19.146
17)	MA 4,4'-DDT	6.402	7.146	21450328	104.2E6	18.496	19.262
18)	B Endrin al...	6.481	7.063	22006634	104.6E6	22.258	22.471
19)	B Endosulfa...	6.692	7.285	28046109	126.4E6	22.054	22.392
20)	A Methoxychlor	6.948	7.605	66112168	256.2E6	96.120	98.114
21)	B Endrin ke...	7.186	7.759	34317286	144.8E6	22.511	22.530

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 10:34
Operator : AR\AJ
Sample : RESC14
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 03:51:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

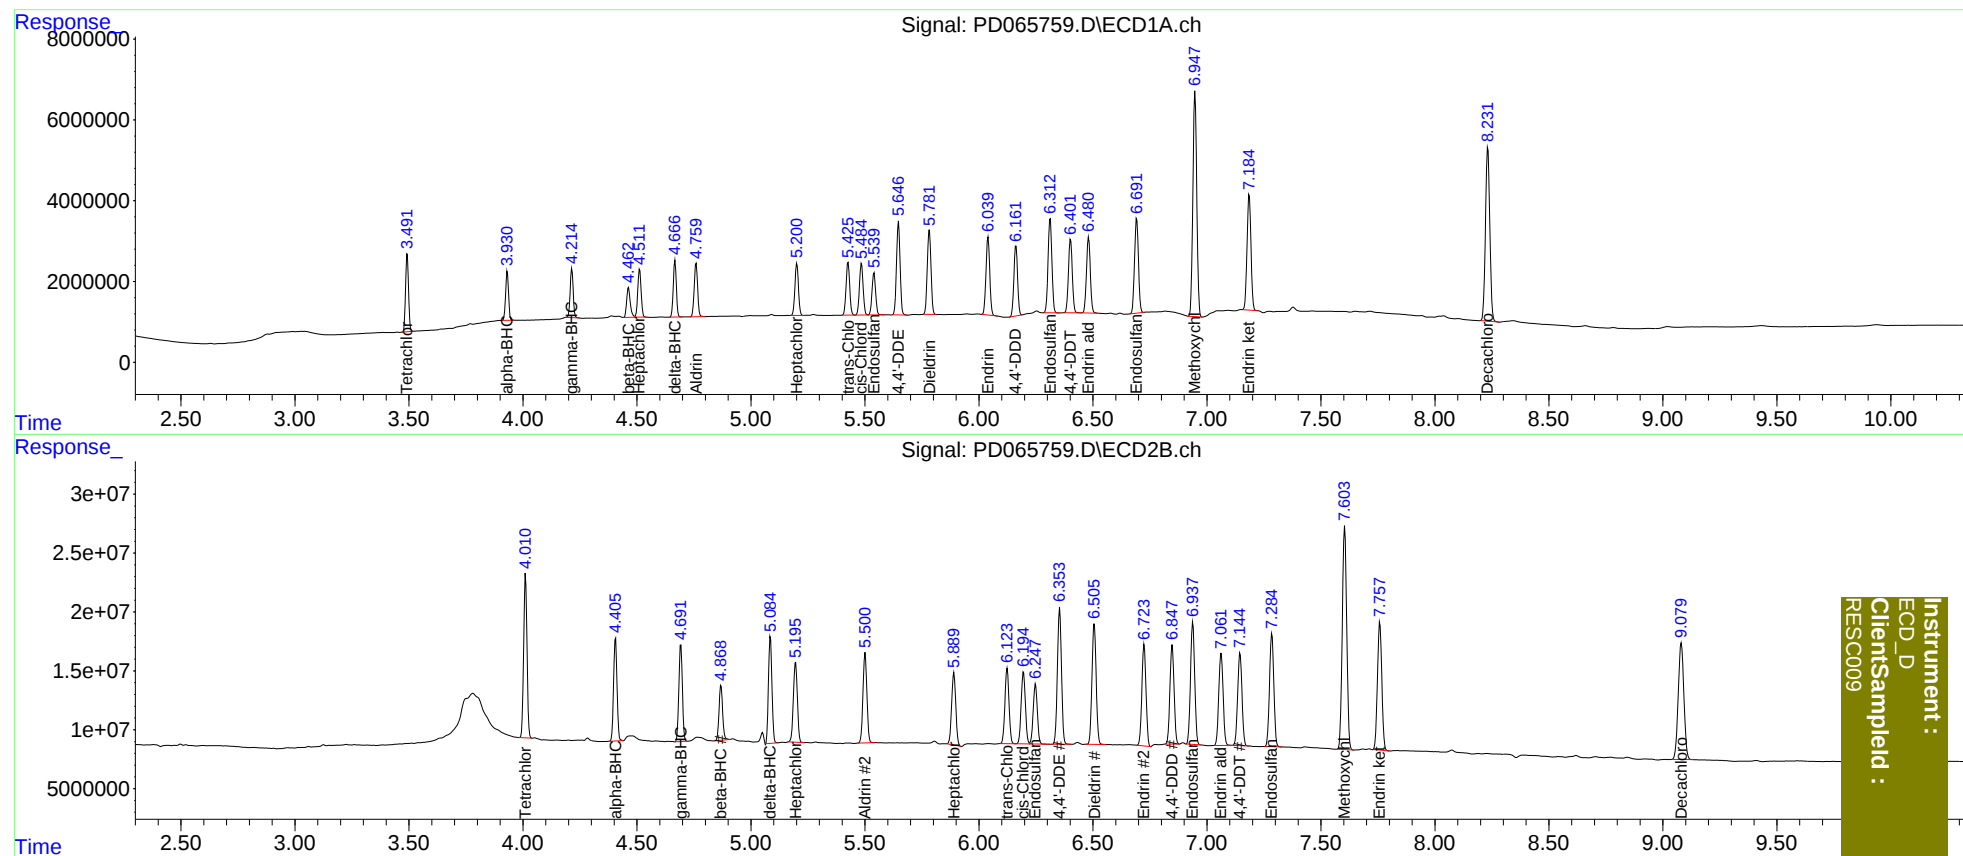

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065759.D
Acq On : 20 Sep 2021 10:34
Operator : AR\AJ
Sample : RESC14
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC009

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Title : GC Extractables
Last Update : Mon Oct 04 09:46:55 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.493	3.932	100.00%
3.932	4.215	100.00%
4.215	4.463	100.00%
4.463	4.512	97.54%
4.512	4.667	100.00%
4.667	4.760	100.00%
4.760	5.202	100.00%
5.202	5.426	100.00%
5.426	5.485	100.00%
5.485	5.540	100.00%
5.540	5.648	100.00%
5.648	5.783	100.00%
5.783	6.040	100.00%
6.040	6.163	100.00%
6.163	6.313	100.00%
6.313	6.402	100.00%
6.402	6.481	100.00%
6.481	6.692	100.00%
6.692	6.948	100.00%
6.948	7.186	100.00%
7.186	8.232	100.00%

Signal #2


4.012	4.406	100.00%
4.406	4.693	100.00%
4.693	4.869	100.00%
4.869	5.086	100.00%
5.086	5.196	100.00%
5.196	5.501	100.00%
5.501	5.891	100.00%
5.891	6.124	100.00%
6.124	6.196	100.00%
6.196	6.248	99.27%
6.248	6.355	100.00%
6.355	6.506	100.00%
6.506	6.725	100.00%
6.725	6.848	100.00%
6.848	6.938	100.00%
6.938	7.063	100.00%
7.063	7.146	100.00%
7.146	7.285	100.00%
7.285	7.605	100.00%
7.605	7.759	100.00%
7.759	9.081	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 10:34
Operator : AR\AJ
Sample : RESC14
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC009

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 03:51:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

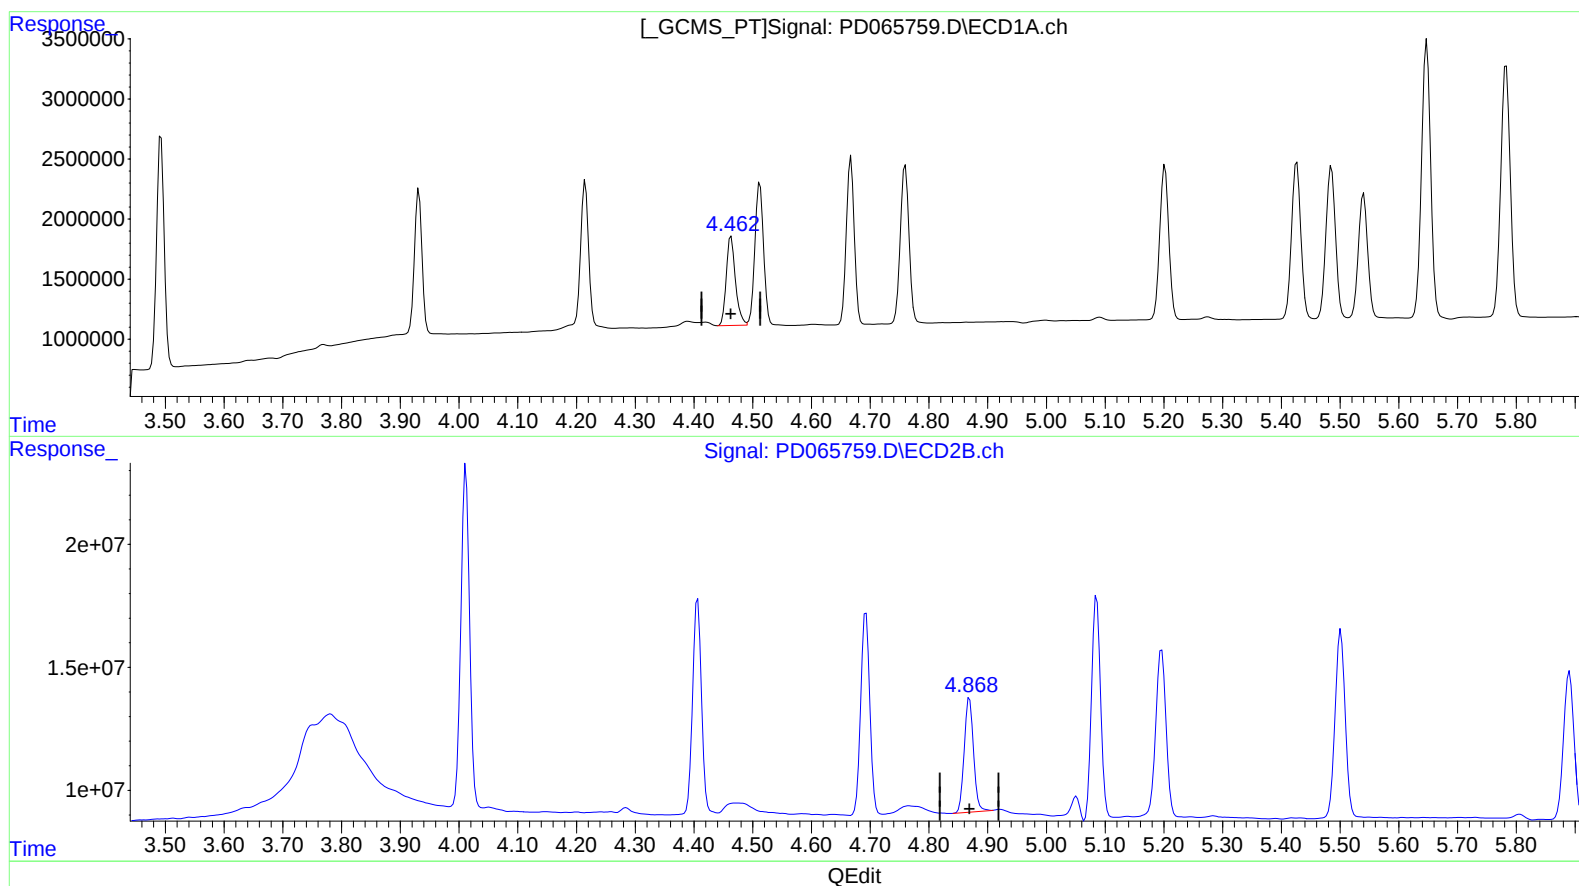

(6) beta-BHC (B)

4.463min 12.201 ng/ml

response 8060229

(6) beta-BHC #2 (B)

4.869min 11.365 ng/ml


response 51126691

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092021\
Data File : PD065759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 10:34
Operator : AR\AJ
Sample : RESC14
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC009

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 03:51:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

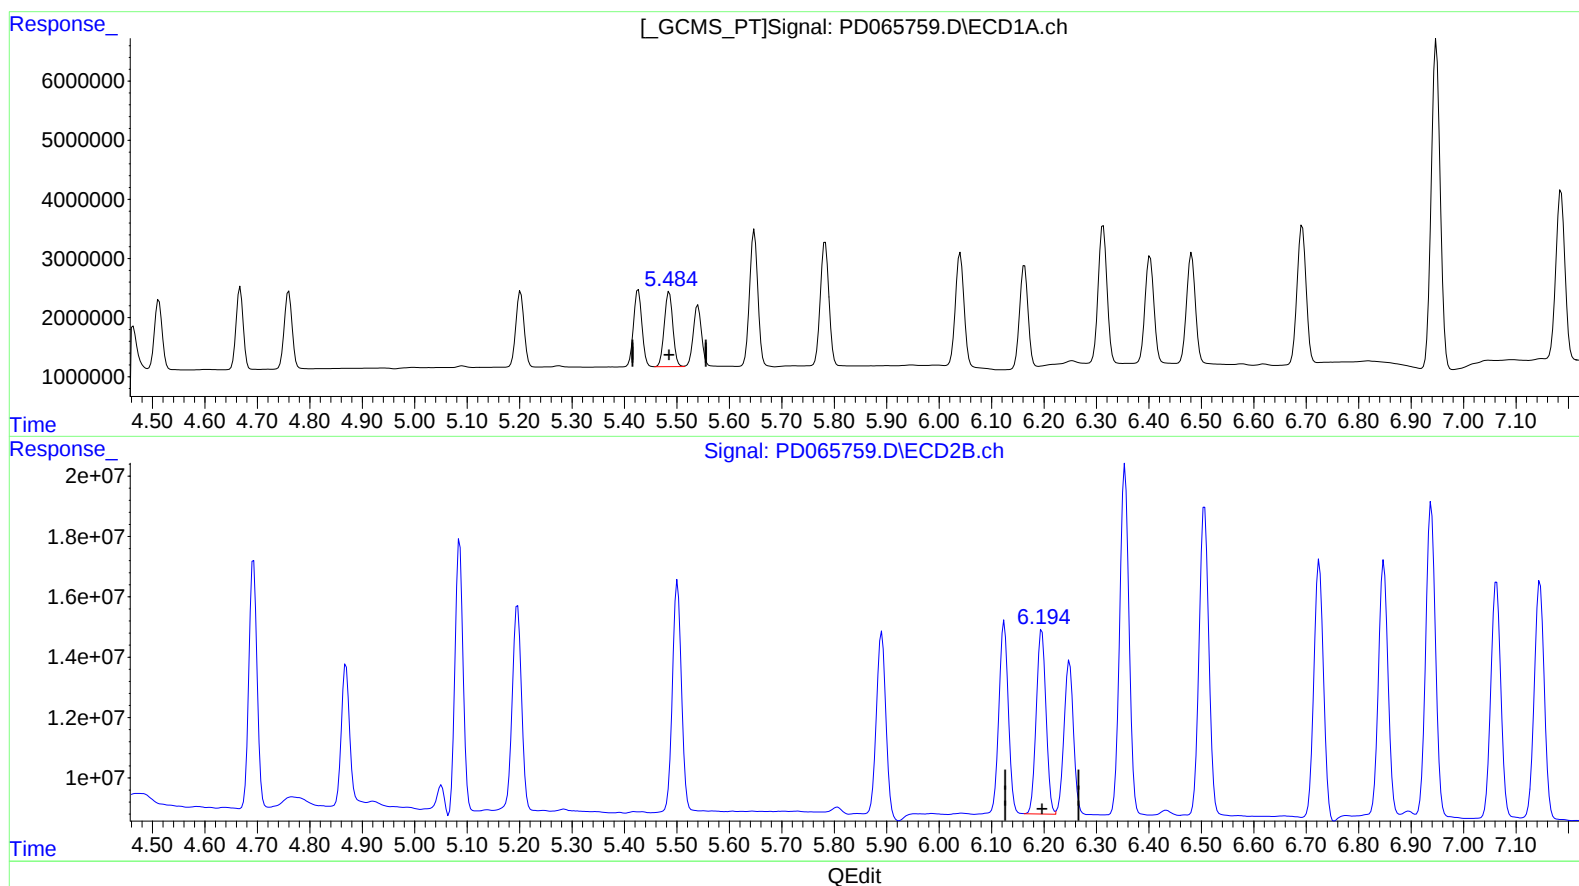

(11) cis-Chlordane (B)

5.485min 11.081 ng/ml

response 14417304

(11) cis-Chlordane #2 (B)

6.196min 11.229 ng/ml

response 78436954