

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092022\
 Data File : PD071949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 11:30
 Operator : AR\AJ
 Sample : N4648-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 N48854-1040

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/20/2022
 Supervised By : Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 23:17:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.813	3.562	29151899	349.1E6	11.922m	12.165m
28) SA Decachlor...	8.001	9.091	29863156	154.2E6	11.854	16.583 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092022\
Data File : PD071949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 11:30
Operator : AR\AJ
Sample : N4648-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
N48854-1040


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/20/2022
Supervised By : Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 23:17:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

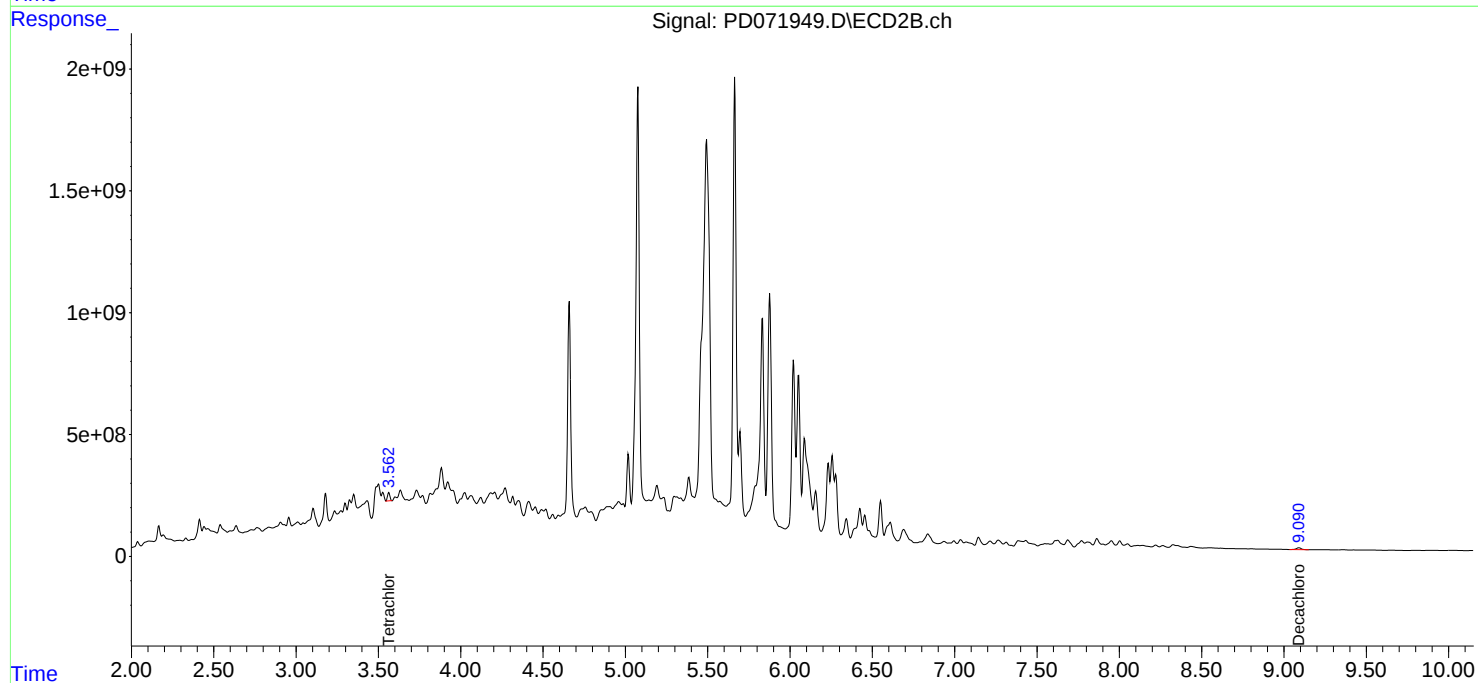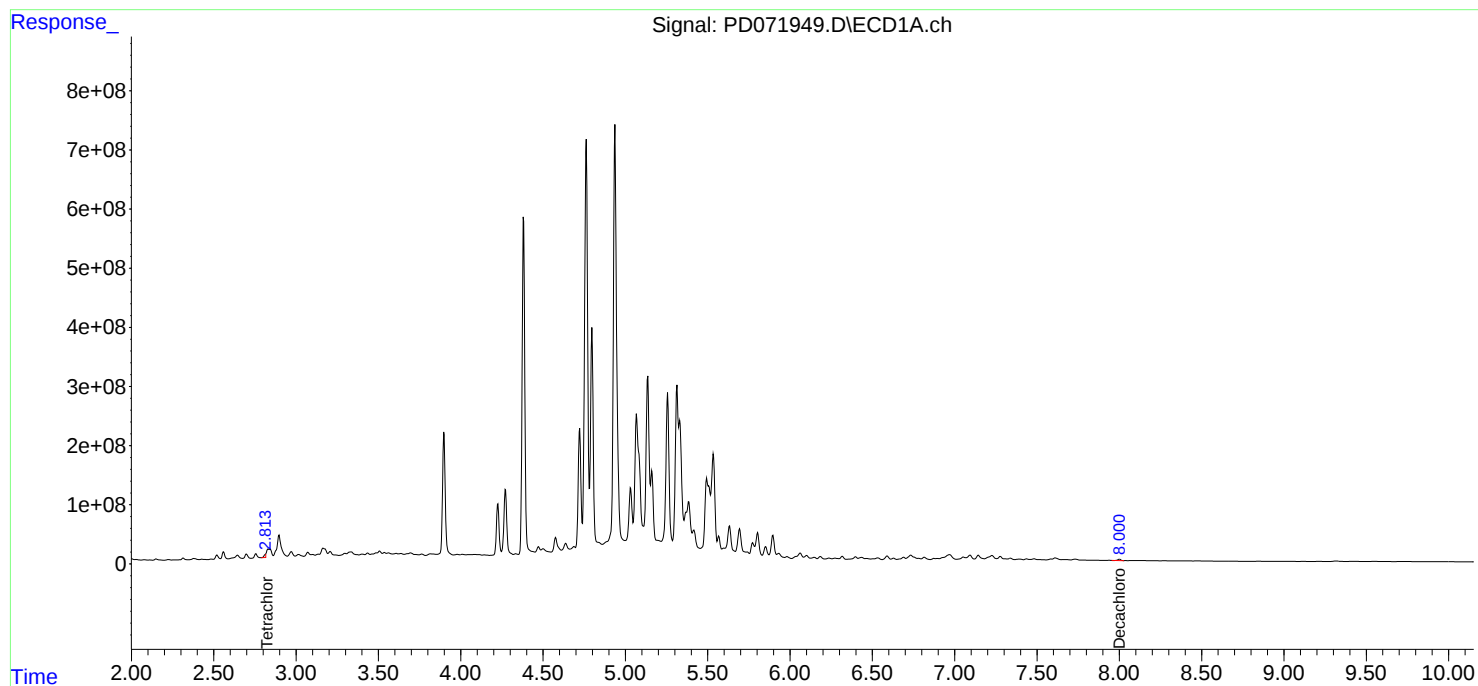

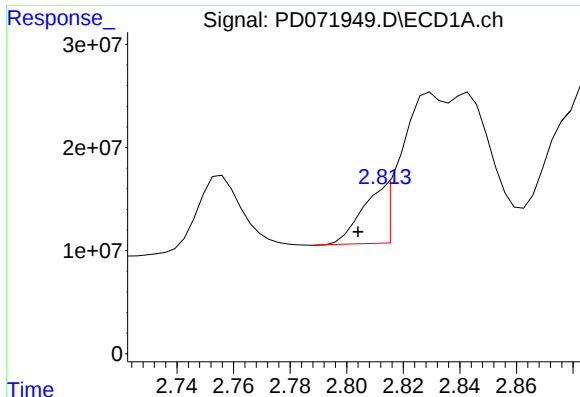


#1 Tetrachloro-m-xylene

R.T.: 2.813 min
Delta R.T.: 0.009 min
Response: 29151899
Conc: 11.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
N48854-1040


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/20/2022
Supervised By :Ankita Jodhani 09/20/2022

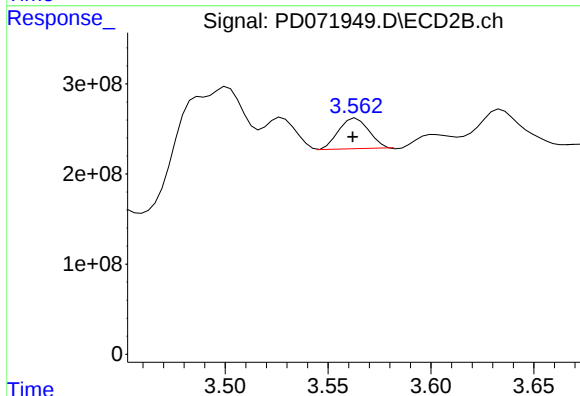


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 349074993
Conc: 12.16 ng/ml m

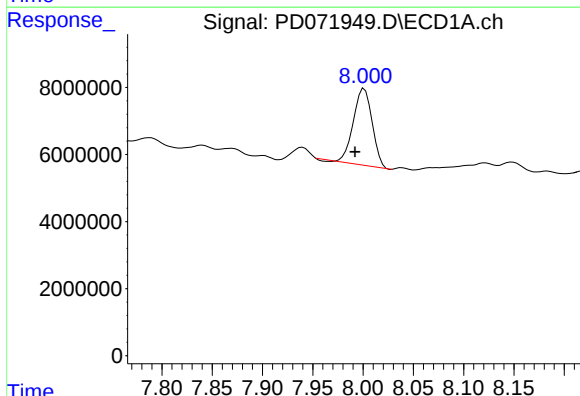

#28 Decachlorobiphenyl

R.T.: 8.001 min
Delta R.T.: 0.009 min
Response: 29863156
Conc: 11.85 ng/ml

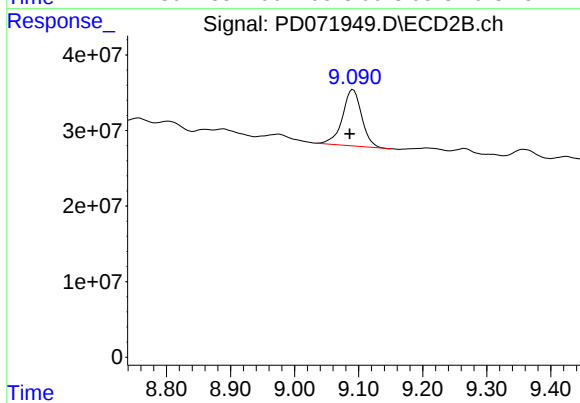

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.005 min
Response: 154173063
Conc: 16.58 ng/ml