

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 12:06
 Operator : AR\AJ
 Sample : PIBLK145
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:30:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	2.893	29340645	86710840	24.229	22.940
27)	SA Decachlor...	8.964	8.088	41990645	76453924	25.597	28.599
Target Compounds							
3)	MA gamma-BHC...	4.218f	0.000	348.5E6	0	139.303	N.D. #
7)	B delta-BHC	4.710	0.000	1162367	0	0.510	N.D. #
10)	B trans-Chl...	5.923f	0.000	2092660	0	1.100	N.D. #
11)	B cis-Chlor...	5.923	0.000	2092660	0	1.044	N.D. #
15)	B Endosulfa...	6.697	0.000	3200576	0	1.746	N.D. #
16)	A 4,4'-DDD	6.697f	0.000	3200576	0	2.429	N.D. #
17)	MA 4,4'-DDT	6.882f	0.000	1365054	0	1.120	N.D. #
18)	B Endrin al...	6.882f	0.000	1365054	0	1.153	N.D. #
20)	A Methoxychlor	7.468f	0.000	5182644	0	7.084	N.D. #
22)	Toxaphene-1	5.785	0.000	2123882	0	433.425	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 12:06
Operator : AR\AJ
Sample : PIBLK145
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:30:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

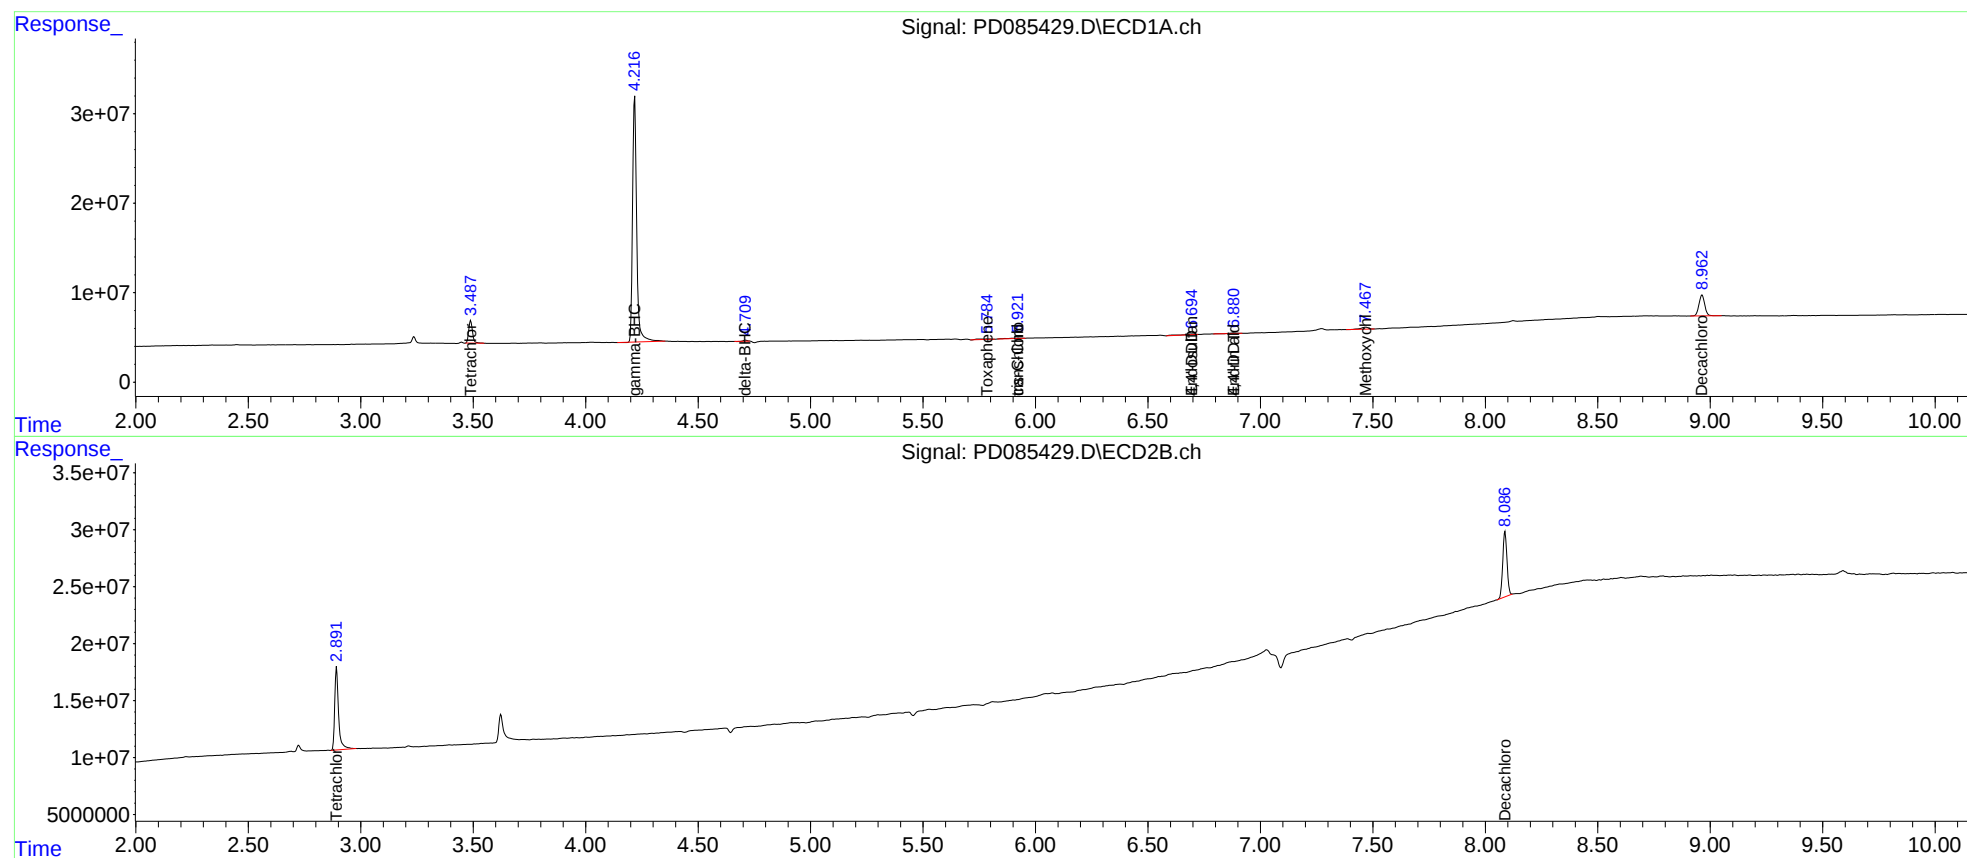

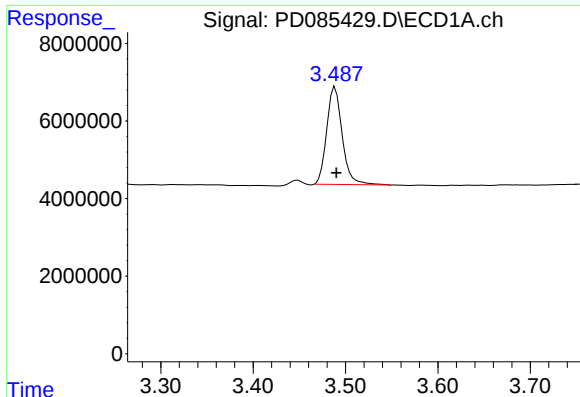


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 29340645
Conc: 24.23 ng/ml

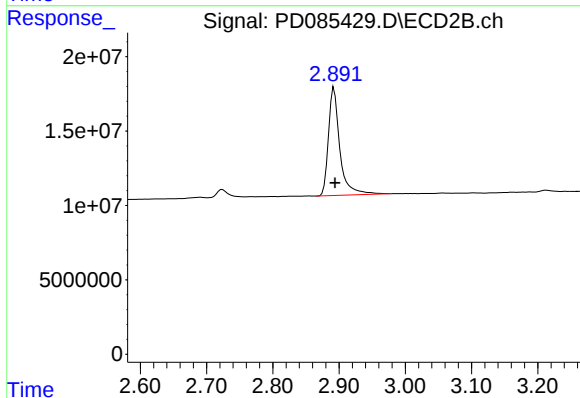


#1 Tetrachloro-m-xylene

R.T.: 2.893 min
Delta R.T.: -0.001 min
Response: 86710840
Conc: 22.94 ng/ml

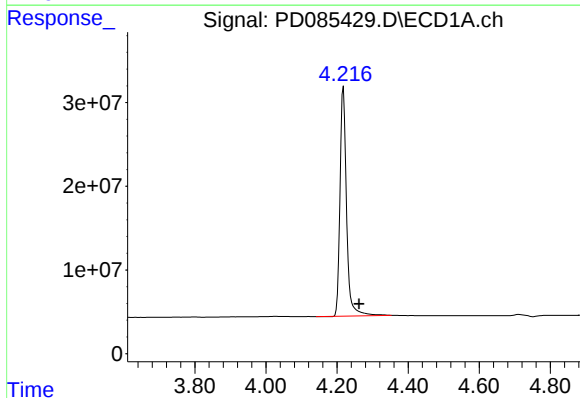


#3 gamma-BHC (Lindane)

R.T.: 4.218 min
Delta R.T.: -0.044 min
Response: 348514060
Conc: 139.30 ng/ml

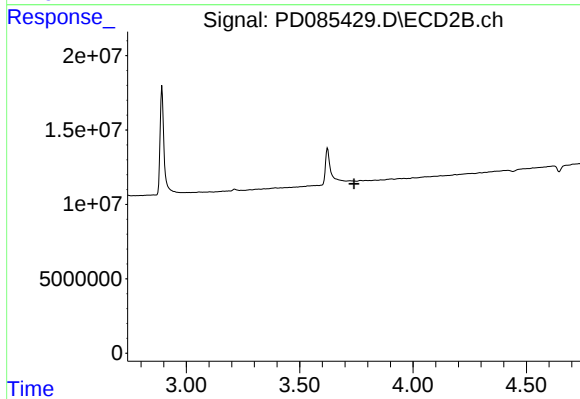


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.739 min
Response: 0
Conc: N.D.

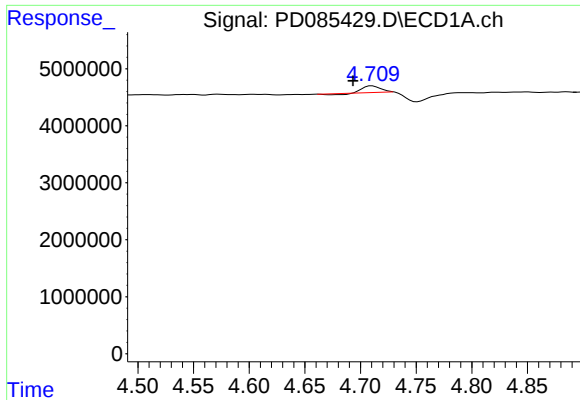


#7 delta-BHC

R.T.: 4.710 min
Delta R.T.: 0.017 min
Response: 1162367
Conc: 0.51 ng/ml

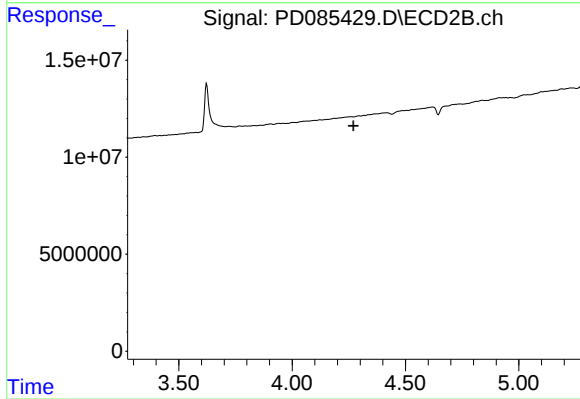


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.

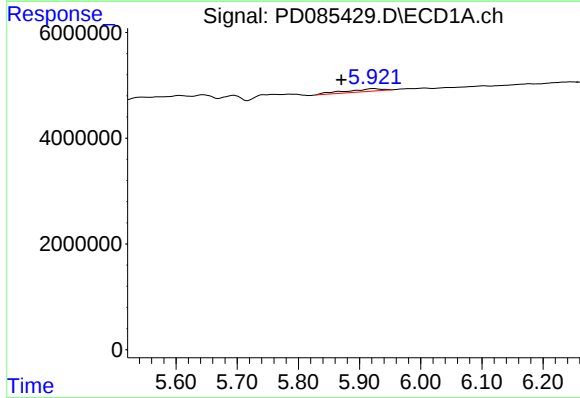


#10 trans-Chlordane

R.T.: 5.923 min
Delta R.T.: 0.052 min
Response: 2092660
Conc: 1.10 ng/ml

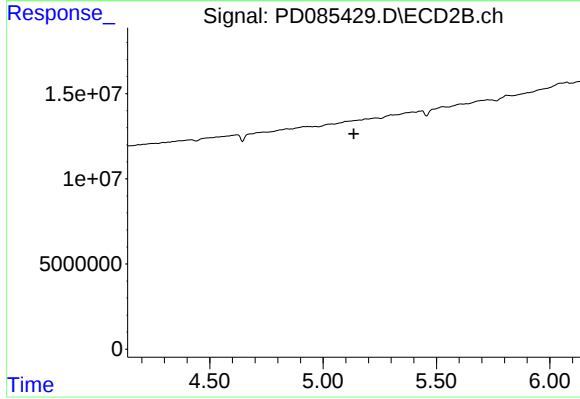


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

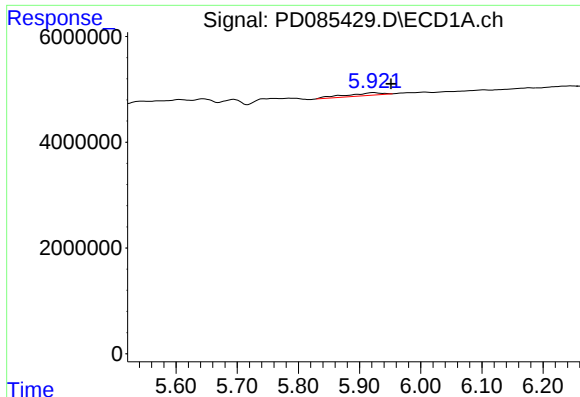


#11 cis-Chlordane

R.T.: 5.923 min
Delta R.T.: -0.029 min
Response: 2092660
Conc: 1.04 ng/ml

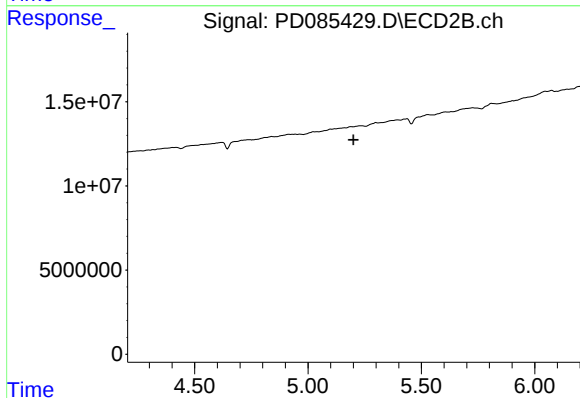


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.201 min
Response: 0
Conc: N.D.

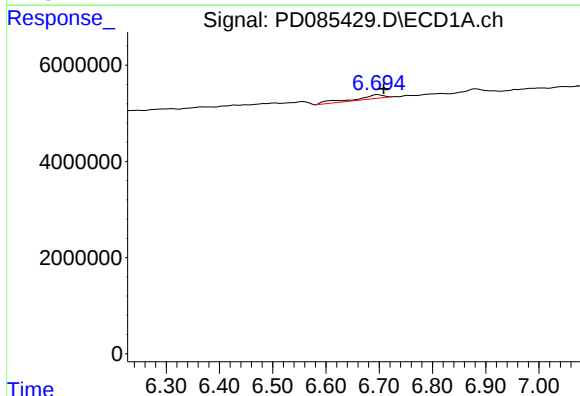


#15 Endosulfan II

R.T.: 6.697 min
Delta R.T.: -0.012 min
Response: 3200576
Conc: 1.75 ng/ml

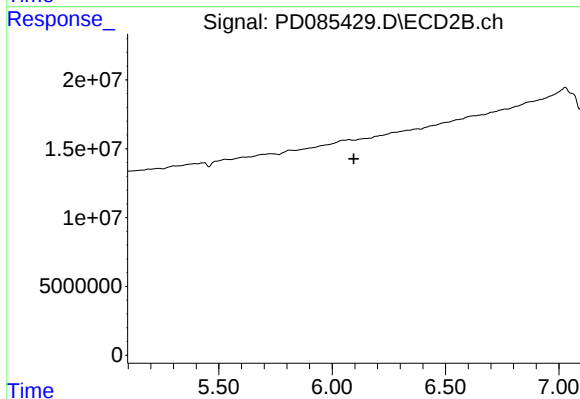


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

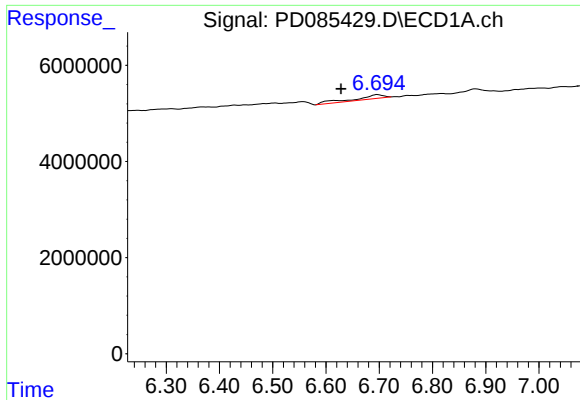


#16 4,4'-DDD

R.T.: 6.697 min
Delta R.T.: 0.068 min
Response: 3200576
Conc: 2.43 ng/ml

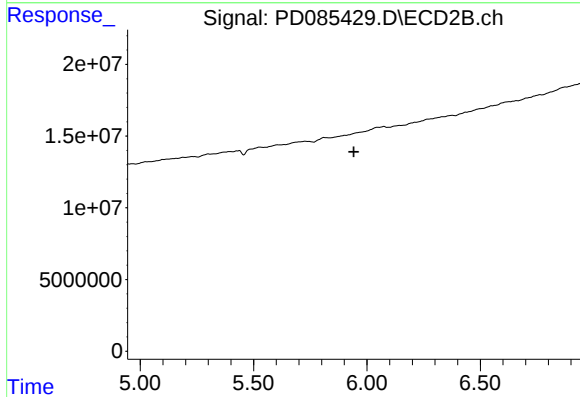


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.942 min
Response: 0
Conc: N.D.

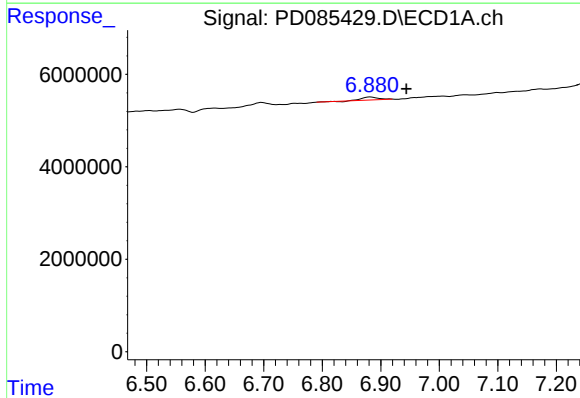


#17 4,4'-DDT

R.T.: 6.882 min
Delta R.T.: -0.062 min
Response: 1365054
Conc: 1.12 ng/ml

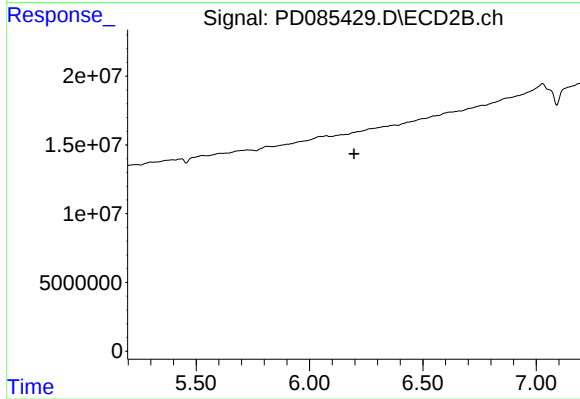


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

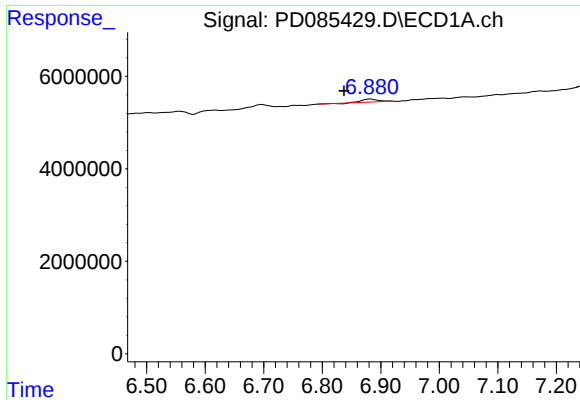


#18 Endrin aldehyde

R.T.: 6.882 min
Delta R.T.: 0.045 min
Response: 1365054
Conc: 1.15 ng/ml

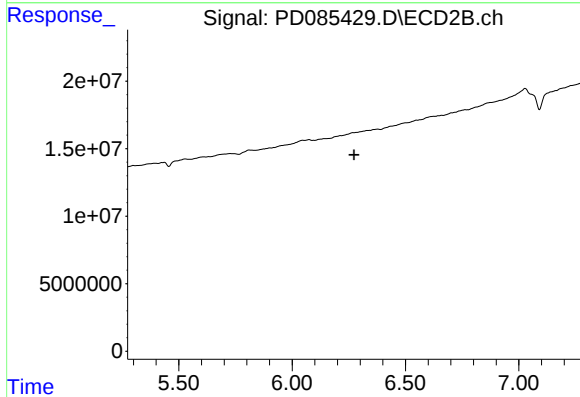


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.274 min
Response: 0
Conc: N.D.

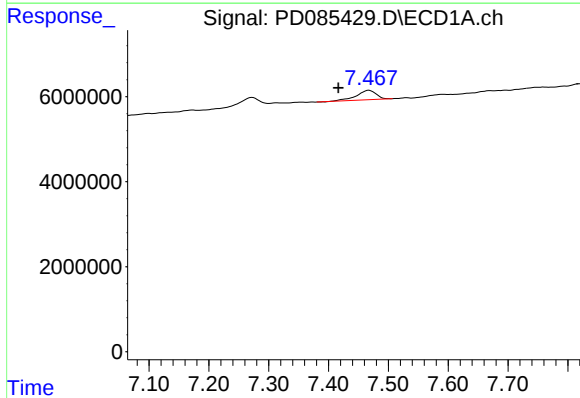


#20 Methoxychlor

R.T.: 7.468 min
Delta R.T.: 0.051 min
Response: 5182644
Conc: 7.08 ng/ml

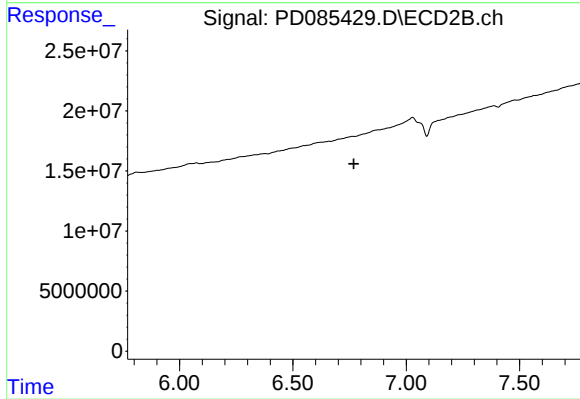


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.768 min
Response: 0
Conc: N.D.

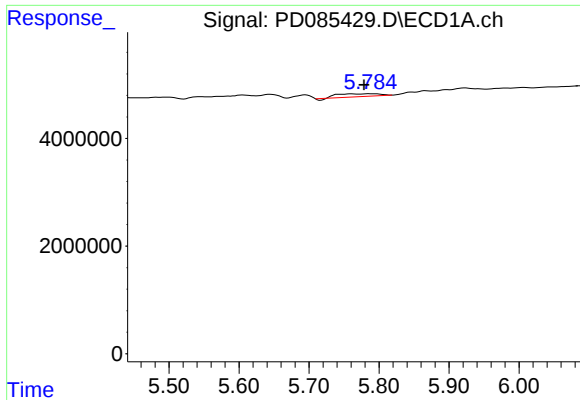


#22 Toxaphene-1

R.T.: 5.785 min
Delta R.T.: 0.007 min
Response: 2123882
Conc: 433.42 ng/ml

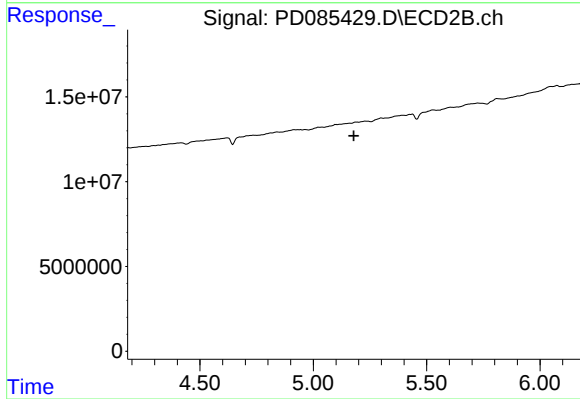


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

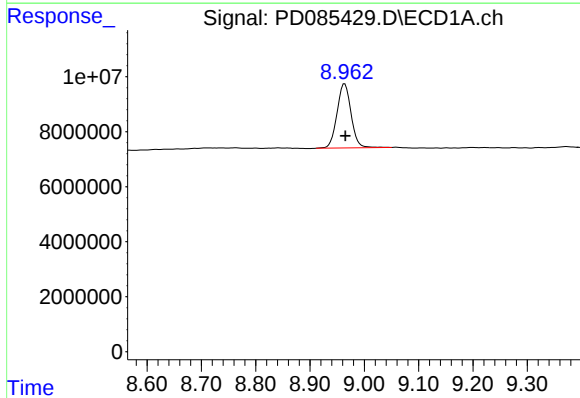

#27 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.002 min
Response: 41990645
Conc: 25.60 ng/ml

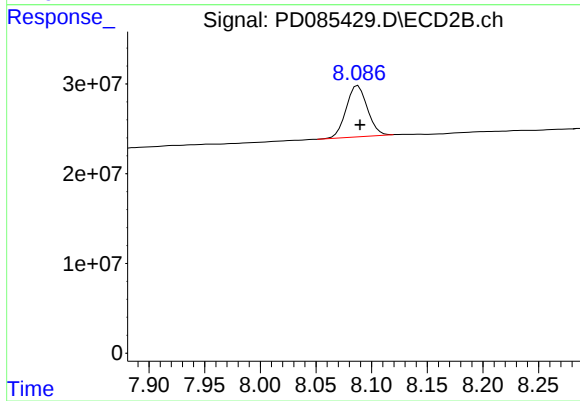

#27 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: -0.002 min
Response: 76453924
Conc: 28.60 ng/ml