

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 23:30
 Operator : AR\AJ
 Sample : P4016-19MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC23MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:42:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.488	2.904	18463080	11395.4E6	15.246m	3014.767m#
2) SA Decachlor...	8.955	8.082	26923351	43747978	16.412m	16.365m
Target Compounds						
2) A alpha-BHC	3.934	3.403	548.2E6	816.9E6	232.010	147.937 #
3) MA gamma-BHC...	4.200f	3.735	106758.5E6	2063.7E6	42672.098m	396.005m#
4) MA Heptachlor	4.855	4.088	111.6E6	219.0E6	52.831m	46.145m
5) MB Aldrin	5.199	4.358	120.9E6	152.9E6	55.692	30.160m#
6) B beta-BHC	4.445	4.028	57897206	84813073	60.712m	36.471m#
7) B delta-BHC	4.692	4.270	655.1E6	990.2E6	287.389	187.981 #
8) B Heptachlo...	5.612	4.878	53104185	781.5E6	26.586m	168.339 #
9) A Endosulfan I	5.996	5.258	122.7E6	150.8E6	69.256m	36.700 #
10) B trans-Chl...	5.865	5.134	106.8E6	222.3E6	56.115m	49.122m
11) B cis-Chlor...	5.945	5.201	103.3E6	222.0E6	51.549m	47.858
12) B 4,4'-DDE	6.117	5.382	204.4E6	243.3E6	116.908m	56.787m#
13) MA Dieldrin	6.268	5.523	229.1E6	360.7E6	118.497	77.479 #
14) MA Endrin	6.492	5.800	164.4E6	383.1E6	102.244m	92.368m
15) B Endosulfa...	6.706	6.091	143.3E6	436.7E6	78.147m	118.026m#
16) A 4,4'-DDD	6.625	5.940	174.1E6	286.0E6	132.162m	85.395m#
17) MA 4,4'-DDT	6.938	6.194	369.2E6	407.4E6	302.833m	128.607m#
18) B Endrin al...	6.838	6.270	178.3E6	202.6E6	150.537m	73.280m#
19) B Endosulfa...	7.067	6.496	138.7E6	271.2E6	91.890m	78.957
20) A Methoxychlor	7.412	6.765	496.7E6	931.7E6	678.837m	574.062m
21) B Endrin ke...	7.546	7.006	119.1E6	334.7E6	74.525	72.067m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 23:30
Operator : AR\AJ
Sample : P4016-19MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:42:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

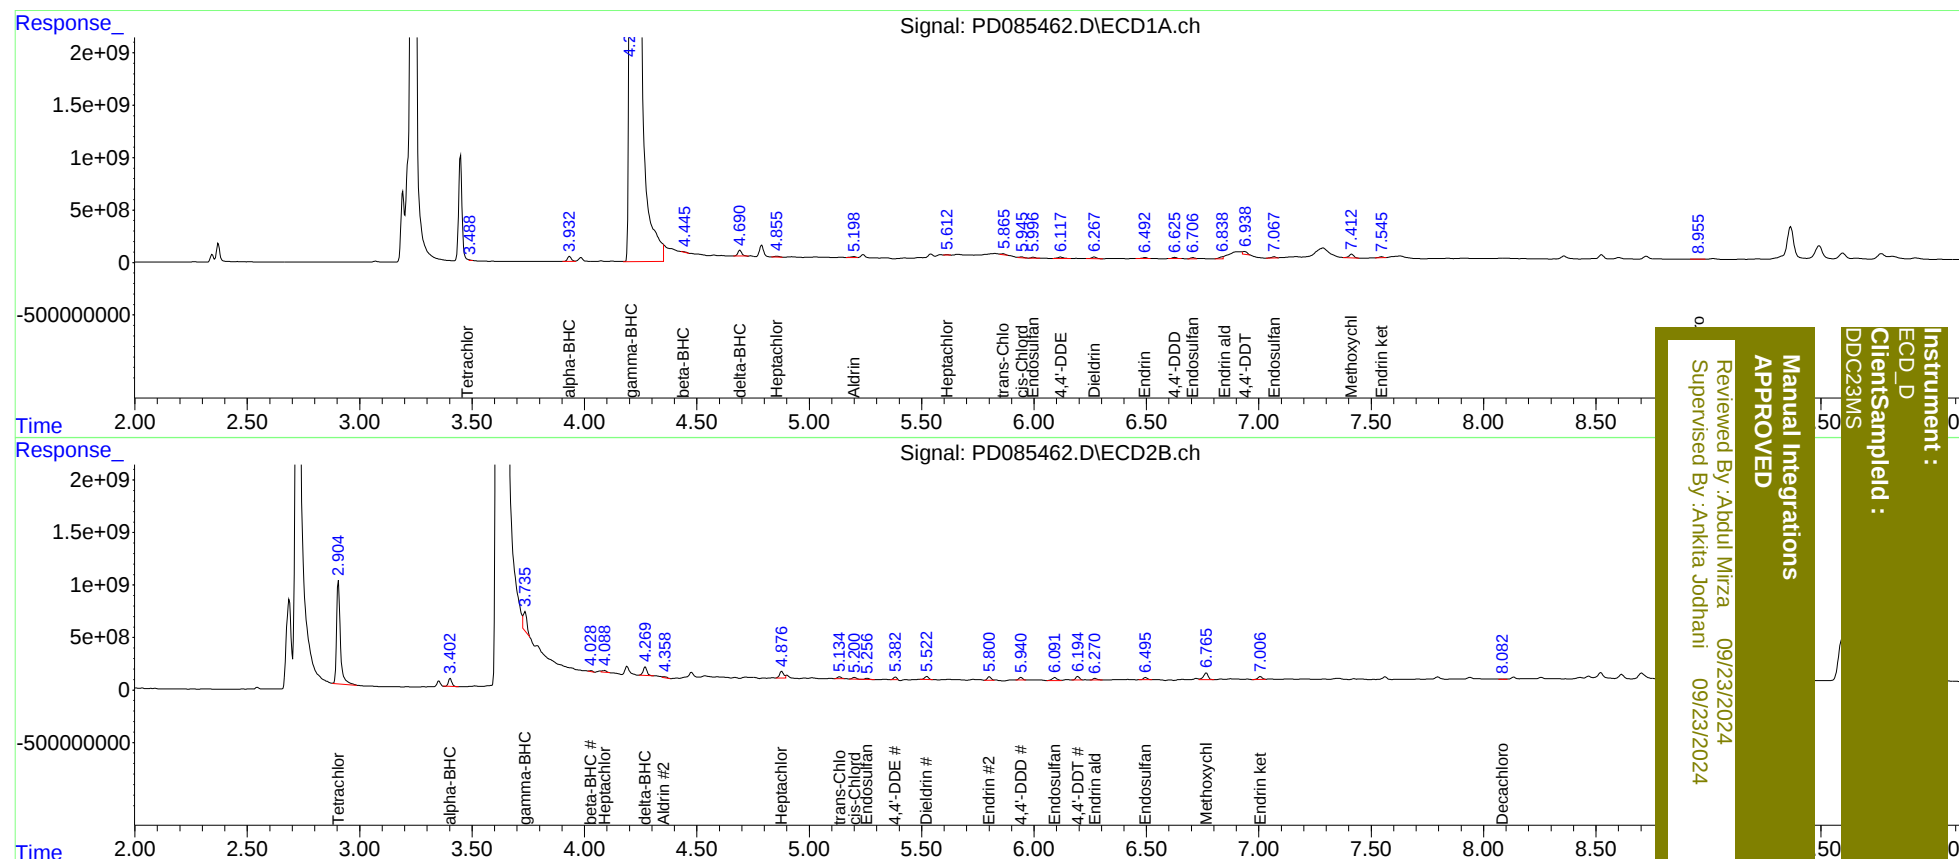

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/23/2024
Supervised By: Ankita Jodhani 09/23/2024

Instrument :
ECD_D
Client Sampled :
DDC23MS