

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2024 01:57
 Operator : AR\AJ
 Sample : P3927-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC93

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 06:50:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.481	2.904	17414240	1953.6E6	14.380m	516.842m#
27)	SA Decachlor...	8.956	8.084	34499193	36409256	21.030m	13.620m#
Target Compounds							
2)	A alpha-BHC	3.933	3.403	296.7E6	547.3E6	125.567	99.112
7)	B delta-BHC	4.692	4.270	427.4E6	685.3E6	187.495	130.102 #
10)	B trans-Chl...	5.853	5.134	70573477	137.5E6	37.080m	30.383m
11)	B cis-Chlor...	5.939	5.204	75122386	149.5E6	37.474m	32.237m
13)	MA Dieldrin	6.273	5.512	60585511	107.5E6	31.338m	23.100m#
14)	MA Endrin	6.471	5.800	85979498	122.0E6	53.477m	29.411m#
16)	A 4,4'-DDD	6.626	5.941	80324169	114.2E6	60.965m	34.087m#
20)	A Methoxychlor	7.403	6.751	21089555	306.1E6	28.825m	188.600m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2024 01:57
Operator : AR\AJ
Sample : P3927-08
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 06:50:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

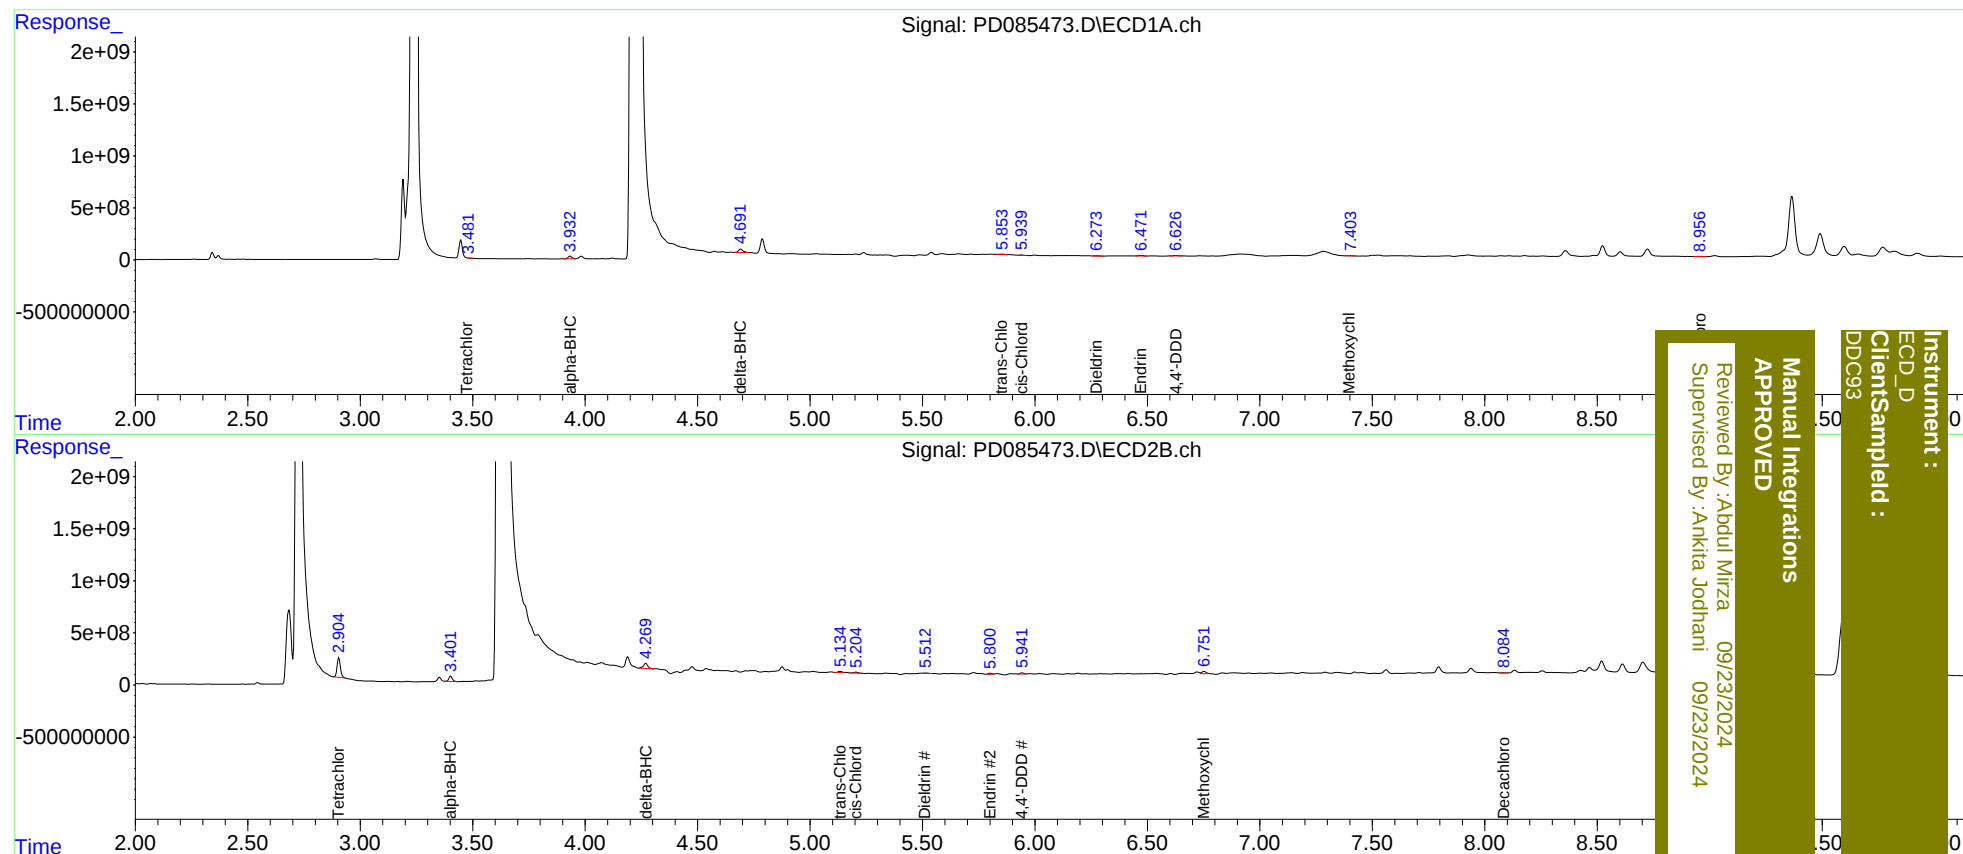

Reviewed By: Abdul Mirza 09/23/2024
Supervised By: Ankita Jodhani 09/23/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC93