

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2024 04:25
 Operator : AR\AJ
 Sample : P3927-19MSD
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 06:16:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	2.905	30715922	1789.5E6	25.365m	473.440 #
27) SA Decachlor...	8.961	8.089	17035983	57707185	10.385	21.586 #
Target Compounds						
2) A alpha-BHC	3.933	3.403	116.0E6	258.7E6	49.106	46.839
3) MA gamma-BHC...	4.202f	3.758	75198.5E6	530.9E6	30057.353m	101.869m#
4) MA Heptachlor	4.855	4.090	115.1E6	391.0E6	54.506	82.379 #
5) MB Aldrin	5.195	4.377	118.5E6	256.2E6	54.588	50.553
6) B beta-BHC	4.431	4.023	57960588	191.1E6	60.778m	82.194m#
7) B delta-BHC	4.691	4.270	166.5E6	234.4E6	73.040	44.496 #
8) B Heptachlo...	5.614	4.879	125.2E6	272.8E6	62.699	58.763m
9) A Endosulfan I	5.995	5.257	88725175	157.9E6	50.061	38.425
10) B trans-Chl...	5.867	5.134	150.2E6	184.8E6	78.916	40.828 #
11) B cis-Chlor...	5.948	5.199	93957102	199.9E6	46.869	43.096
12) B 4,4'-DDE	6.119	5.383	196.5E6	396.7E6	112.393	92.603m
13) MA Dieldrin	6.268	5.522	227.5E6	389.6E6	117.676	83.700m#
14) MA Endrin	6.494	5.800	185.1E6	461.5E6	115.157	111.262
15) B Endosulfa...	6.705	6.093	151.2E6	350.4E6	82.452	94.712
16) A 4,4'-DDD	6.625	5.939	145.9E6	300.7E6	110.738m	89.794m
17) MA 4,4'-DDT	6.939	6.194	269.4E6	332.4E6	220.972m	104.930m#
18) B Endrin al...	6.833	6.272	101.6E6	247.1E6	85.799m	89.377
19) B Endosulfa...	7.066	6.496	148.1E6	326.6E6	98.123m	95.098
20) A Methoxychlor	7.413	6.767	372.6E6	749.3E6	509.292	461.694
21) B Endrin ke...	7.547	7.007	187.8E6	384.8E6	117.483	82.846 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2024 04:25
Operator : AR\AJ
Sample : P3927-19MSD
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 06:16:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

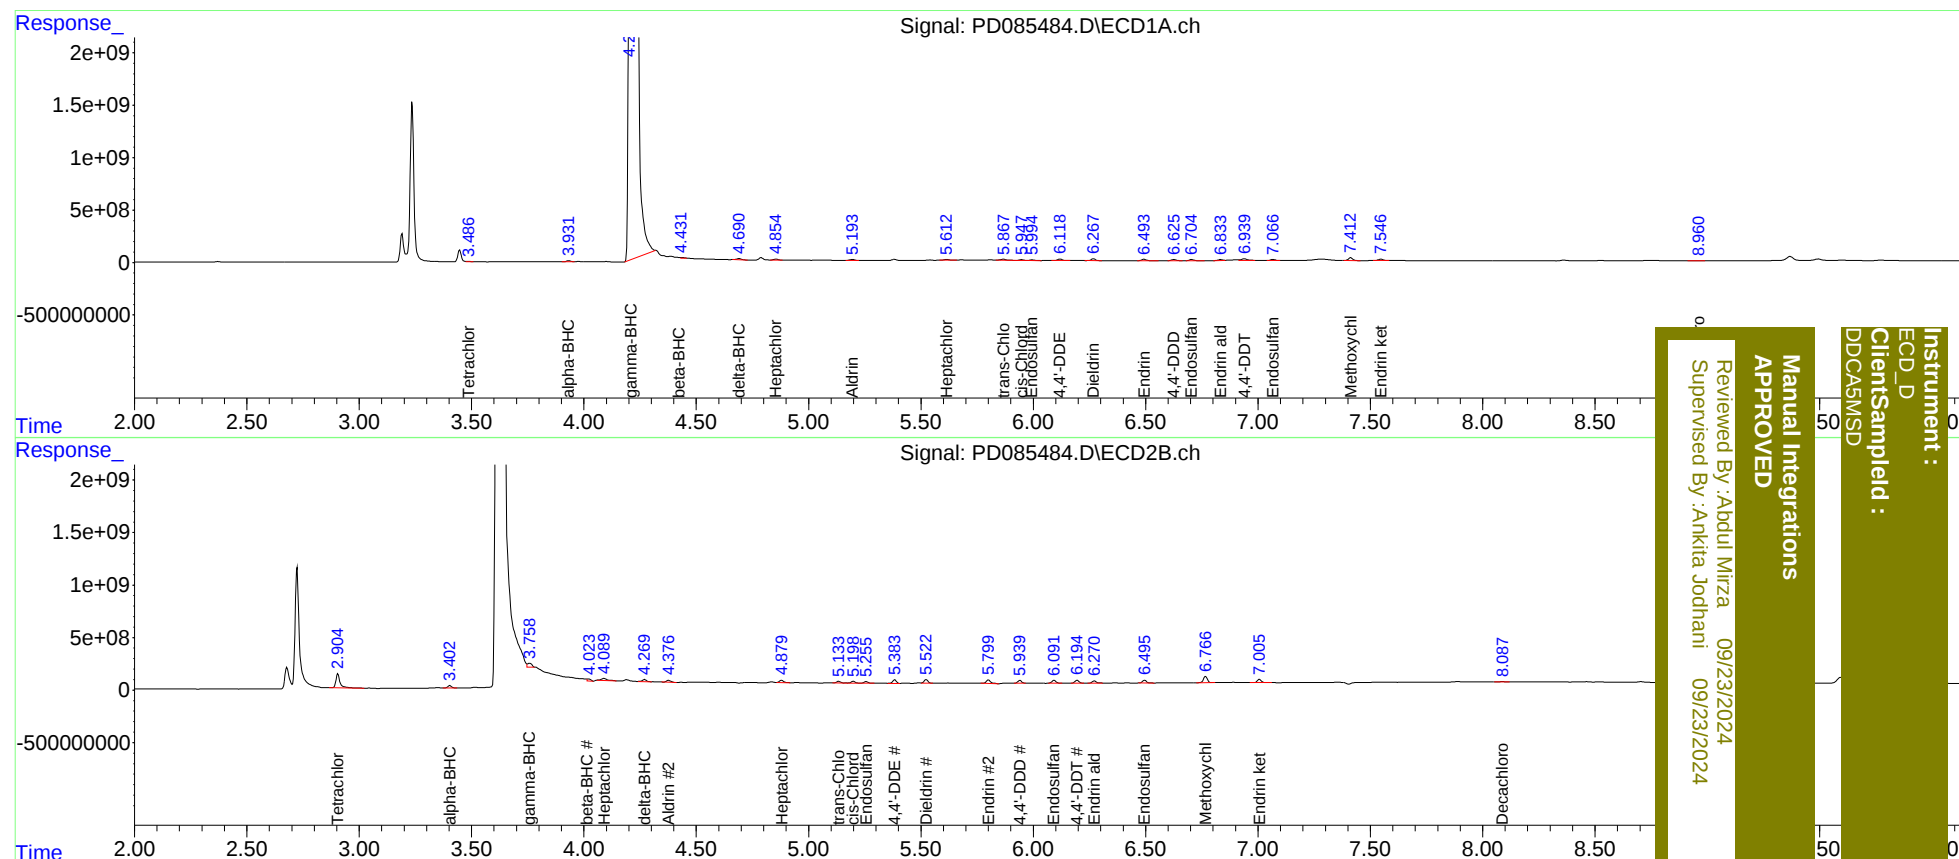

Reviewed By: Abdul Mirza 09/23/2024
Supervised By: Ankita Jodhani 09/23/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCASMSD