

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2024 04:38
 Operator : AR\AJ
 Sample : P3927-20
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 06:16:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.487	2.903	16512842	461.1E6	13.636m	121.986m#
2) SA Decachlor...	8.958	8.086	22169631	34175738	13.514m	12.784m
Target Compounds						
2) A alpha-BHC	3.932	3.402	42379293	139.3E6	17.937	25.233 #
7) B delta-BHC	4.692	4.270	80450948	132.4E6	35.292	25.139 #
13) MA Dieldrin	6.271	5.512	29077231	78818289	15.040m	16.932m
14) MA Endrin	6.471	5.801	52936565	71876638	32.925m	17.329m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2024 04:38
Operator : AR\AJ
Sample : P3927-20
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 06:16:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

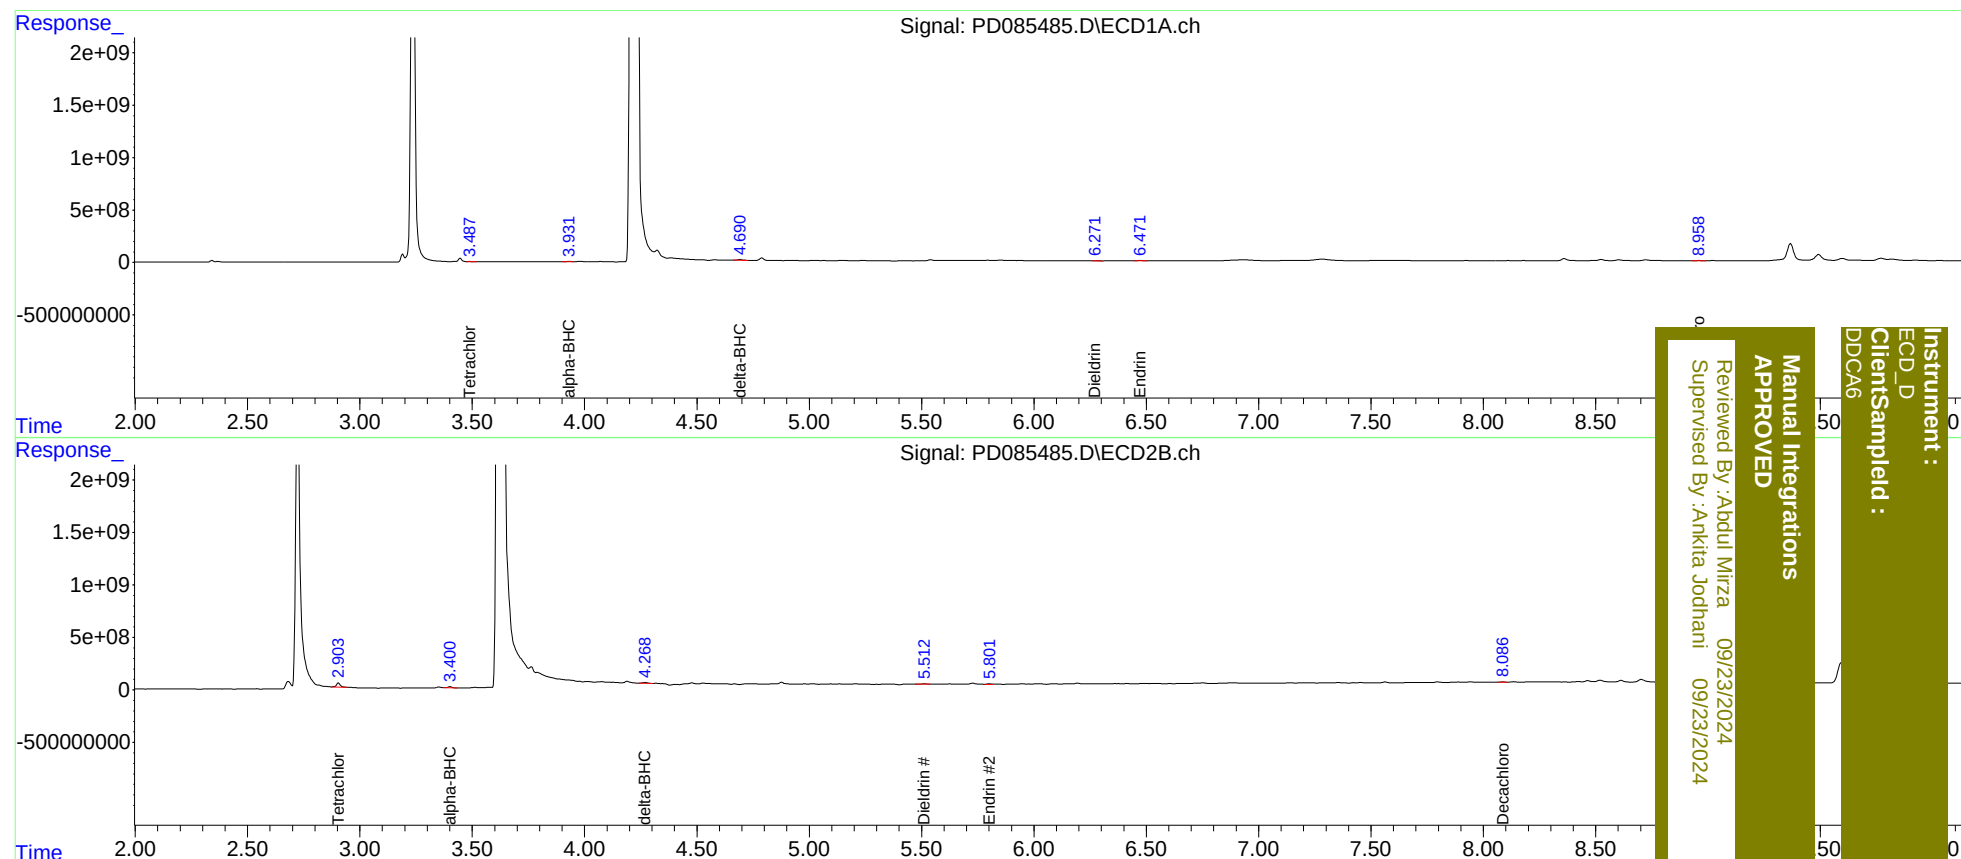

Instrument :
ECD_D
ClientSampled :
DDCA6

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024