

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 20:36
 Operator : AR\AJ
 Sample : P4016-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVT7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:37:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	2.904	29883596	993.5E6	24.677m	262.851m#
27) SA Decachlor...	8.960	8.086	30347628	61469330	18.500m	22.994m
Target Compounds						
2) A alpha-BHC	3.932	3.403	4182240	9408533	1.770m	1.704
7) B delta-BHC	4.710	4.270	526.6E6	11999742	230.988m	2.278 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 20:36
Operator : AR\AJ
Sample : P4016-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:37:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

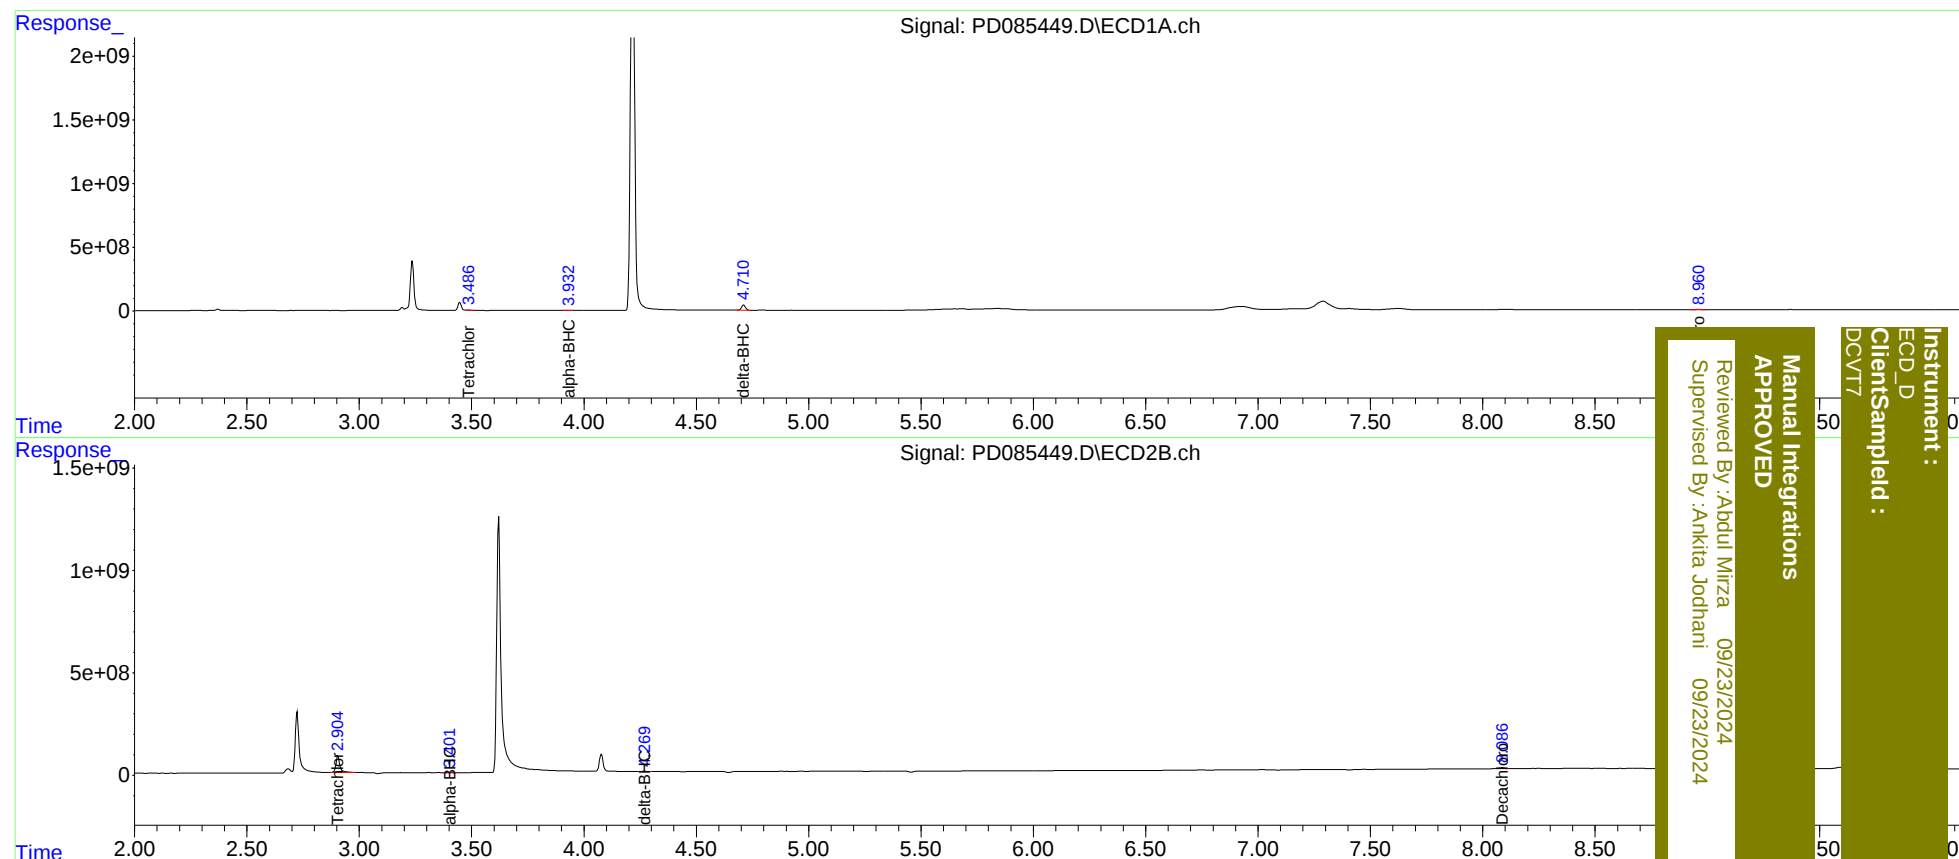

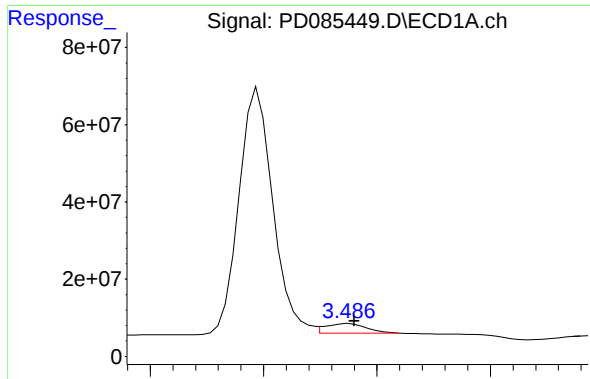


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.004 min
Response: 29883596
Conc: 24.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVT7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

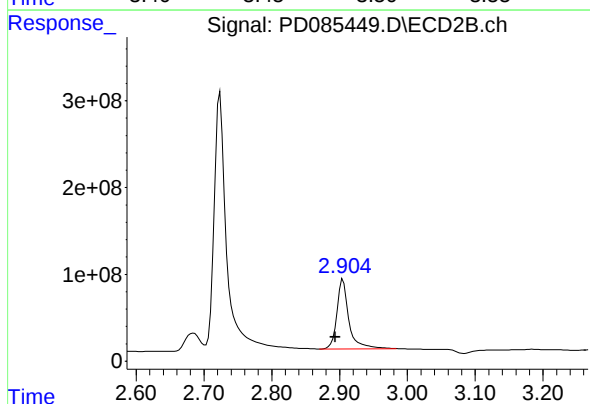


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: 0.010 min
Response: 993538118
Conc: 262.85 ng/ml m

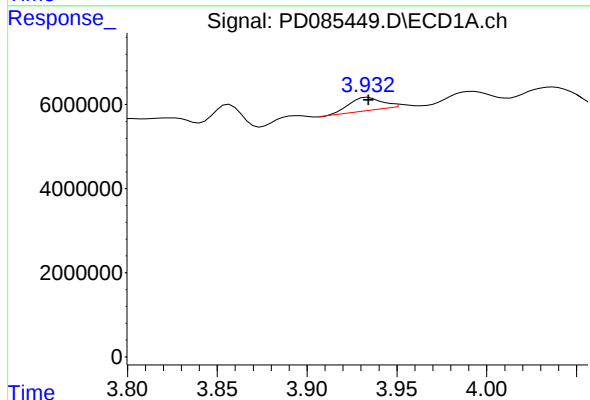


#2 alpha-BHC

R.T.: 3.932 min
Delta R.T.: -0.002 min
Response: 4182240
Conc: 1.77 ng/ml m

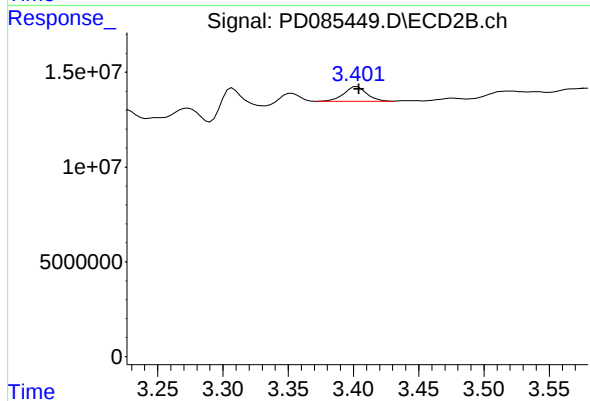

#2 alpha-BHC

R.T.: 3.403 min
Delta R.T.: -0.001 min
Response: 9408533
Conc: 1.70 ng/ml

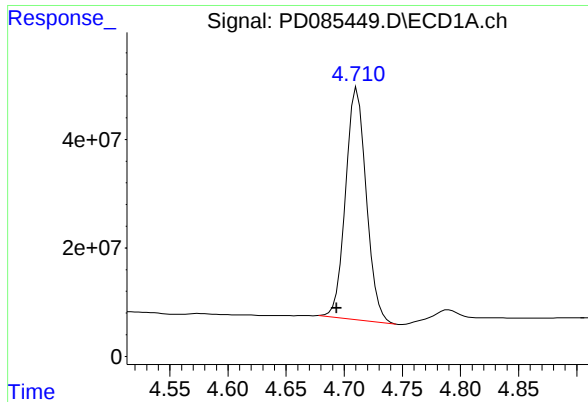


#7 delta-BHC

R.T.: 4.710 min
Delta R.T.: 0.016 min
Response: 526563695
Conc: 230.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVT7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

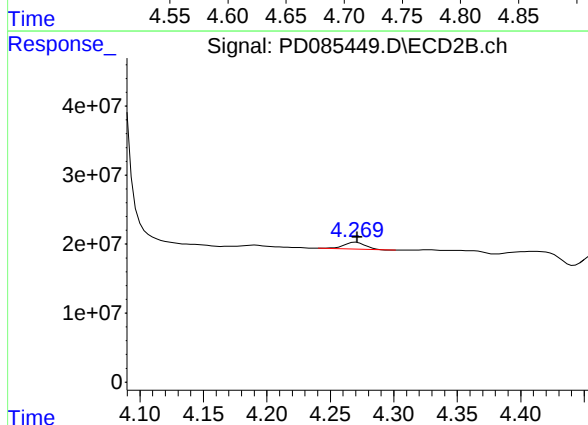


#7 delta-BHC

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 11999742
Conc: 2.28 ng/ml

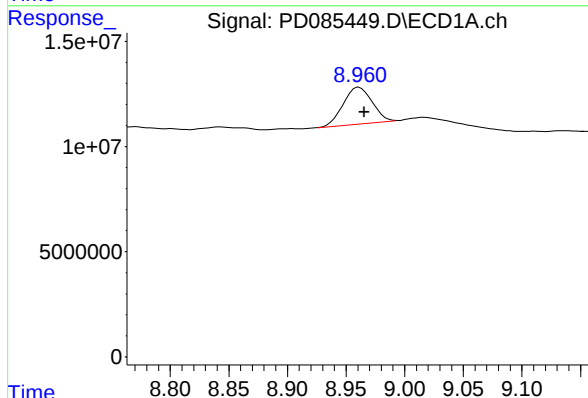

#27 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.006 min
Response: 30347628
Conc: 18.50 ng/ml m

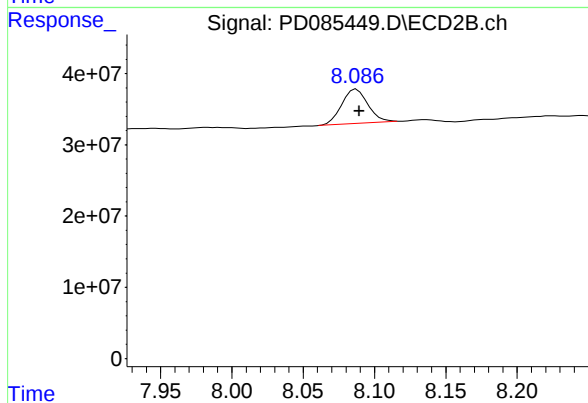

#27 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: -0.003 min
Response: 61469330
Conc: 22.99 ng/ml m