

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 22:10
 Operator : AR\AJ
 Sample : P4016-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVW4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:40:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.487	2.903	18564150	206.2E6	15.330m	54.555m#
27) SA Decachlor...	8.977	8.087	63199032	47656306	38.525m	17.827m#
Target Compounds						
2) A alpha-BHC	3.943	3.400	1252598	4778899	0.530m	0.865m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 22:10
Operator : AR\AJ
Sample : P4016-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:40:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

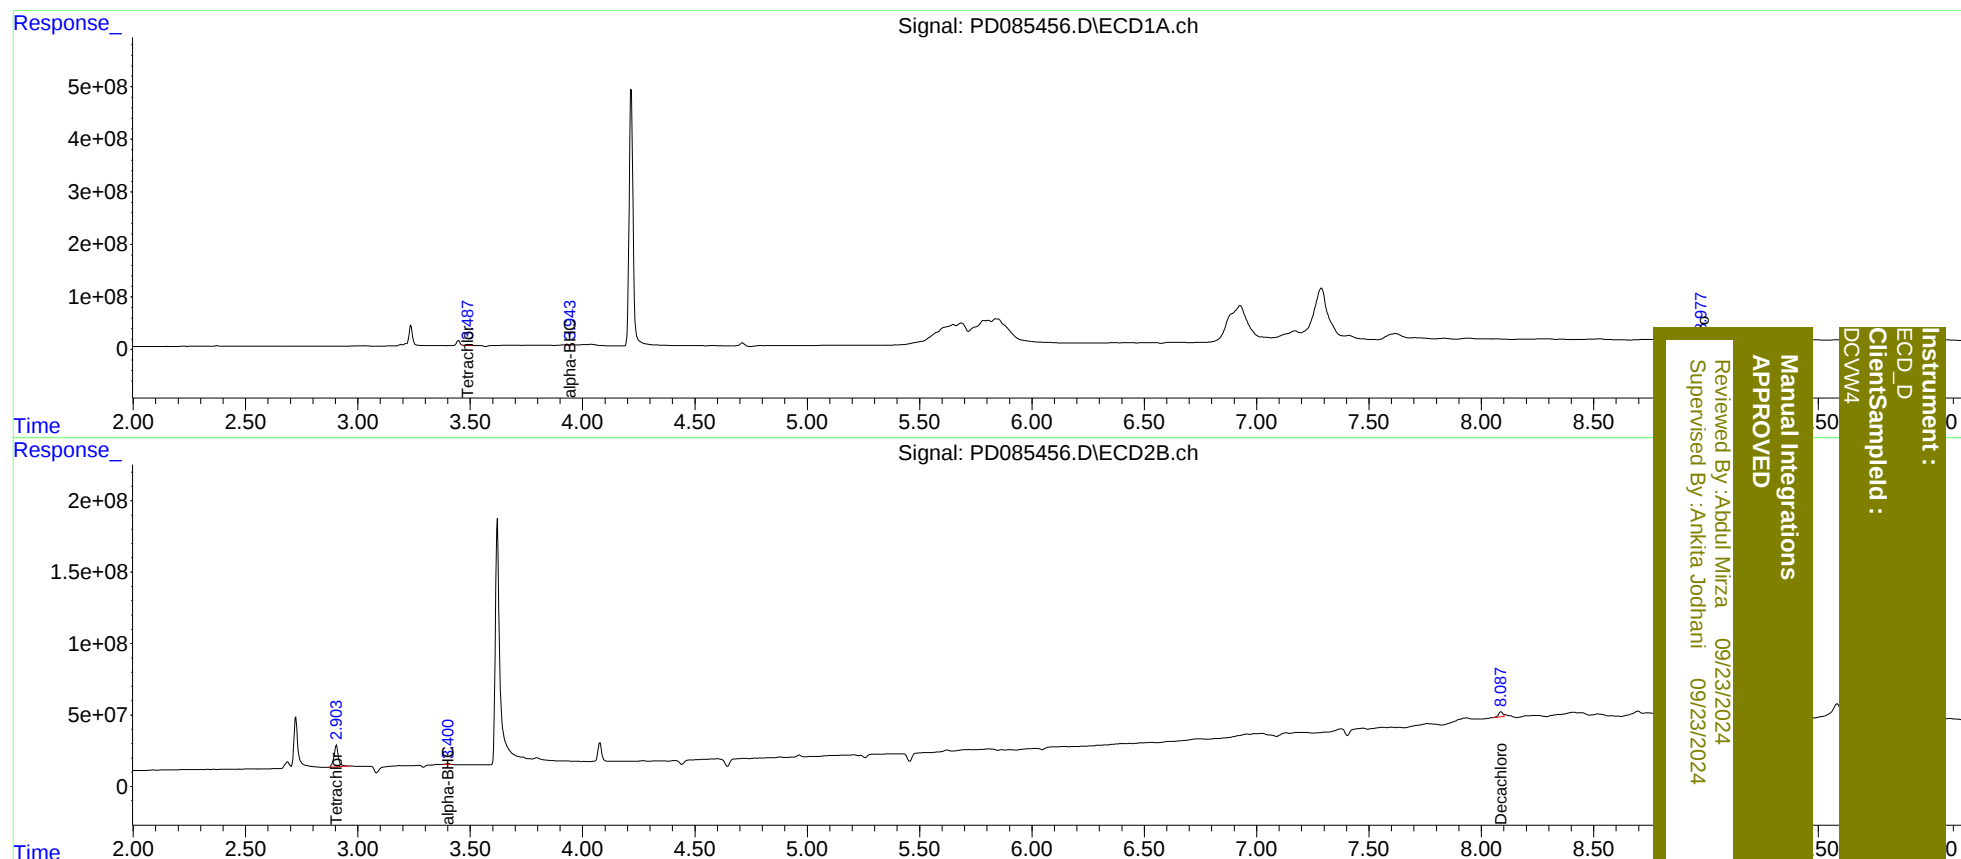

Reviewed By: Abdul Mirza 09/23/2024
Supervised By: Ankita Jodhani 09/23/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DCW/4

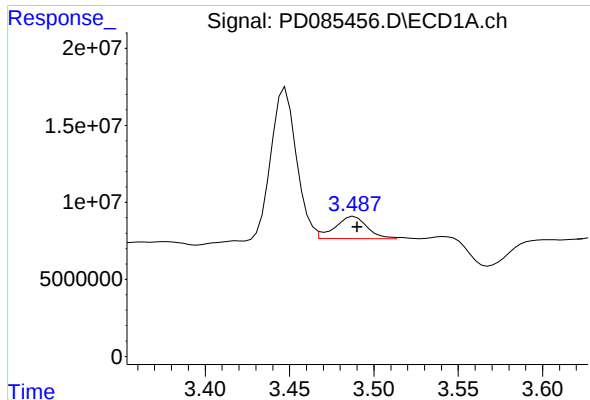


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 18564150
Conc: 15.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVW4


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

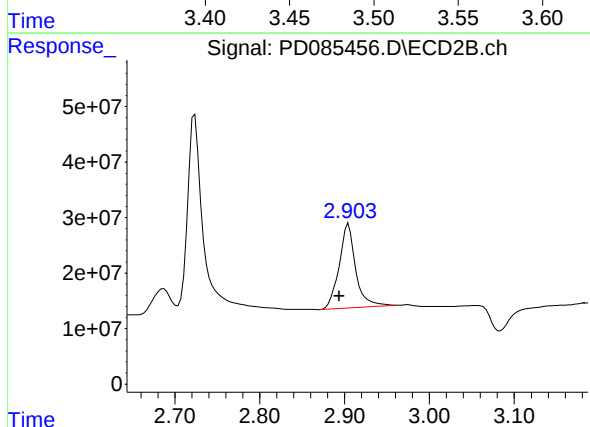


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: 0.009 min
Response: 206209450
Conc: 54.55 ng/ml m

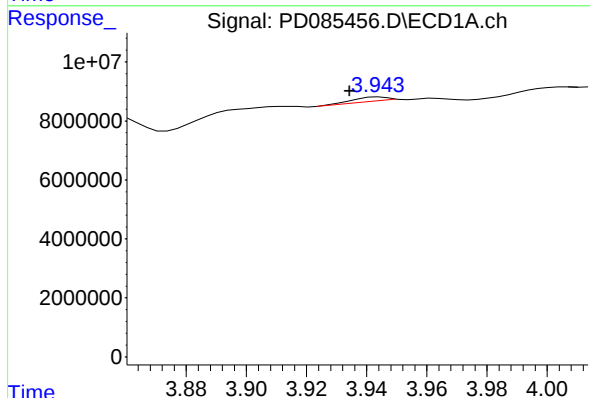


#2 alpha-BHC

R.T.: 3.943 min
Delta R.T.: 0.008 min
Response: 1252598
Conc: 0.53 ng/ml m

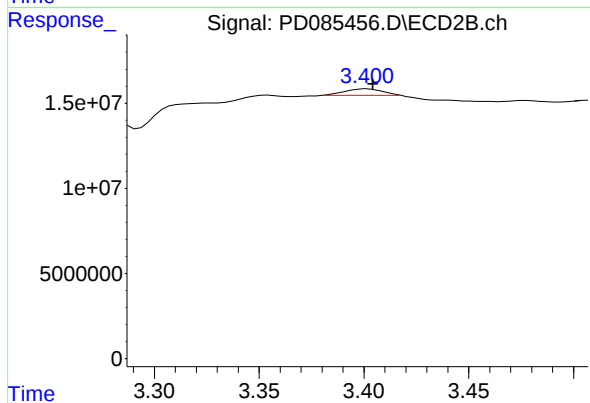

#2 alpha-BHC

R.T.: 3.400 min
Delta R.T.: -0.004 min
Response: 4778899
Conc: 0.87 ng/ml m

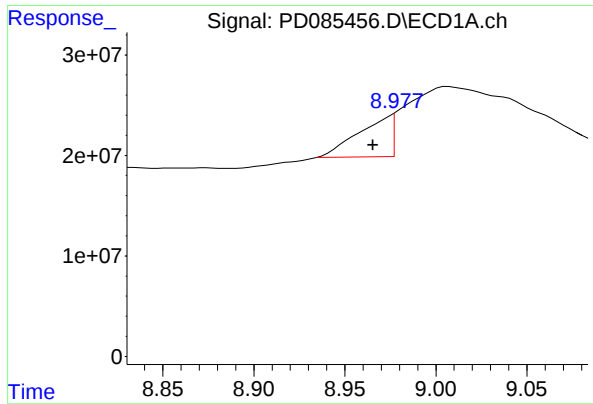


#27 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.012 min
Response: 63199032
Conc: 38.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVW4

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

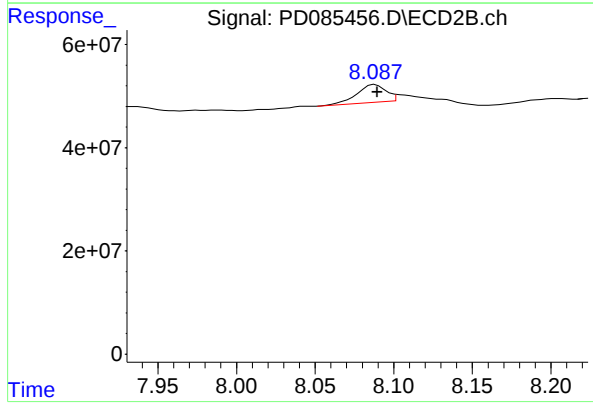

#27 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 47656306
Conc: 17.83 ng/ml m