

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 22:23
 Operator : AR\AJ
 Sample : P4016-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVW5

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

09/23/2024
 Supervised By :Ankita
 Jodhani

09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:40:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.488	2.900	21289489	152.7E6	17.580	40.400 #
27) SA Decachlor...	8.959	8.086	35701110	56867516	21.763m	21.272m


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 22:23
Operator : AR\AJ
Sample : P4016-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:40:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

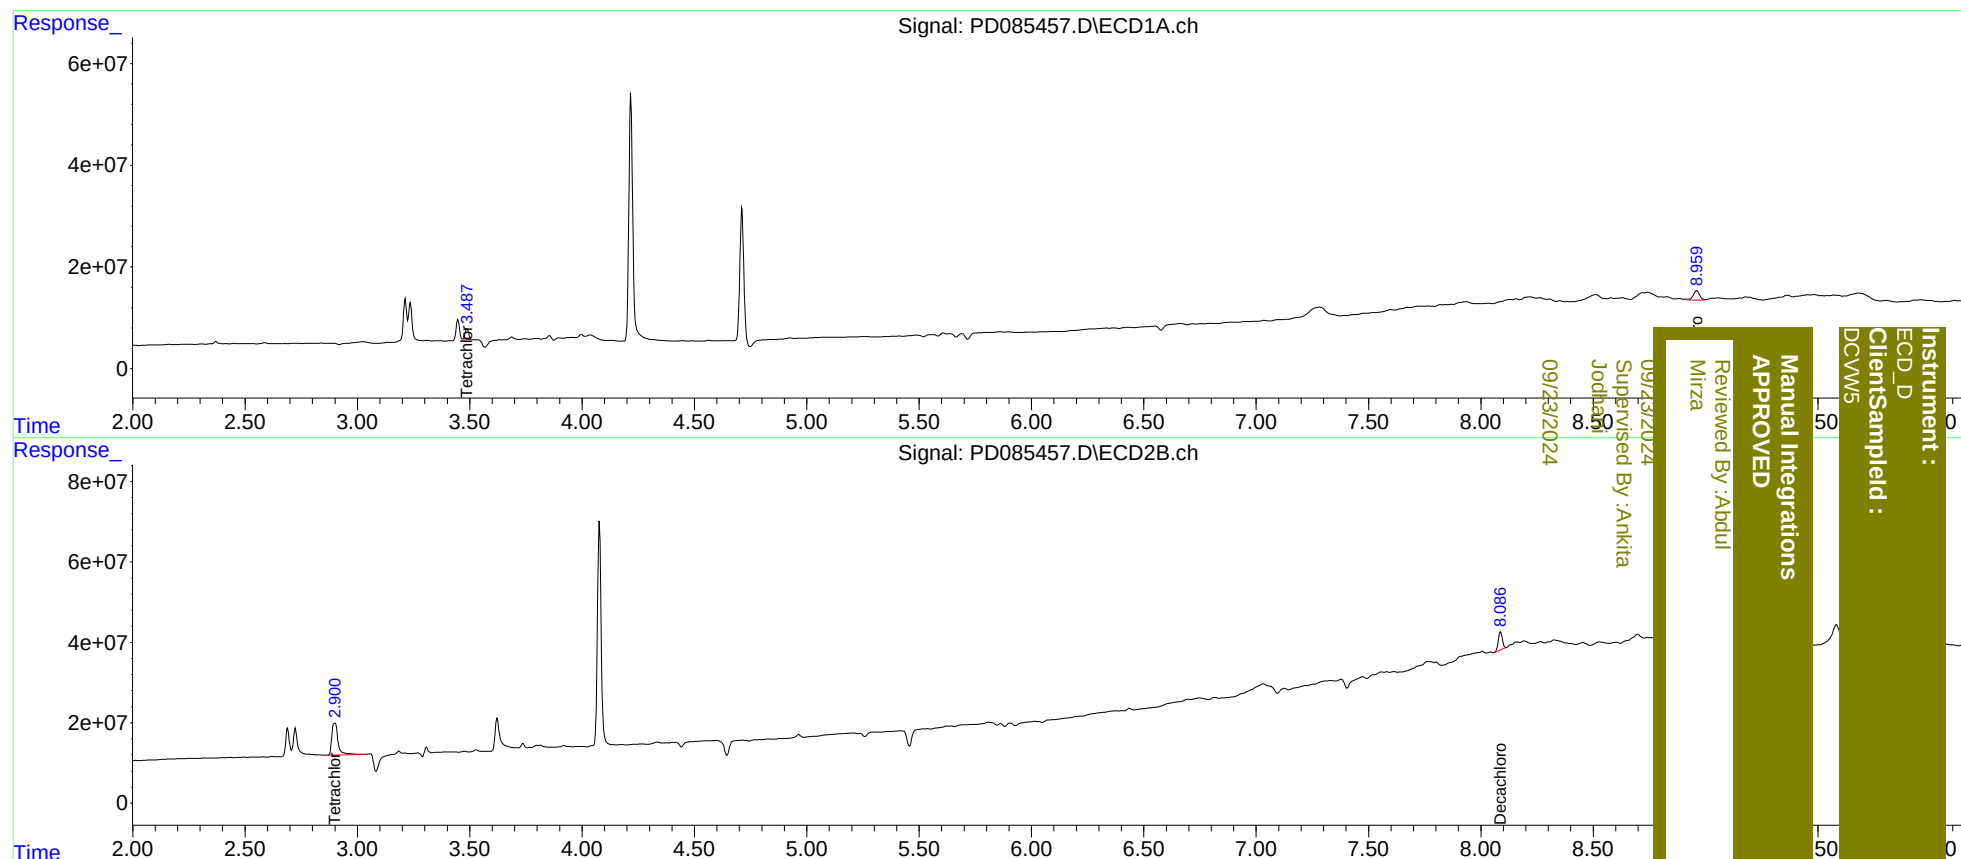

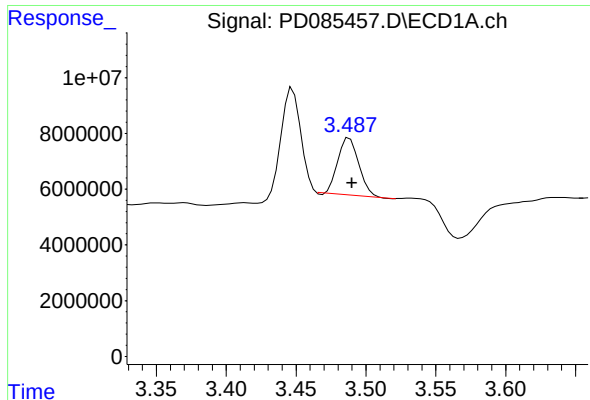

#1 Tetrachloro-m-xylene

R.T.: 3.488 min
Delta R.T.: -0.002 min
Response: 21289489
Conc: 17.58 ng/ml


Instrument :
ECD_D
ClientSampleId :
DCVW5

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza


09/23/2024
Supervised By :Ankita
Jodhani

09/23/2024

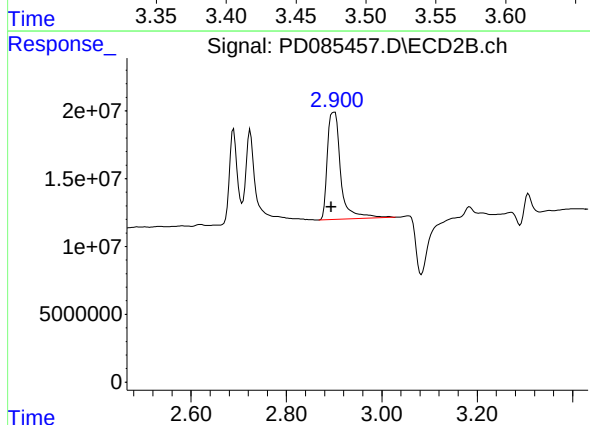


#1 Tetrachloro-m-xylene

R.T.: 2.900 min
Delta R.T.: 0.006 min
Response: 152707311
Conc: 40.40 ng/ml

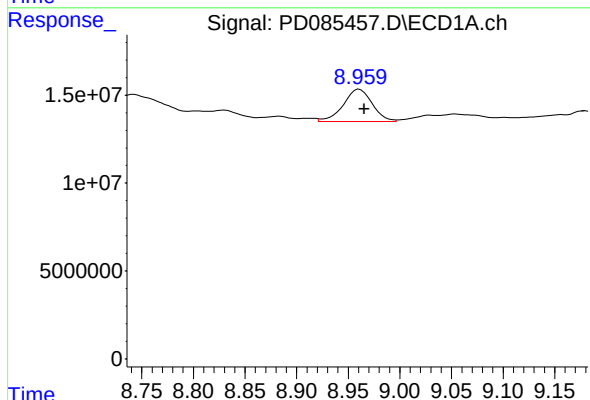

#27 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.006 min
Response: 35701110
Conc: 21.76 ng/ml m

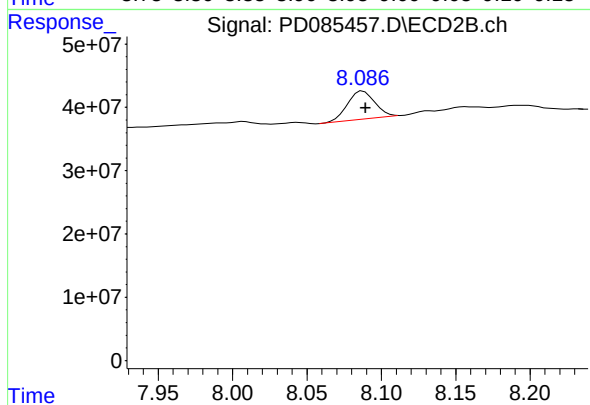

#27 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 56867516
Conc: 21.27 ng/ml m