

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
 Data File : PD085480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2024 03:31
 Operator : AR\AJ
 Sample : P3927-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DD2D2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 06:15:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.487	2.904	13973694	197.9E6	11.539m	52.355 #
2) SA Decachlor...	8.960	8.087	22435798	42761615	13.677	15.996
Target Compounds						
7) B delta-BHC	4.710	4.270	193.5E6	7717314	84.868m	1.465 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092024\
Data File : PD085480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2024 03:31
Operator : AR\AJ
Sample : P3927-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 06:15:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

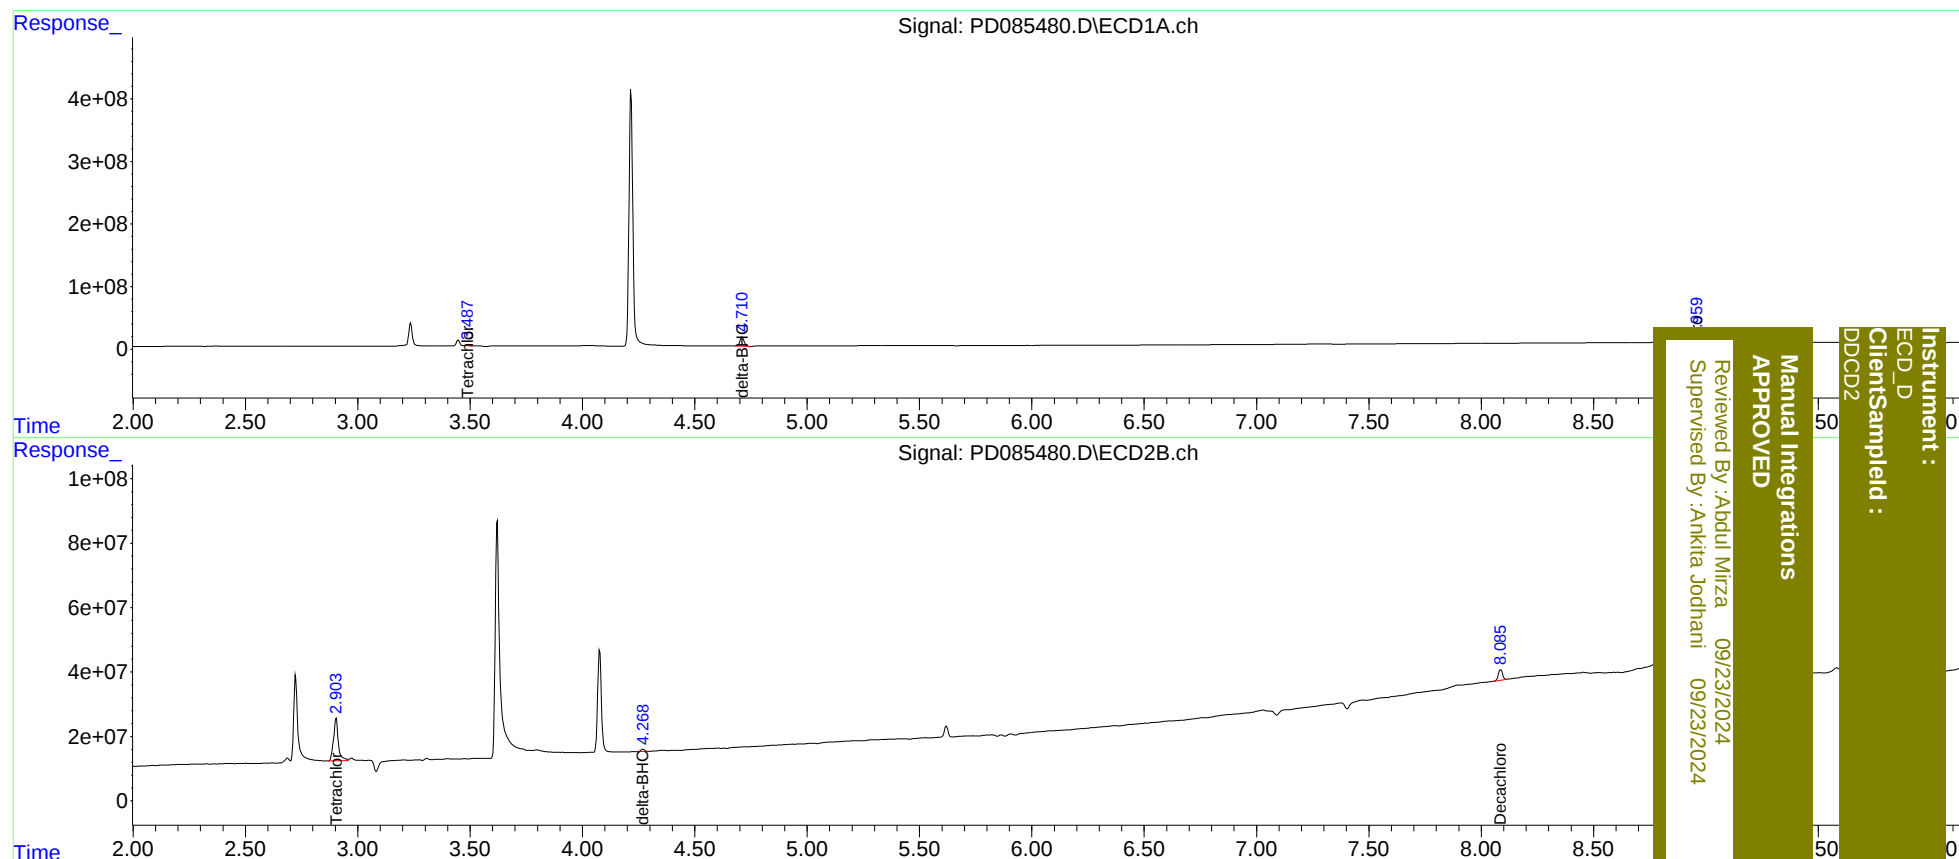

Reviewed By: Abdul Mirza 09/23/2024
Supervised By: Ankita Jodhani 09/23/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDCD2

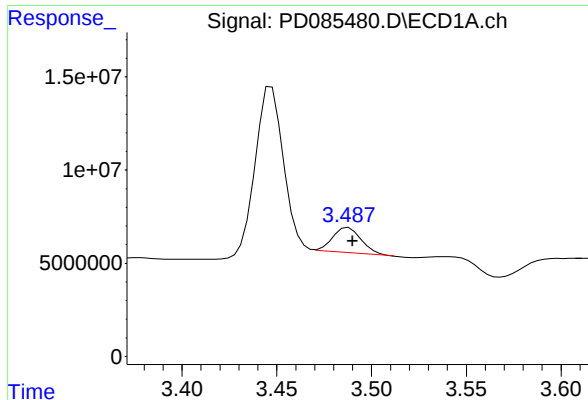

#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.003 min
Response: 13973694
Conc: 11.54 ng/ml

Instrument :

ECD_D


ClientSampleId :

DDCD2

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

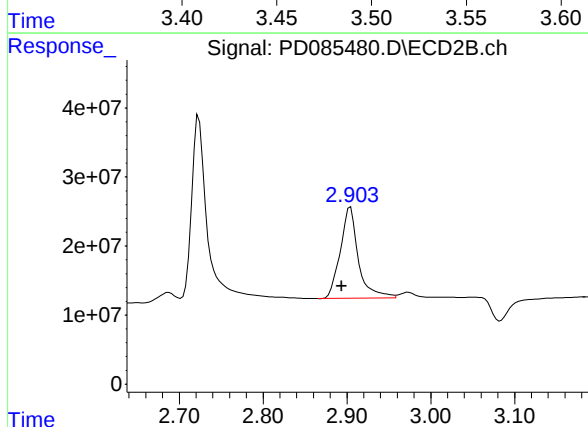


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: 0.010 min
Response: 197894931
Conc: 52.36 ng/ml

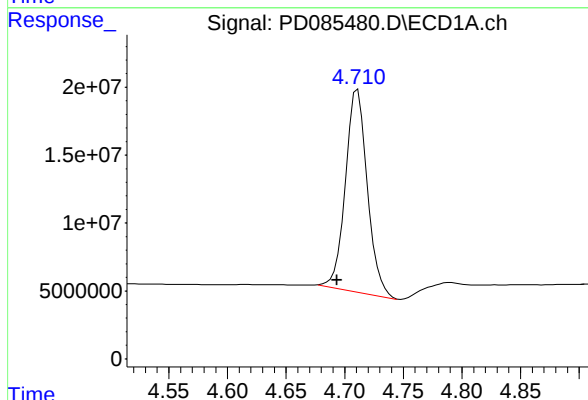


#7 delta-BHC

R.T.: 4.710 min
Delta R.T.: 0.016 min
Response: 193467024
Conc: 84.87 ng/ml m

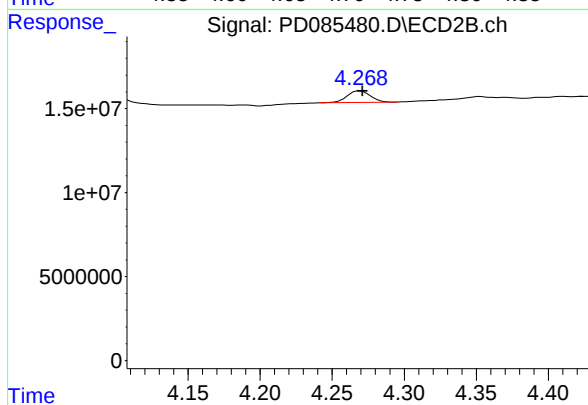

#7 delta-BHC

R.T.: 4.270 min
Delta R.T.: -0.001 min
Response: 7717314
Conc: 1.47 ng/ml

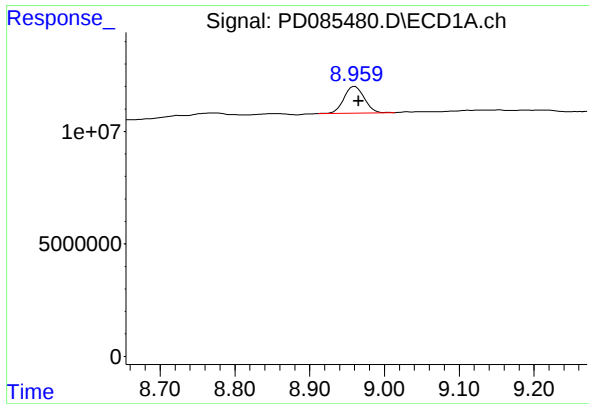


#27 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.005 min
Response: 22435798
Conc: 13.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
DDCD2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

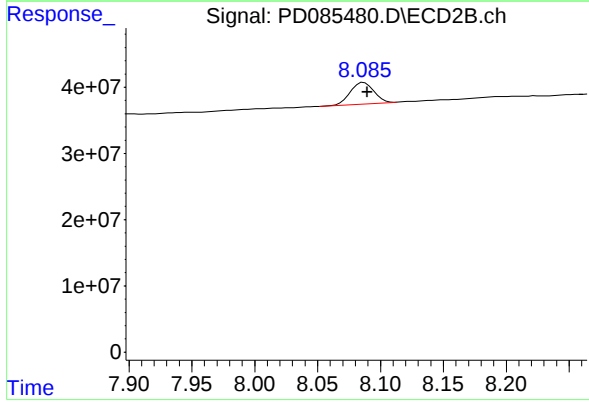

#27 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 42761615
Conc: 16.00 ng/ml