

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
 Data File : PD071959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 14:21
 Operator : AR\AJ
 Sample : N4595-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8G9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/20/2022
 Supervised By :Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 23:21:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.563	35778296	291.0E6	13.719m	8.881 #
2)	SA Decachlor...	7.995	9.087	40716193	144.6E6	15.516	15.127
Target Compounds							
16)	A 4,4'-DDD	5.840	6.737	8702886	45177417	3.306m	3.692m
18)	B Endrin al...	6.166	6.956	4130428	23316345	1.786m	2.285 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
Data File : PD071959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 14:21
Operator : AR\AJ
Sample : N4595-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 23:21:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

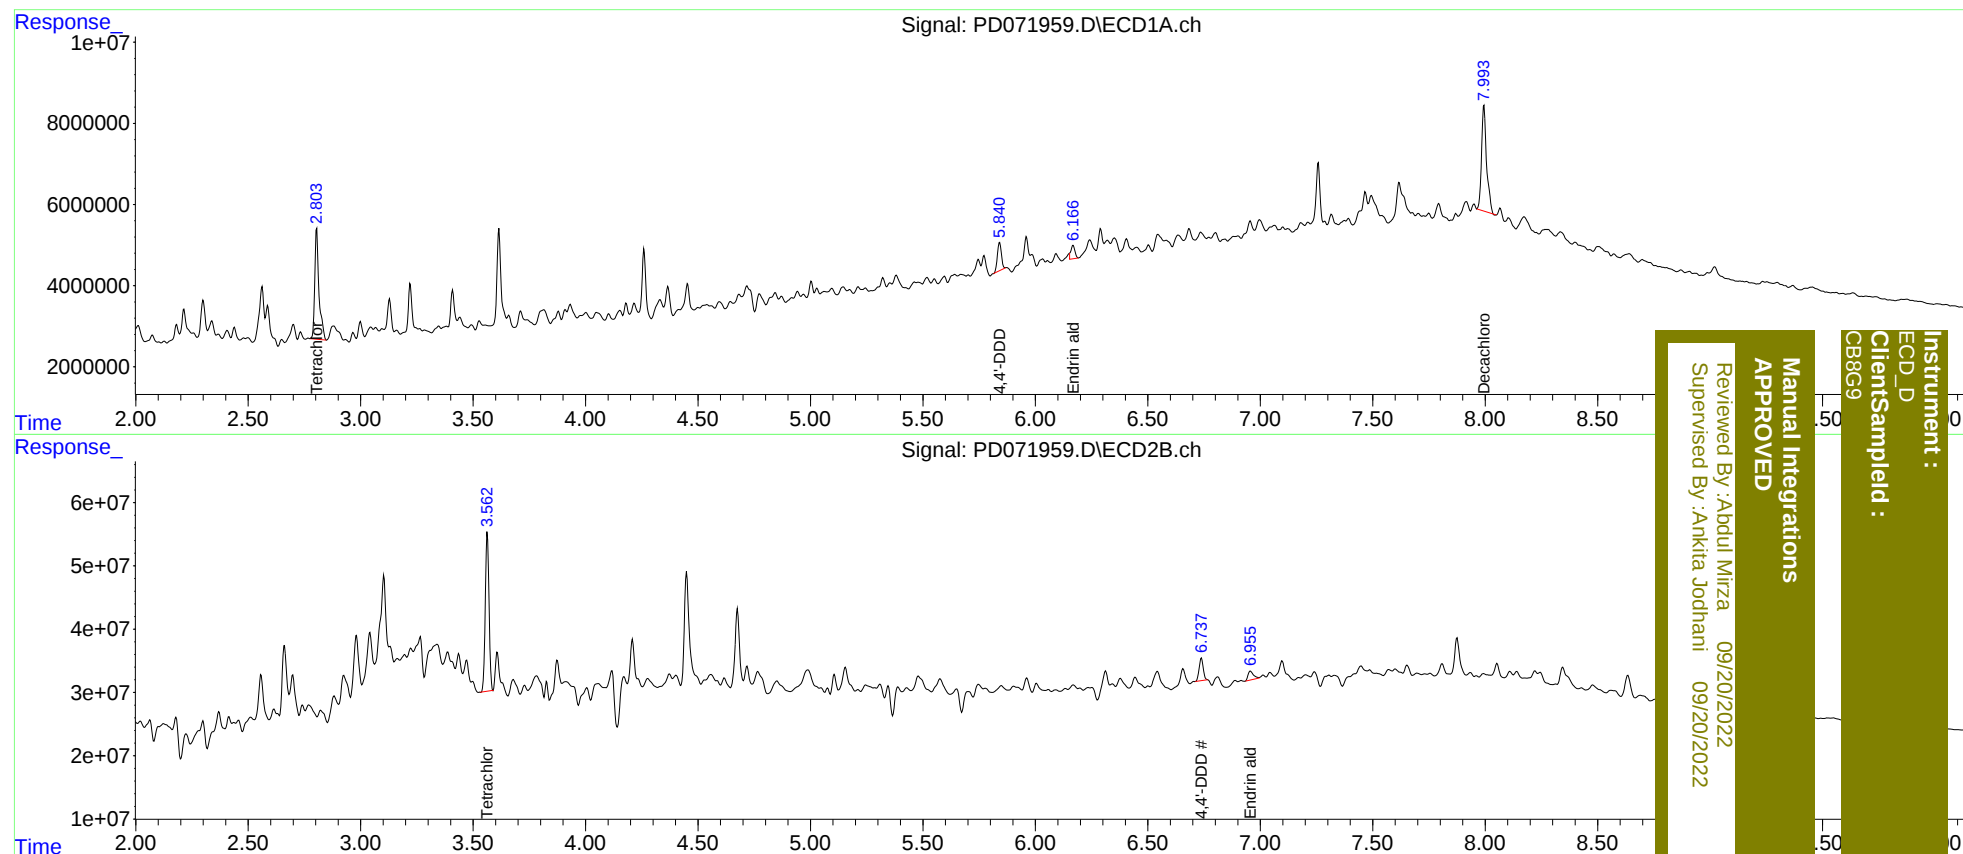

Reviewed By: Abdul Mirza 09/20/2022
Supervised By: Ankita Jodhani 09/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CB8G9