

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
 Data File : PD071965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 15:42
 Operator : AR\AJ
 Sample : N4595-10MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8J0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/20/2022
 Supervised By : Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 23:22:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.564	32637790	430.7E6	12.515m	13.144
27)	SA Decachlor...	7.995	9.089	50184436	209.2E6	19.124	21.888
Target Compounds							
2)	A alpha-BHC	3.313	4.030	153.7E6	1606.3E6	39.847	36.408
3)	MA gamma-BHC...	3.646	4.365	147.0E6	1355.8E6	39.830	36.453
4)	MA Heptachlor	3.992	4.943	133.6E6	895.9E6	35.091	33.180
5)	MB Aldrin	4.275	5.285	133.4E6	768.6E6	37.487	35.577
6)	B beta-BHC	3.945	4.572	59451935	537.6E6	37.426	37.560
7)	B delta-BHC	4.178	4.819	142.7E6	857.0E6	40.847	32.605m
8)	B Heptachlo...	4.782	5.716	123.3E6	595.0E6	37.840	35.187
9)	A Endosulfan I	5.155	6.104	113.0E6	572.1E6	35.869	36.426
10)	B trans-Chl...	5.035	5.971	123.9E6	615.3E6	36.594	36.347
11)	B cis-Chlor...	5.100	6.048	121.7E6	602.5E6	36.495	36.962
12)	B 4,4'-DDE	5.290	6.222	236.8E6	1119.3E6	77.206	76.707
13)	MA Dieldrin	5.423	6.381	200.6E6	1193.2E6	57.915	74.556 #
14)	MA Endrin	5.700	6.615	229.3E6	1019.9E6	76.558	77.520
15)	B Endosulfa...	5.995	6.840	214.3E6	996.6E6	80.624	82.674
16)	A 4,4'-DDD	5.848	6.746	192.2E6	921.3E6	73.035	75.292
17)	MA 4,4'-DDT	6.102	7.057	209.8E6	966.5E6	77.080	80.102
18)	B Endrin al...	6.176	6.971	169.8E6	786.9E6	73.393	77.124
19)	B Endosulfa...	6.400	7.204	197.3E6	886.4E6	74.057	78.055
20)	A Methoxychlor	6.682	7.534	525.3E6	2130.0E6	365.707	388.197
21)	B Endrin ke...	6.909	7.696	239.5E6	1019.2E6	80.033m	82.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
Data File : PD071965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 15:42
Operator : AR\AJ
Sample : N4595-10MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 23:22:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

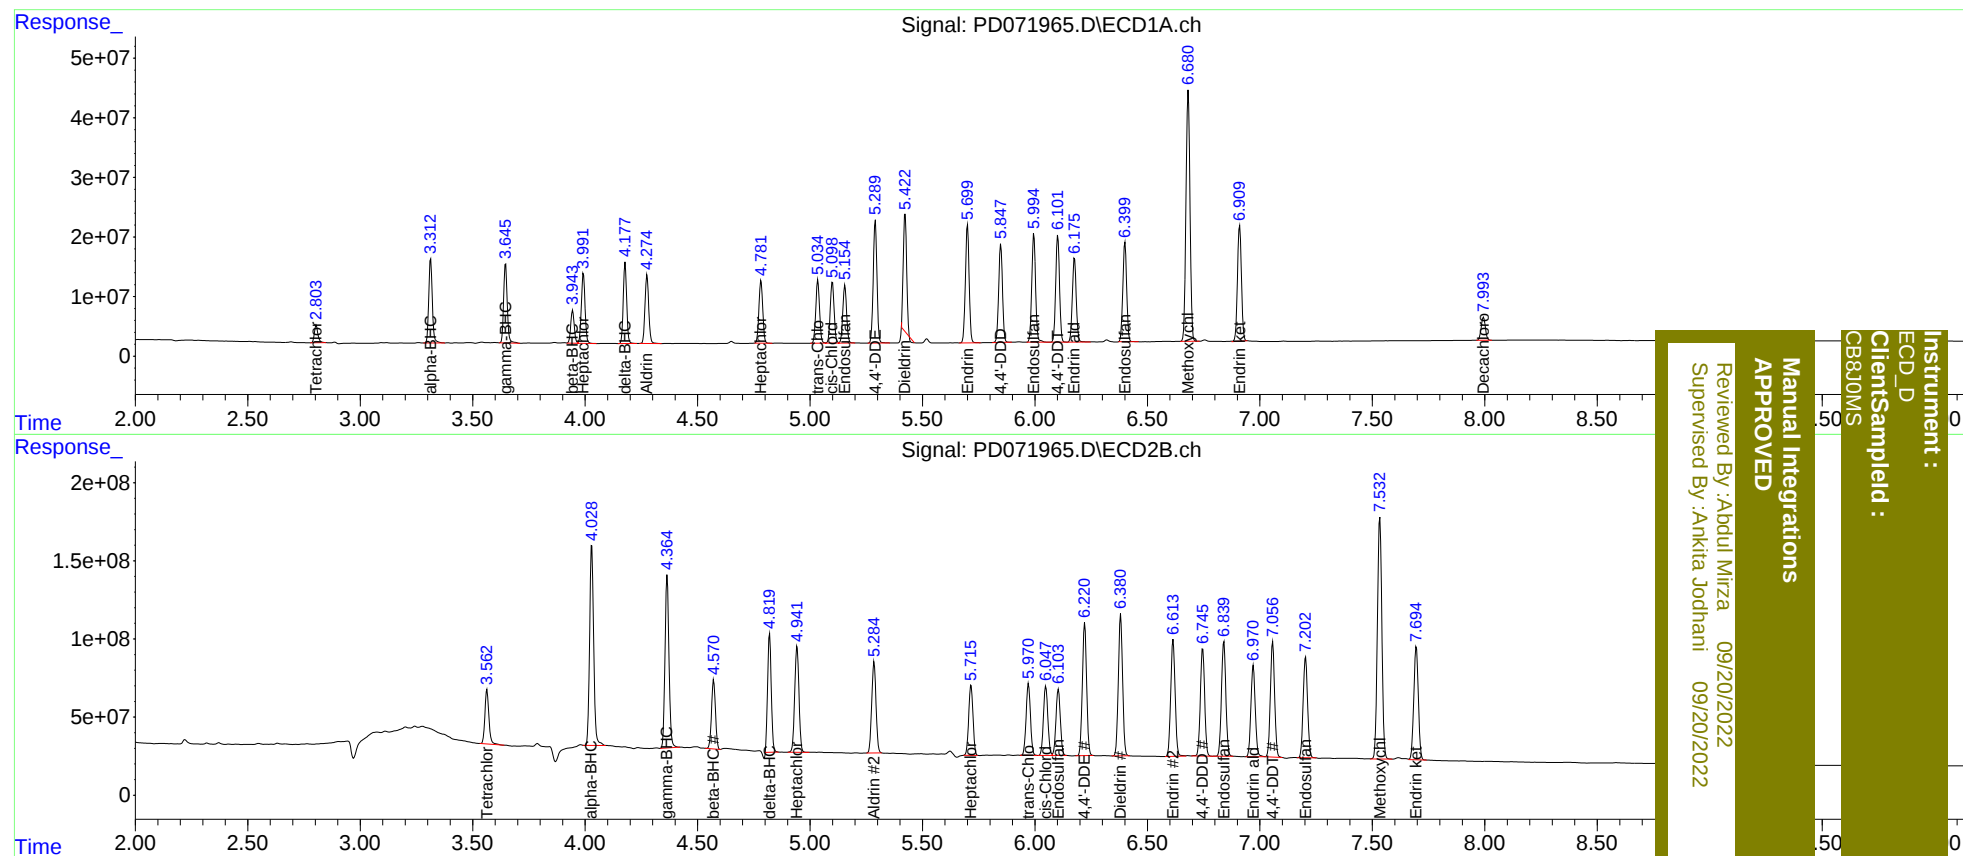

Reviewed By: Abdul Mirza 09/20/2022
Supervised By: Ankita Jodhani 09/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
CB8J0MS