

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
 Data File : PD071967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 16:08
 Operator : AR\AJ
 Sample : PB147721BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS721

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/20/2022
 Supervised By :Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 23:22:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.564	49435221	643.3E6	18.956m	19.631
27)	SA Decachlor...	7.995	9.090	90895396	367.3E6	34.637	38.423
Target Compounds							
2)	A alpha-BHC	3.313	4.030	17996975	226.9E6	4.666	5.143
3)	MA gamma-BHC...	3.647	4.365	17988627	210.1E6	4.872	5.648
4)	MA Heptachlor	3.992	4.943	17660412	156.7E6	4.640	5.803 #
5)	MB Aldrin	4.276	5.285	18049418	133.5E6	5.070	6.179
6)	B beta-BHC	3.945	4.572	8546422	82596324	5.380	5.771
7)	B delta-BHC	4.178	4.819	15076543	140.7E6	4.315	5.355m
8)	B Heptachlo...	4.782	5.717	16878421	105.2E6	5.178	6.222
9)	A Endosulfan I	5.156	6.105	15503211	92069685	4.919	5.862
10)	B trans-Chl...	5.035	5.972	17137865	102.6E6	5.062	6.062
11)	B cis-Chlor...	5.100	6.049	16991567	100.1E6	5.094	6.140
12)	B 4,4'-DDE	5.290	6.222	30266800	178.4E6	9.868	12.223
13)	MA Dieldrin	5.422	6.382	33410603	189.0E6	9.648m	11.812
14)	MA Endrin	5.701	6.614	29466694	155.0E6	9.839	11.782
15)	B Endosulfa...	5.996	6.840	28263449	151.8E6	10.633	12.592
16)	A 4,4'-DDD	5.849	6.746	25730712	144.2E6	9.776	11.785
17)	MA 4,4'-DDT	6.103	7.057	25569983	144.3E6	9.393	11.961 #
18)	B Endrin al...	6.176	6.971	22276567	114.9E6	9.630	11.265
19)	B Endosulfa...	6.401	7.204	26019334	129.8E6	9.767	11.428
20)	A Methoxychlor	6.682	7.534	76028421	342.5E6	52.934	62.426
21)	B Endrin ke...	6.909	7.696	32157281	154.9E6	10.746m	12.514

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092122\
Data File : PD071967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 16:08
Operator : AR\AJ
Sample : PB147721BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 23:22:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

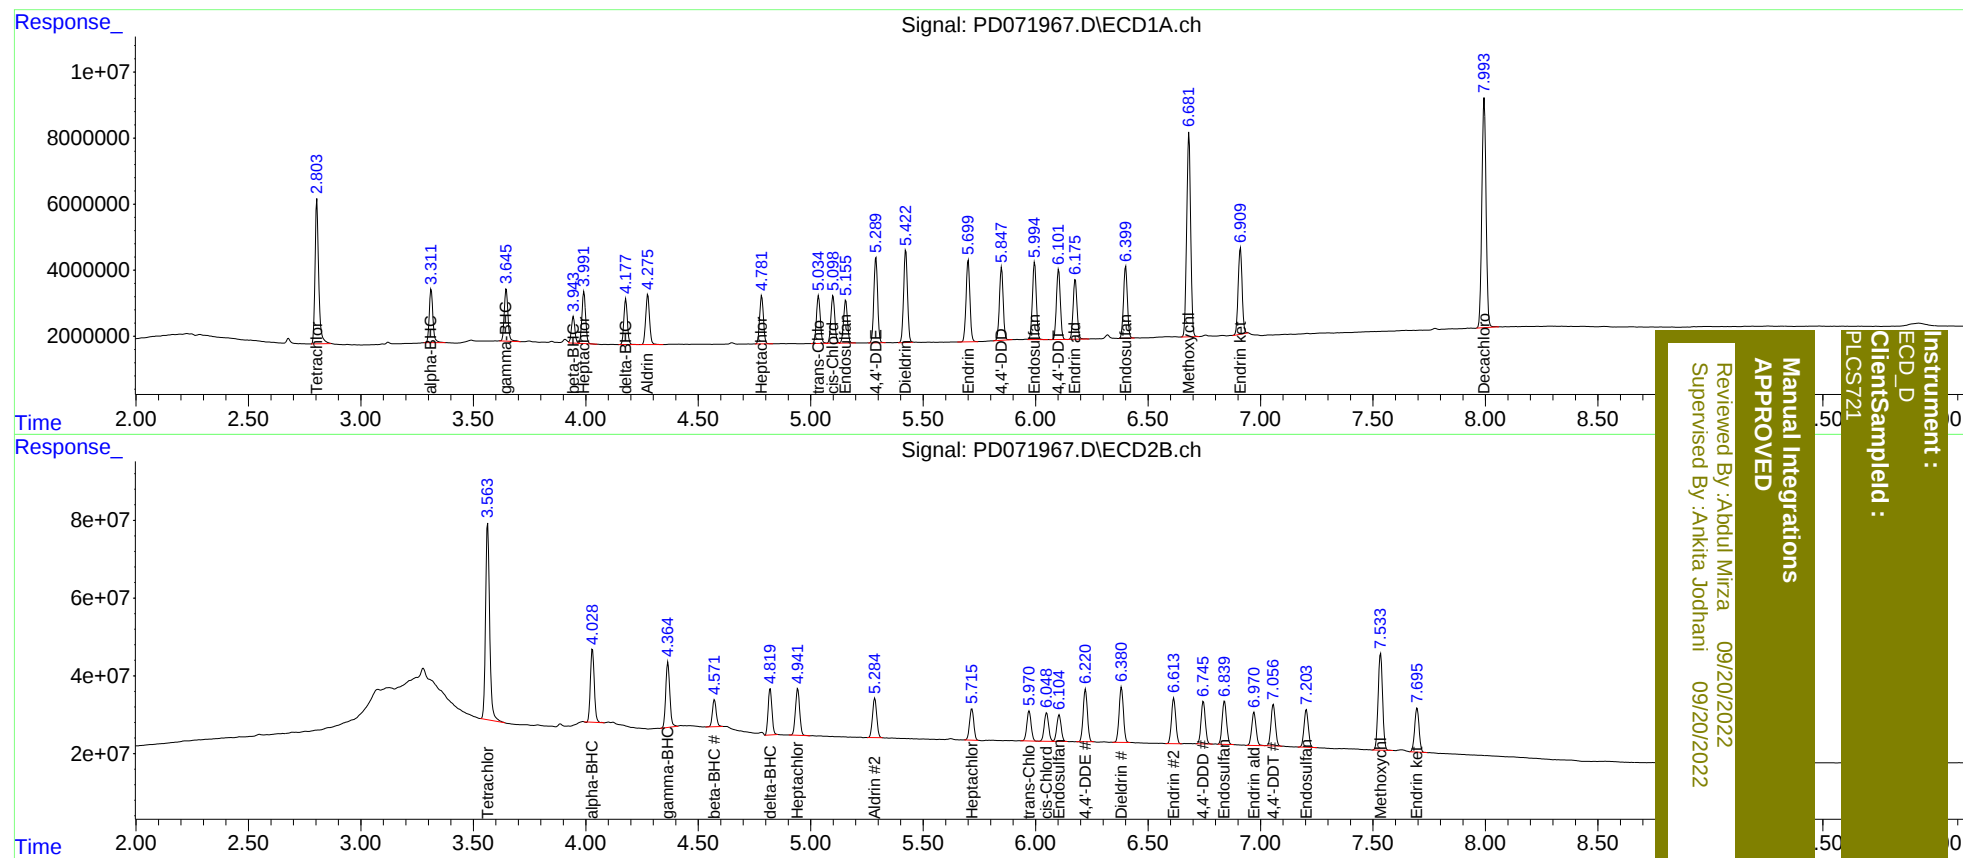

Instrument :
ECD_D
ClientSampled :
PLC5721

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/20/2022
Supervised By :Ankita Jodhani 09/20/2022