

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
 Data File : PD078150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 15:04
 Operator : AR\AJ
 Sample : 04450-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:26:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	57148863	35459893	22.520	23.994
27)	SA Decachlor...	9.083	7.898	66934038	34681745	21.426	21.415
Target Compounds							
3)	MA gamma-BHC...	0.000	3.639f	0	64652	N.D.	<MDL
6)	B beta-BHC	0.000	3.846f	0	909431	N.D.	0.920
7)	B delta-BHC	4.770	0.000	2134268	0	0.532	N.D. #
15)	B Endosulfa...	0.000	5.874f	0	532944	N.D.	0.294


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
Data File : PD078150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 15:04
Operator : AR\AJ
Sample : 04450-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:26:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

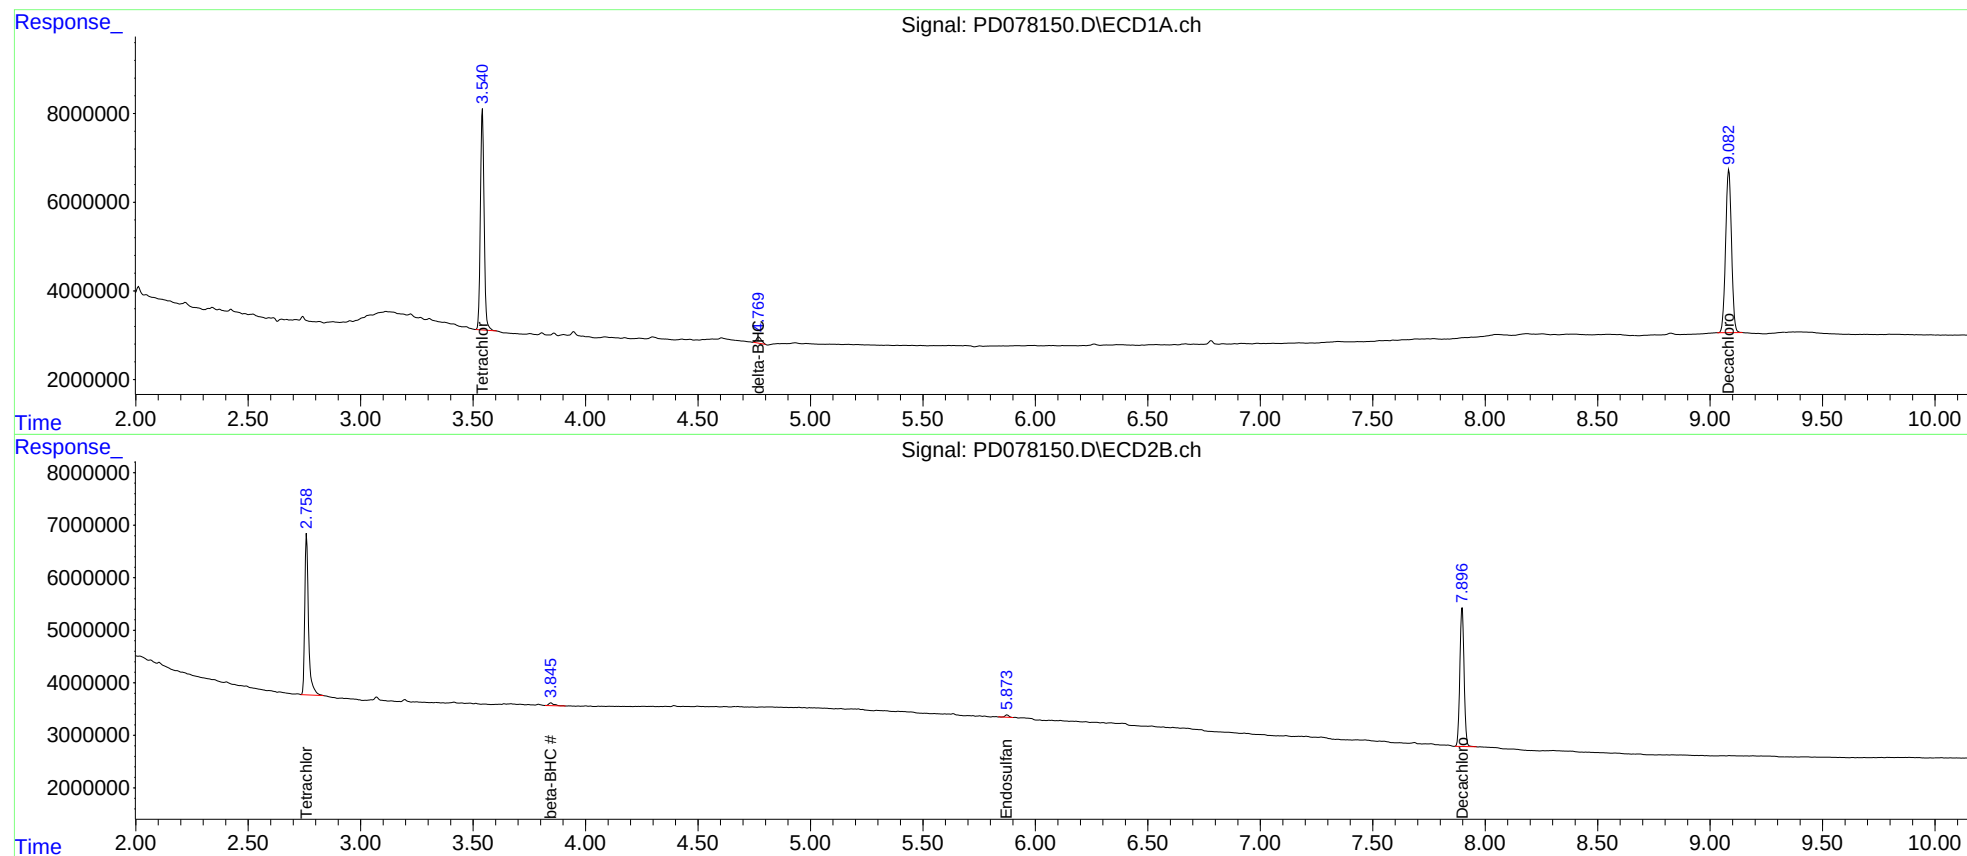

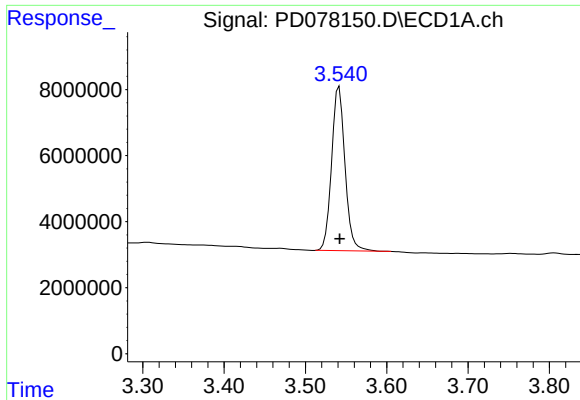


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 57148863
Conc: 22.52 ng/ml

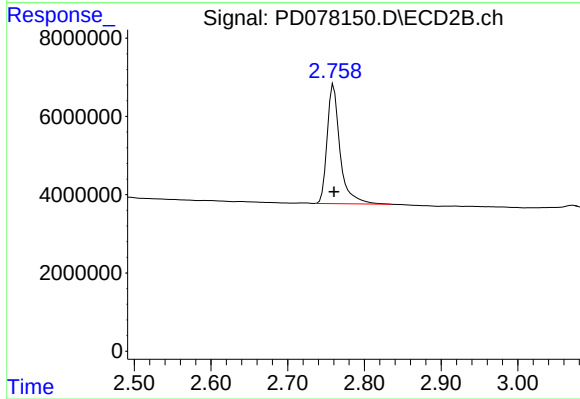


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 35459893
Conc: 23.99 ng/ml

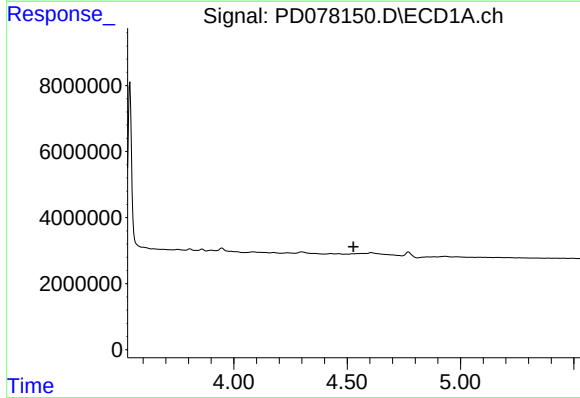


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

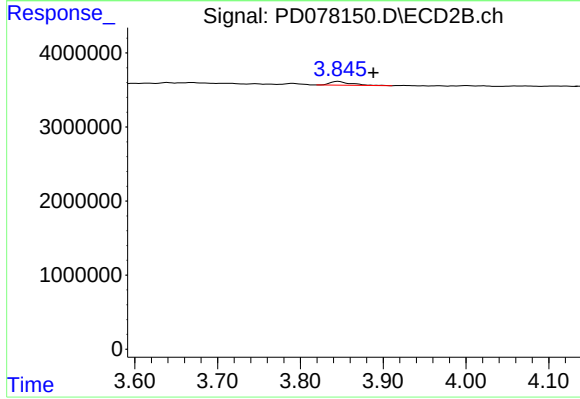


#6 beta-BHC

R.T.: 3.846 min
Delta R.T.: -0.042 min
Response: 909431
Conc: 0.92 ng/ml

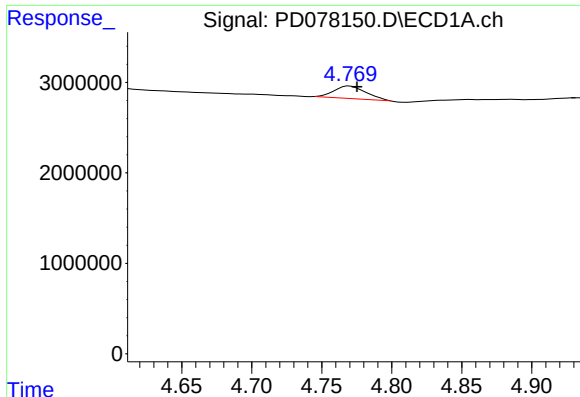


#7 delta-BHC

R.T.: 4.770 min
Delta R.T.: -0.005 min
Response: 2134268
Conc: 0.53 ng/ml

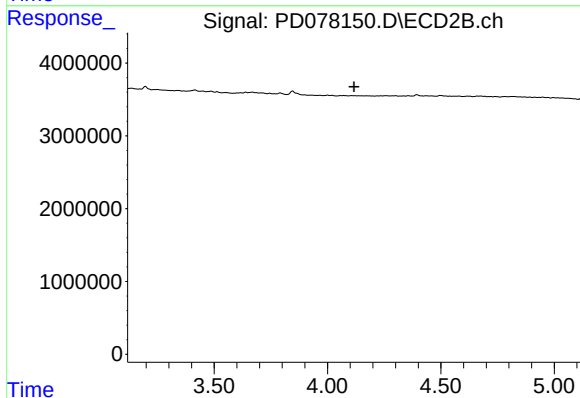


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.118 min
Response: 0
Conc: N.D.

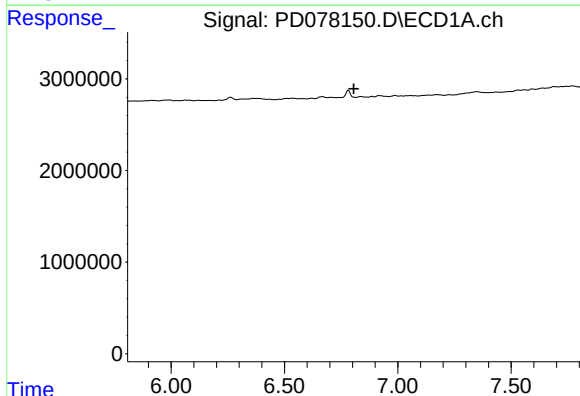


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.806 min
Response: 0
Conc: N.D.

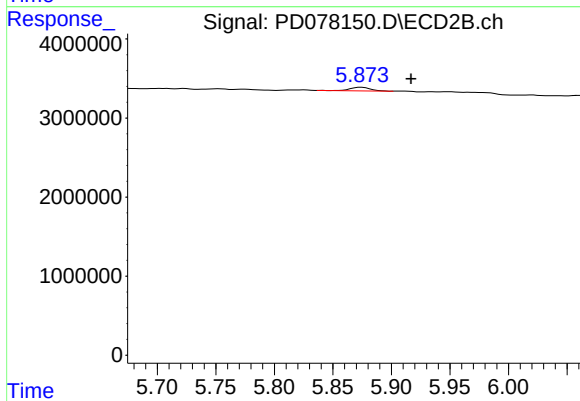


#15 Endosulfan II

R.T.: 5.874 min
Delta R.T.: -0.043 min
Response: 532944
Conc: 0.29 ng/ml

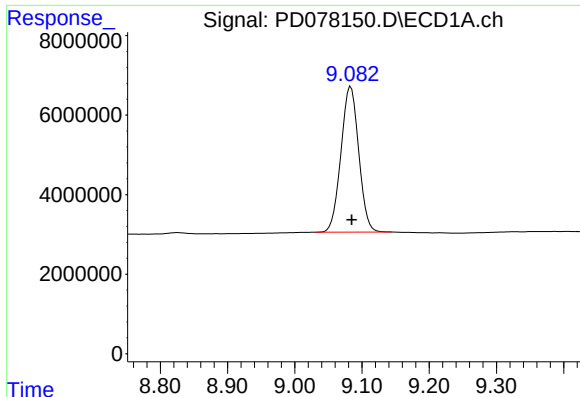

#27 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 66934038
Conc: 21.43 ng/ml

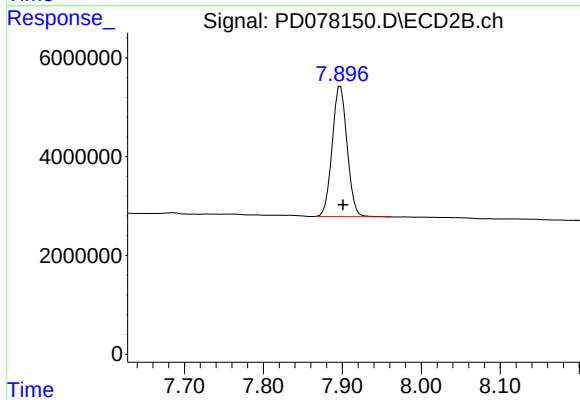

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 34681745
Conc: 21.41 ng/ml