

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
 Data File : PD078168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 19:23
 Operator : AR\AJ
 Sample : 04417-12MS
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYM9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/21/2023
 Supervised By : Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:41:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.759	23360732	20977785	9.205m	14.195m#
27)	SA Decachlor...	9.075	7.898	61808437	29510947	19.786	18.222
Target Compounds							
2)	A alpha-BHC	3.998	3.258	63914754	39413109	14.927	17.388m
3)	MA gamma-BHC...	4.331	3.593	65459884	65103145	16.190	30.153 #
4)	MA Heptachlor	4.920	3.931	58404699	41681127	13.976m	18.748 #
5)	MB Aldrin	5.276	4.212	309.3E6	60356885	74.085	26.928 #
6)	B beta-BHC	4.529	3.888	21879891	13381369	11.910	13.543
7)	B delta-BHC	4.777	4.118	66353838	36739173	16.525	16.482
8)	B Heptachlo...	5.686	4.711	256.5E6	40232888	66.366m	19.154 #
9)	A Endosulfan I	6.080	5.073	82802196	107.5E6	24.668	59.915 #
10)	B trans-Chl...	5.942	4.958	171.9E6	20325865	46.164m	10.179m#
11)	B cis-Chlor...	6.028	5.024	81433395	34489280	21.129	16.865
12)	B 4,4'-DDE	6.200	5.214	213.2E6	58174435	60.149m	30.624 #
13)	MA Dieldrin	6.353	5.347	531.7E6	139.5E6	142.059	67.504 #
14)	MA Endrin	6.586	5.625	231.0E6	126.4E6	74.857	69.109
15)	B Endosulfa...	6.804	5.913	344.0E6	91956147	103.882	50.813 #
16)	A 4,4'-DDD	6.728	5.769	1010.4E6	65497197	379.861	48.662 #
17)	MA 4,4'-DDT	7.005	6.013	1130.3E6	580.4E6	412.548m	410.686m
18)	B Endrin al...	6.938	6.112	149.9E6	166.9E6	57.702m	118.679m#
19)	B Endosulfa...	7.149	6.315	605.4E6	331.6E6	199.777m	200.693
20)	A Methoxychlor	7.510	6.591	306.5E6	69188658	196.543	88.668m#
21)	B Endrin ke...	7.650	6.825	143.4E6	51897669	41.640m	27.087 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
Data File : PD078168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 19:23
Operator : AR\AJ
Sample : 04417-12MS
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:41:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

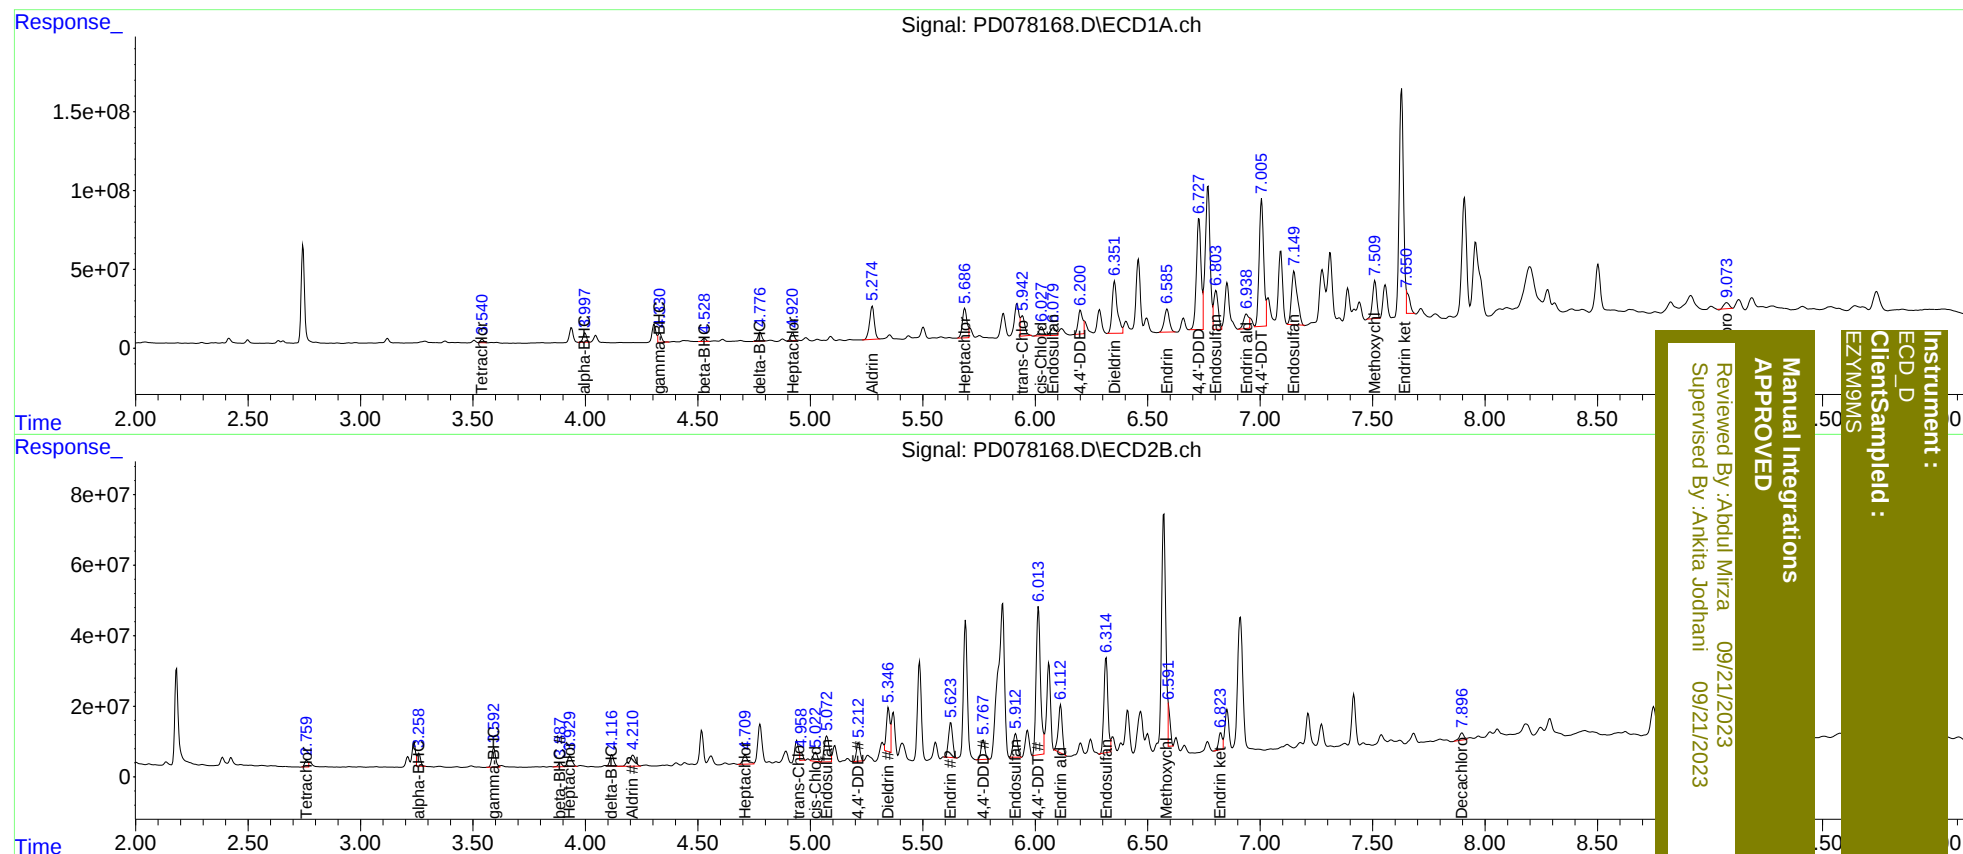

Instrument :
ECD_D
ClientSampled :
EZYM9MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 09/21/2023
Supervised By: Ankita Jodhani 09/21/2023