

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
 Data File : PD078166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 18:57
 Operator : AR\AJ
 Sample : 04417-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYF5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:39:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.759	35211345	23761232	13.875	16.078
2)	SA Decachlor...	9.080	7.897	22678604	15809468	7.260	9.762 #
Target Compounds							
7)	B delta-BHC	4.775	4.124	4640961	4075375	1.156	1.828 #
14)	MA Endrin	6.582	5.626	242.8E6	372.2E6	78.687	203.588m#
15)	B Endosulfa...	6.798	5.907	424.2E6	137.6E6	128.115	76.032 #
17)	MA 4,4'-DDT	7.004	6.012	2443.0E6	1288.7E6	891.674m	911.826m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
Data File : PD078166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 18:57
Operator : AR\AJ
Sample : 04417-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:39:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

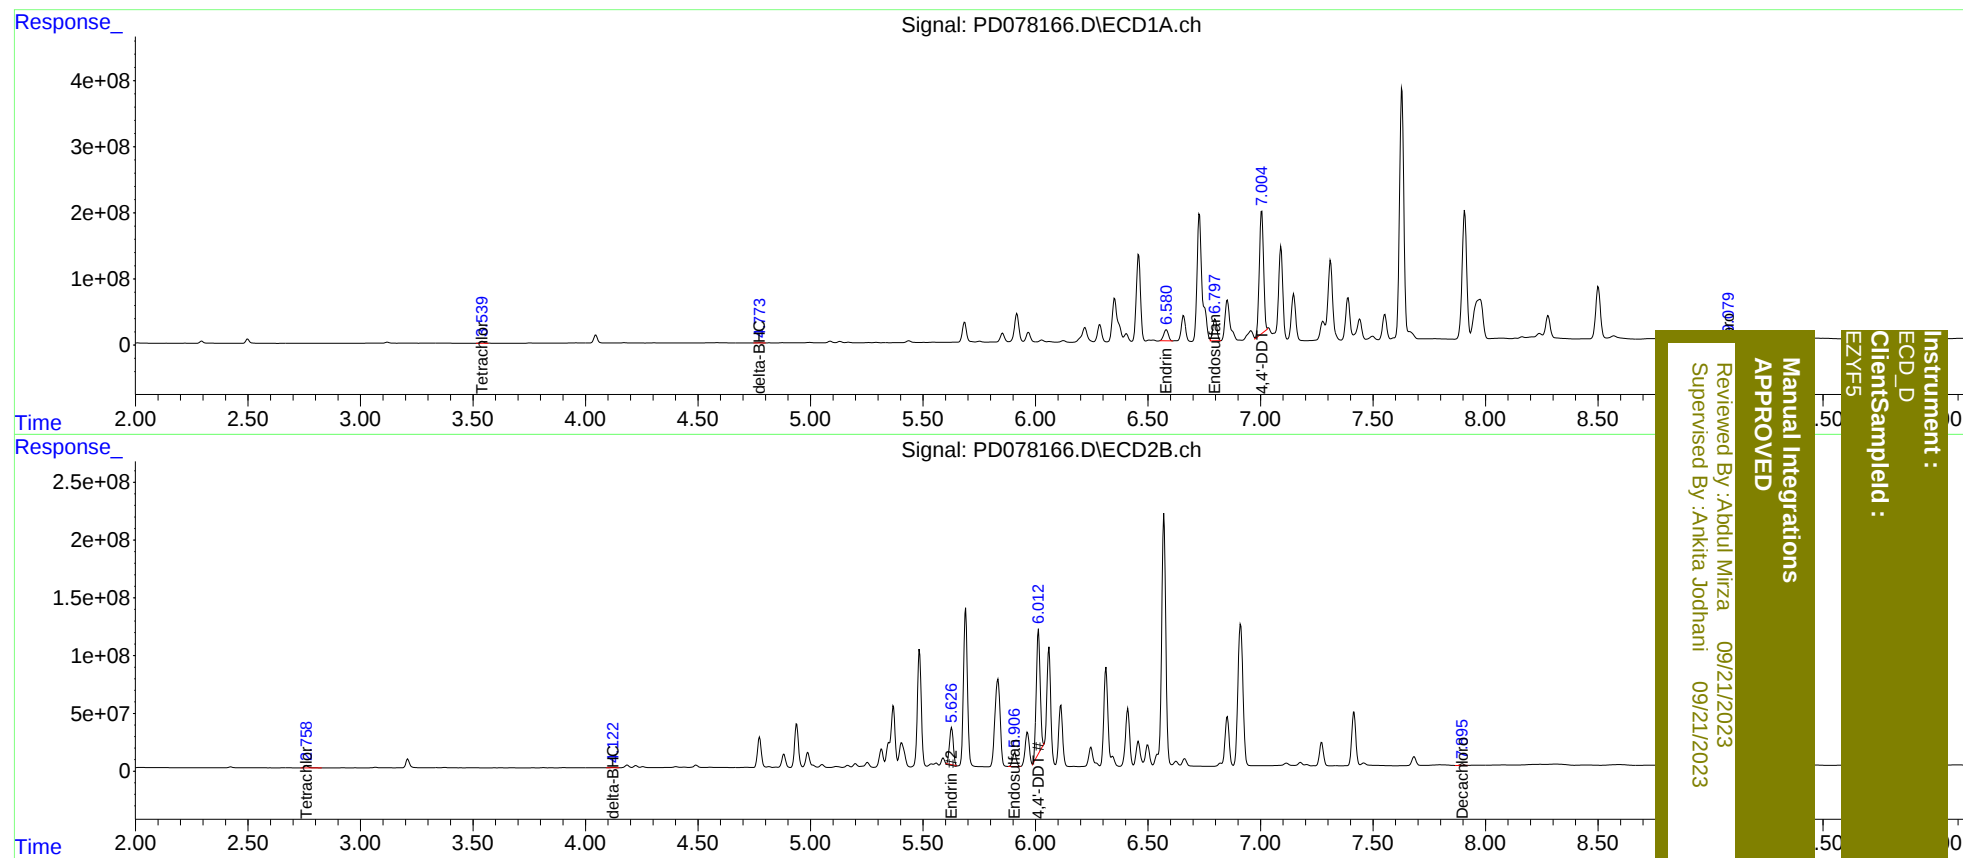

Instrument :
ECD_D
ClientSampled :
EZYF5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023