

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
 Data File : PD078169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 19:37
 Operator : AR\AJ
 Sample : 04417-13MSD
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYM9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/21/2023
 Supervised By : Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:42:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.759	24003391	18775597	9.459m	12.704m#
27)	SA Decachlor...	9.074	7.898	51748423	28492654	16.565	17.593
Target Compounds							
2)	A alpha-BHC	3.998	3.258	64161031	35426105	14.985	15.629m
3)	MA gamma-BHC...	4.330	3.593	63014235	65132845	15.585	30.167 #
4)	MA Heptachlor	4.920	3.930	60246584	40935278	14.417m	18.412 #
5)	MB Aldrin	5.276	4.211	306.3E6	58912755	73.361	26.284 #
6)	B beta-BHC	4.529	3.888	21474149	12677435	11.689	12.830
7)	B delta-BHC	4.777	4.118	65469441	36164721	16.305	16.224
8)	B Heptachlo...	5.685	4.711	253.6E6	39406082	65.612m	18.761 #
9)	A Endosulfan I	6.080	5.074	76936397	107.3E6	22.920	59.763 #
10)	B trans-Chl...	5.942	4.952	165.7E6	19041923	44.515m	9.536m#
11)	B cis-Chlor...	6.028	5.024	79606050	33674904	20.655	16.467
12)	B 4,4'-DDE	6.200	5.214	203.3E6	60168787	57.344m	31.674 #
13)	MA Dieldrin	6.353	5.347	526.7E6	134.5E6	140.705	65.111 #
14)	MA Endrin	6.586	5.624	230.6E6	126.5E6	74.754	69.166
15)	B Endosulfa...	6.804	5.913	335.8E6	90486871	101.401	50.002 #
16)	A 4,4'-DDD	6.729	5.769	986.7E6	64305472	370.960	47.777 #
17)	MA 4,4'-DDT	7.005	6.013	1142.0E6	579.9E6	416.832m	410.332m
18)	B Endrin al...	6.936	6.111	127.4E6	173.5E6	49.021m	123.341m#
19)	B Endosulfa...	7.150	6.315	594.7E6	328.1E6	196.254m	198.560
20)	A Methoxychlor	7.510	6.588	296.7E6	87410693	190.202	112.020m#
21)	B Endrin ke...	7.651	6.824	112.4E6	53191512	32.638m	27.762

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092123\
Data File : PD078169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 19:37
Operator : AR\AJ
Sample : 04417-13MSD
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:42:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

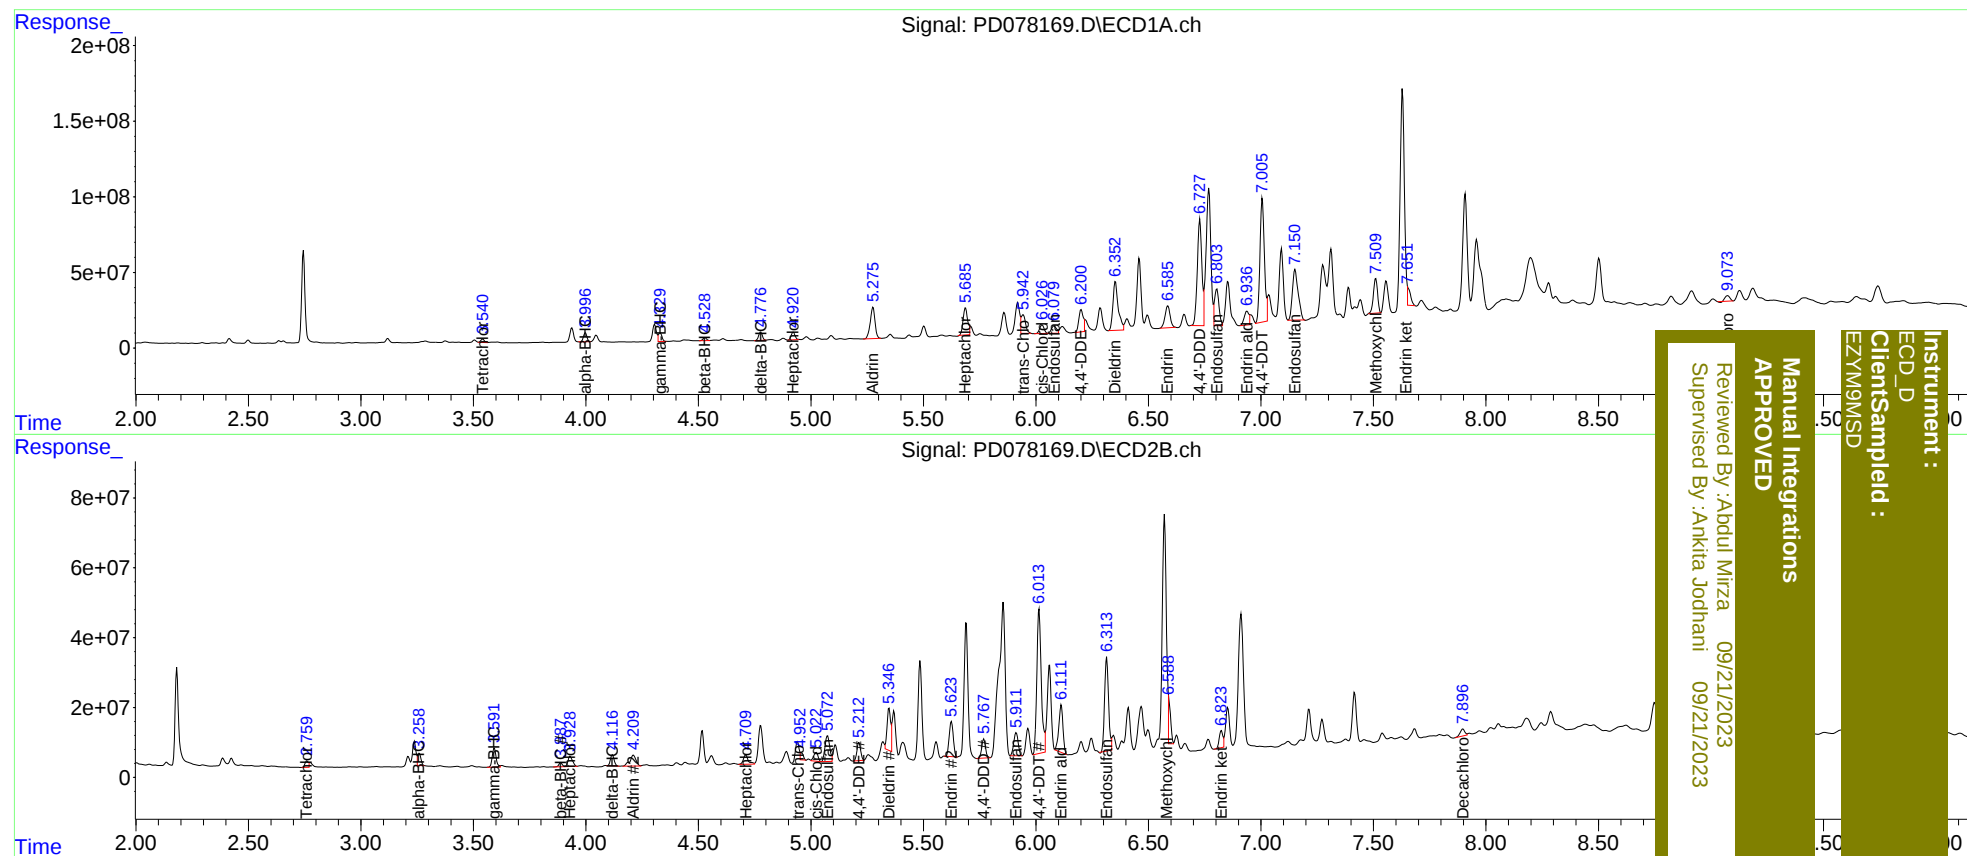

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/21/2023
Supervised By: Ankita Jodhani 09/21/2023

Instrument :
ECD_D
Client Sampled :
EZYM9MSD