

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
 Data File : PD065795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 18:09
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 04:08:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 04:04:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	71246643	438.9E6	74.801	74.348
28)	SA Decachlor...	8.234	9.085	100.5E6	288.2E6	73.348	73.773
Target Compounds							
23)	Chlordane-1	4.362	5.008	23474187	168.9E6	747.564	746.377
24)	Chlordane-2	4.862	5.477	29052004	156.5E6	736.749	737.998
25)	Chlordane-3	5.428	6.125	87227541	582.9E6	740.935	738.602
26)	Chlordane-4	5.486	6.198	73052368	677.0E6	741.656	738.608
27)	Chlordane-5	6.323	7.009	33818046	134.3E6	733.772	737.485



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
Data File : PD065795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 18:09
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 04:08:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 04:04:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

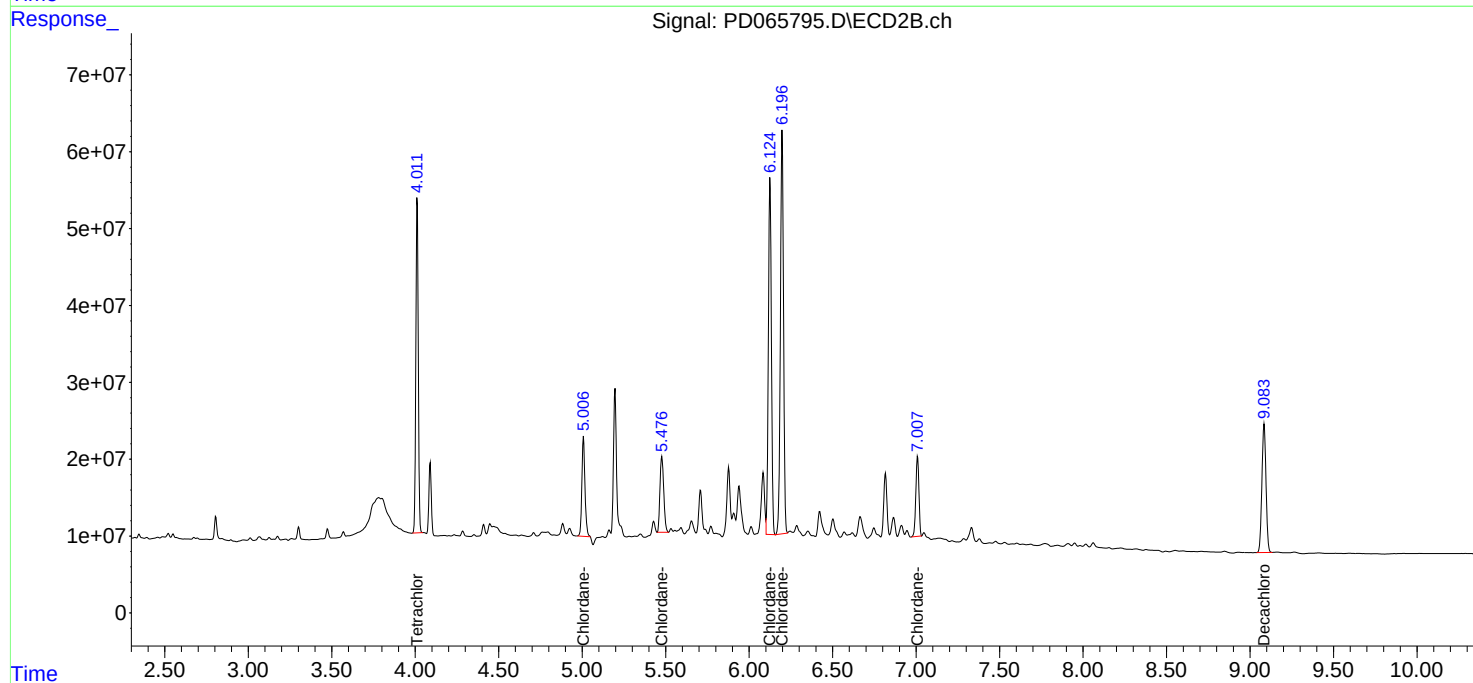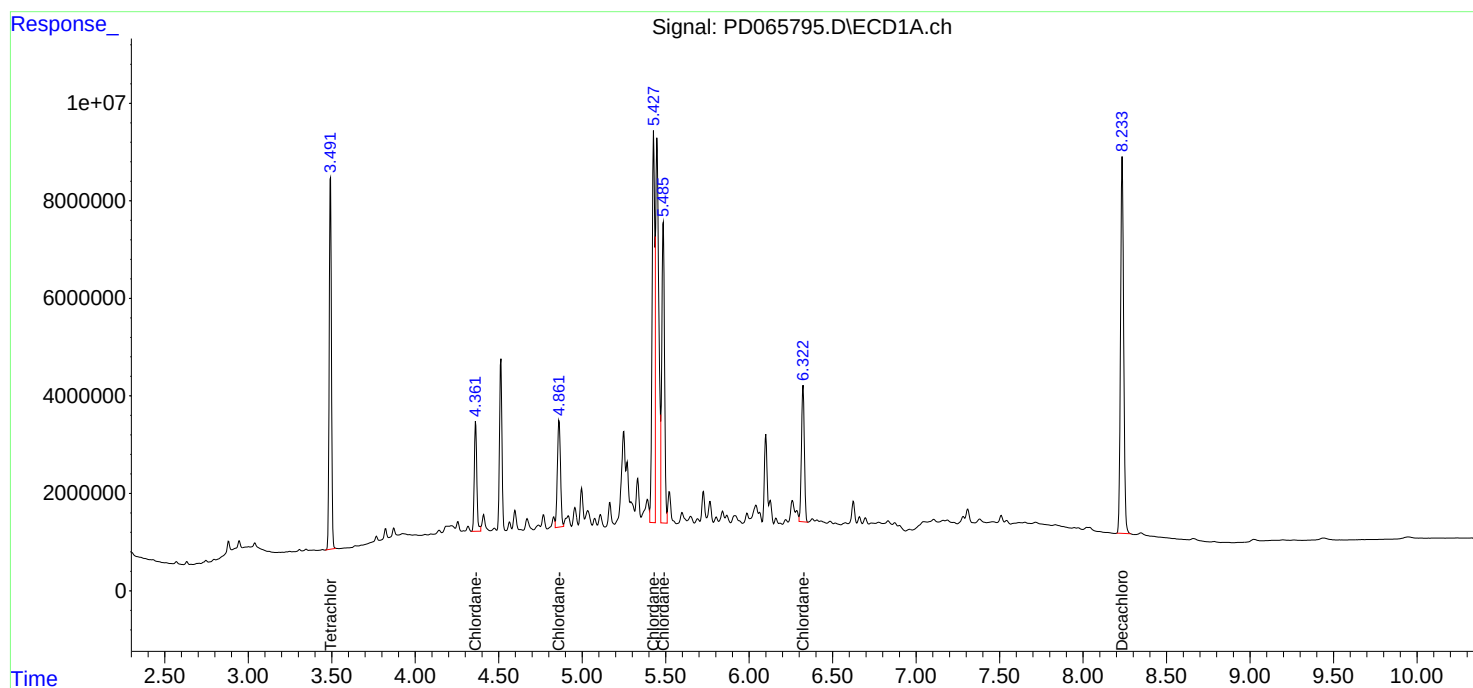


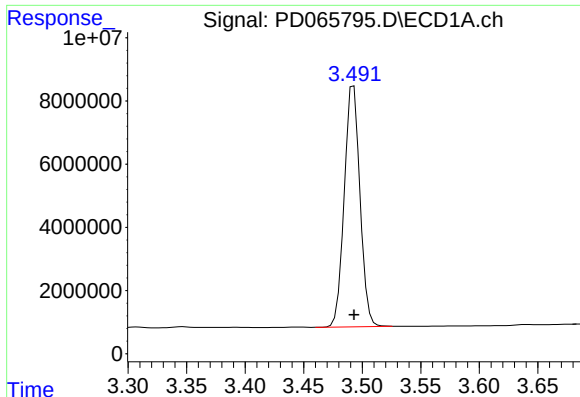

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 71246643
Conc: 74.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

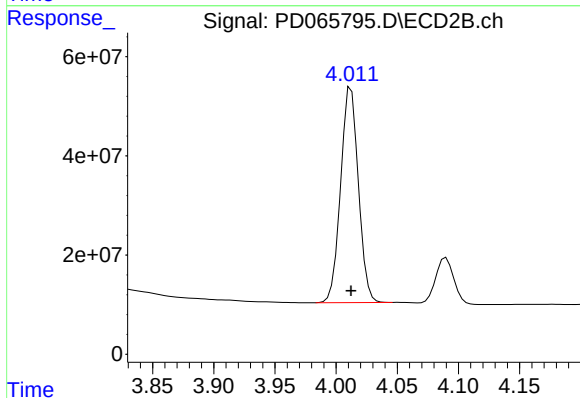


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 438880339
Conc: 74.35 ng/ml

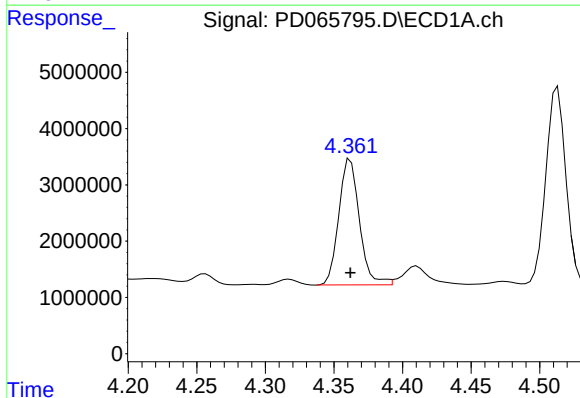


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 23474187
Conc: 747.56 ng/ml

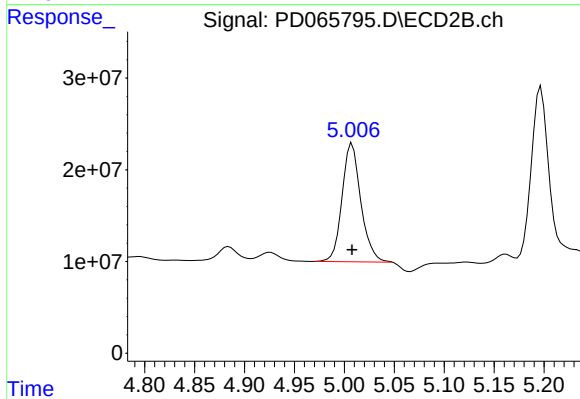

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 168940833
Conc: 746.38 ng/ml

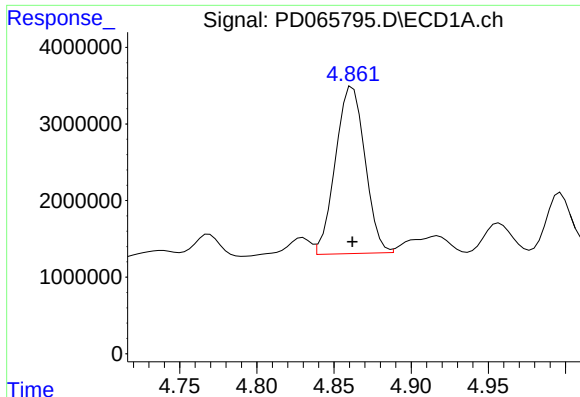

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 29052004
Conc: 736.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

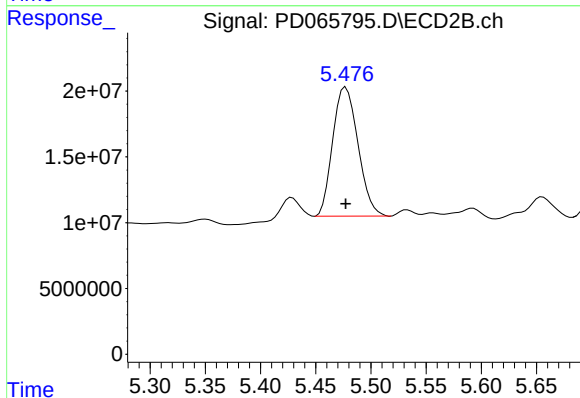


#24 Chlordane-2

R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 156536975
Conc: 738.00 ng/ml

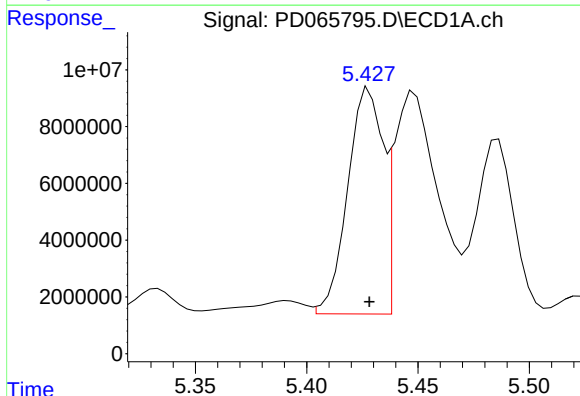


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 87227541
Conc: 740.94 ng/ml

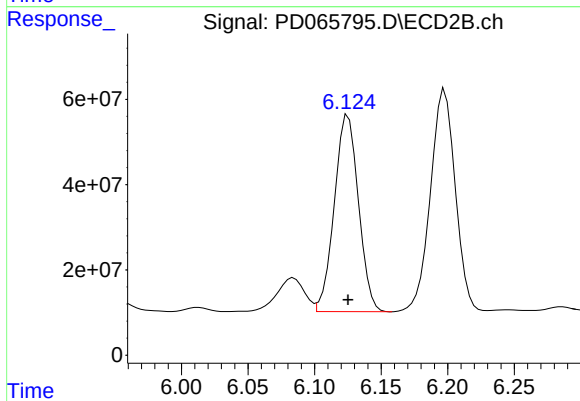

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 582895941
Conc: 738.60 ng/ml

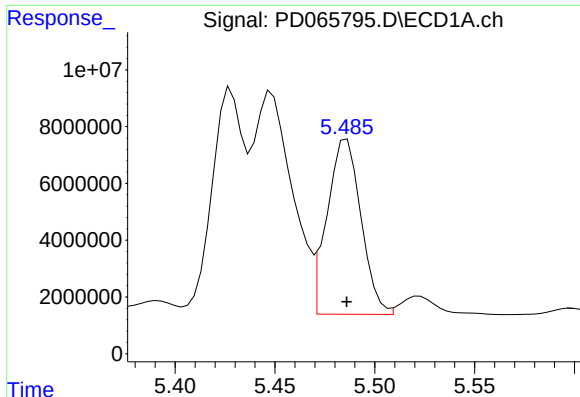

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 73052368
Conc: 741.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

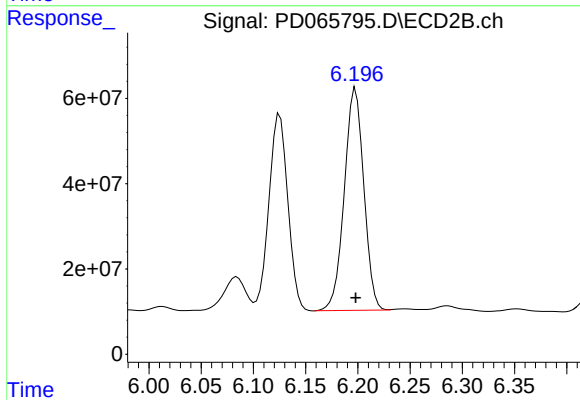


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 677002174
Conc: 738.61 ng/ml

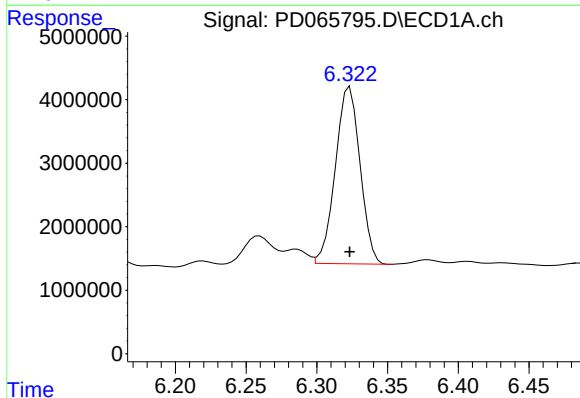


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 33818046
Conc: 733.77 ng/ml

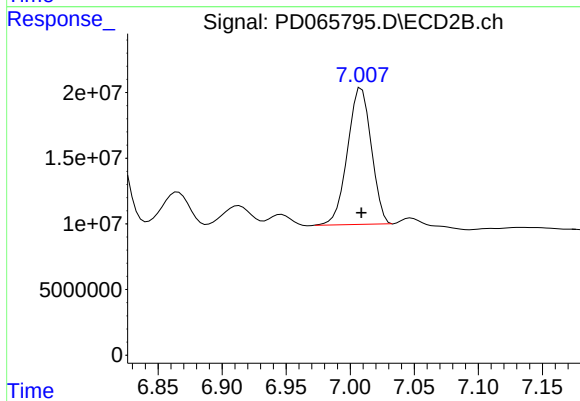

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 134341121
Conc: 737.48 ng/ml

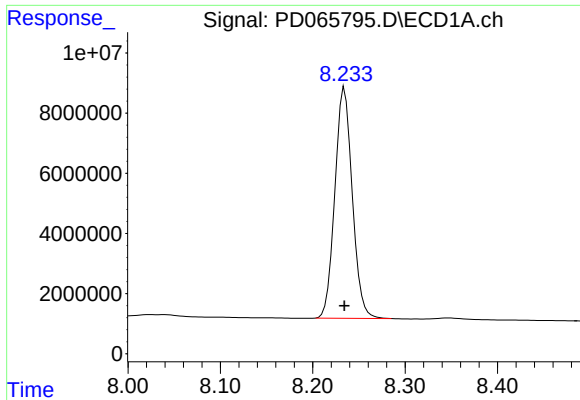

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 100510909
Conc: 73.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

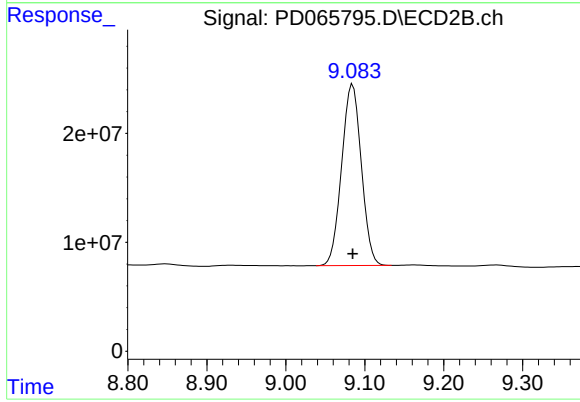

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 288198128
Conc: 73.77 ng/ml