

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
 Data File : PD065797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 18:36
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 04:10:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 04:04:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	4.012	23586475	153.8E6	24.822	25.781
28)	SA Decachlor...	8.235	9.085	37327454	106.2E6	26.643	26.599
Target Compounds							
23)	Chlordane-1	4.362	5.007	8260862	55891086	259.681	247.687
24)	Chlordane-2	4.862	5.478	10772581	58218401	266.998	267.916
25)	Chlordane-3	5.428	6.125	28788183	204.6E6	245.879	256.914
26)	Chlordane-4	5.486	6.198	24404822	241.0E6	248.322	259.582
27)	Chlordane-5	6.323	7.009	12194546	46732956	260.787	254.879



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
Data File : PD065797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 18:36
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 04:10:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 04:04:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

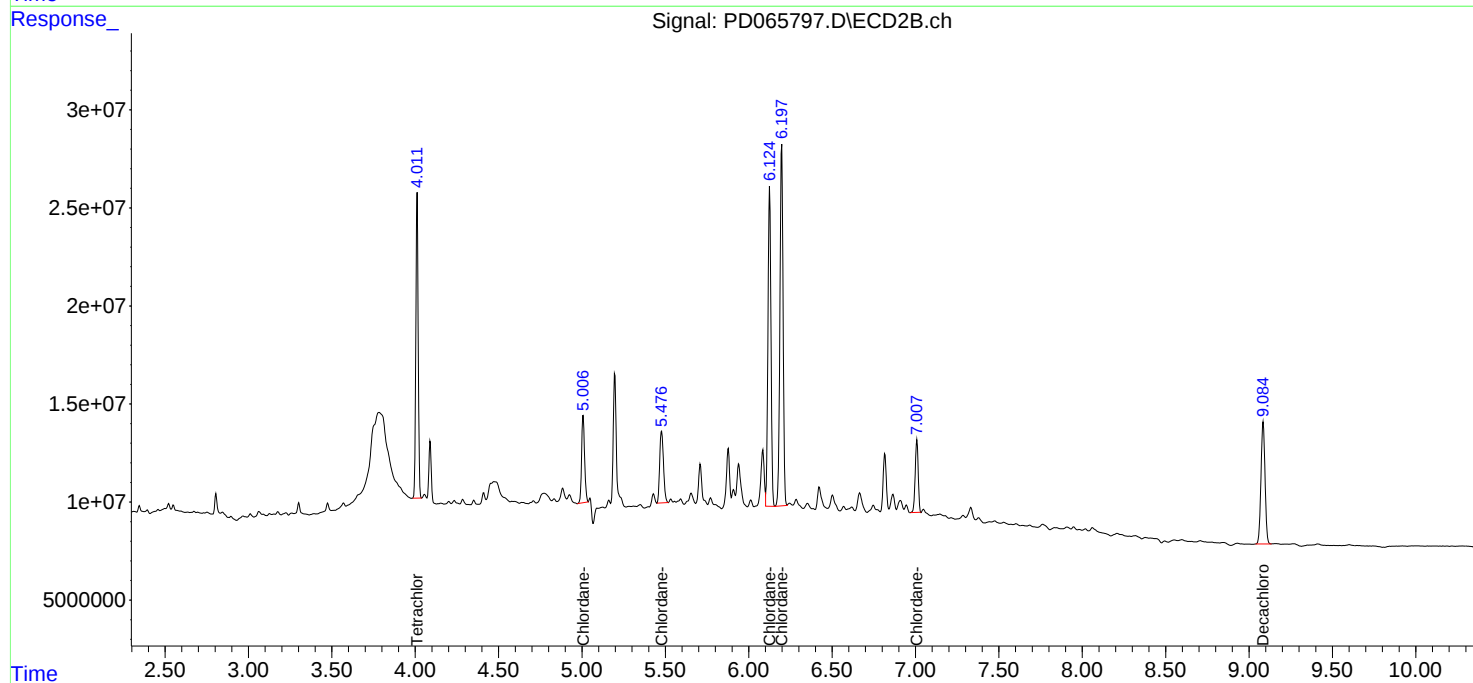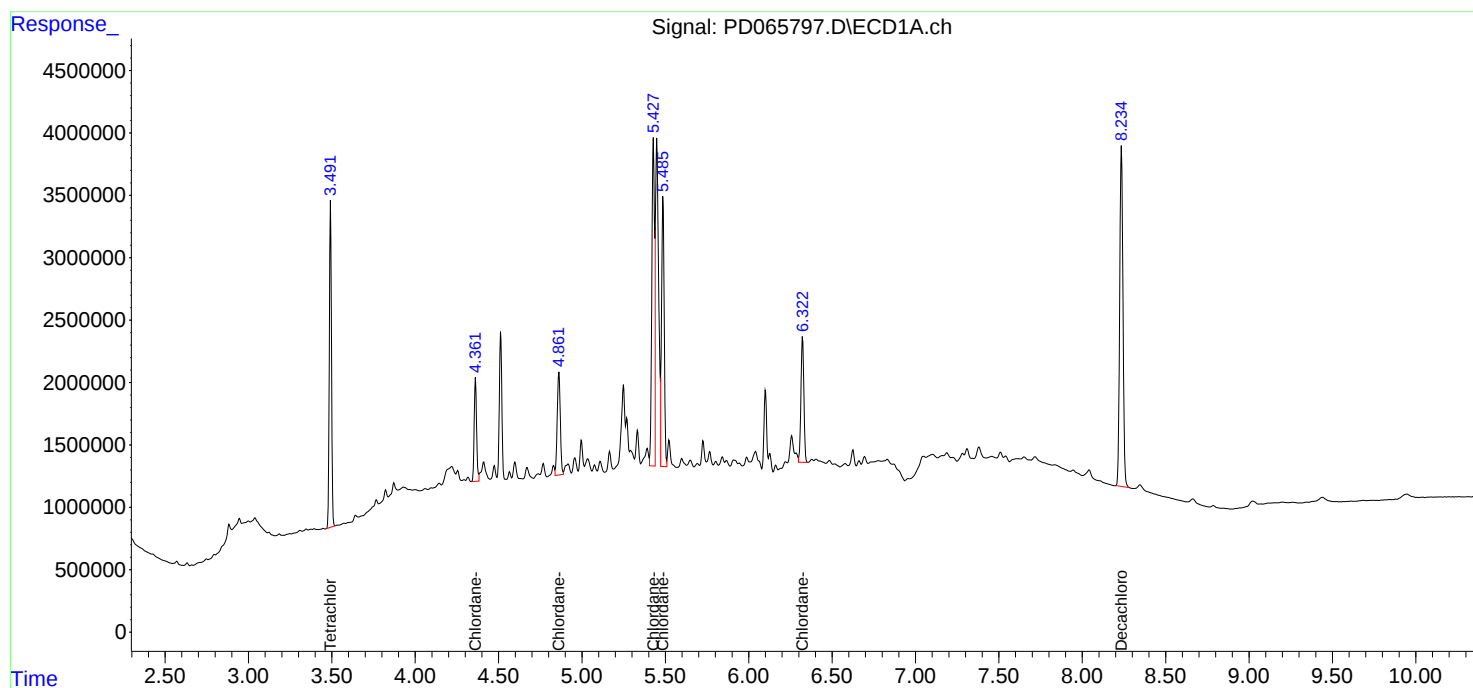


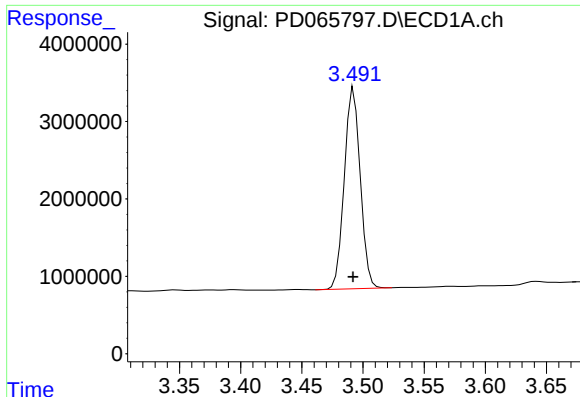

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 23586475
Conc: 24.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

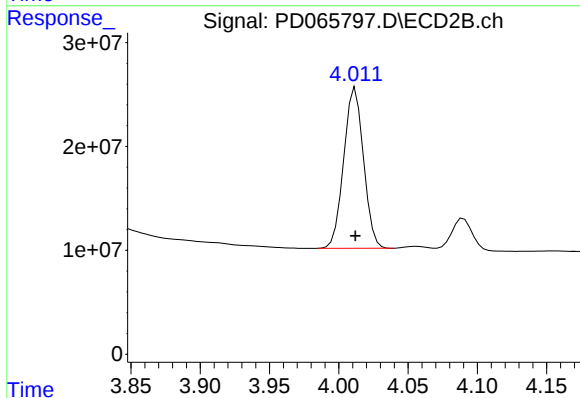


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 153787364
Conc: 25.78 ng/ml

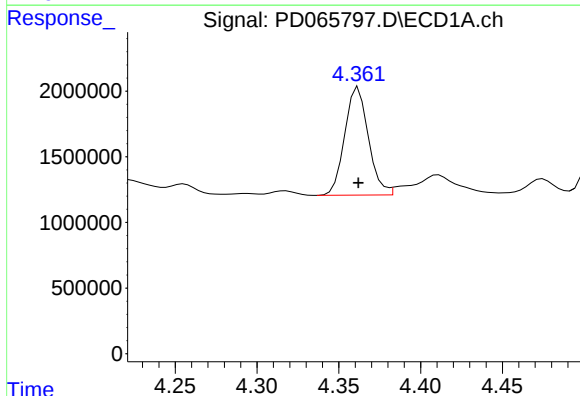


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 8260862
Conc: 259.68 ng/ml

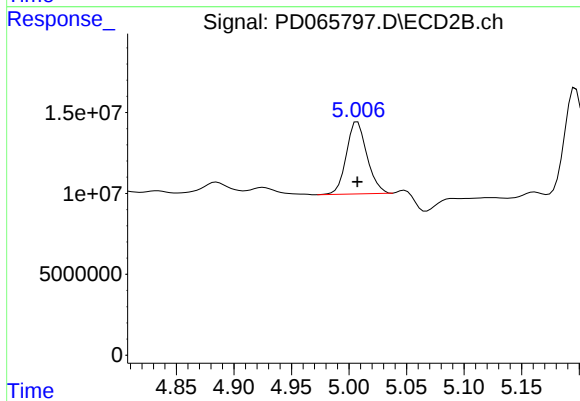

#23 Chlordane-1


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 55891086
Conc: 247.69 ng/ml

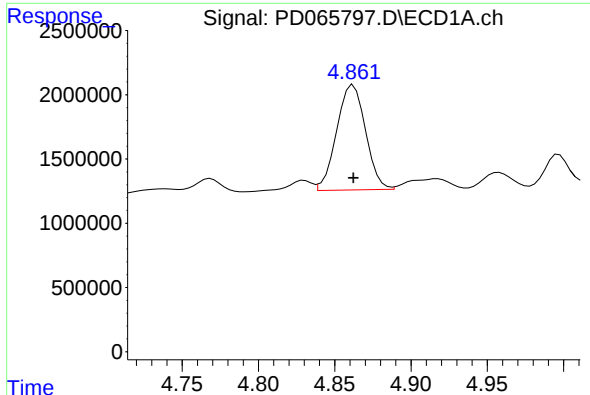

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 10772581
Conc: 267.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

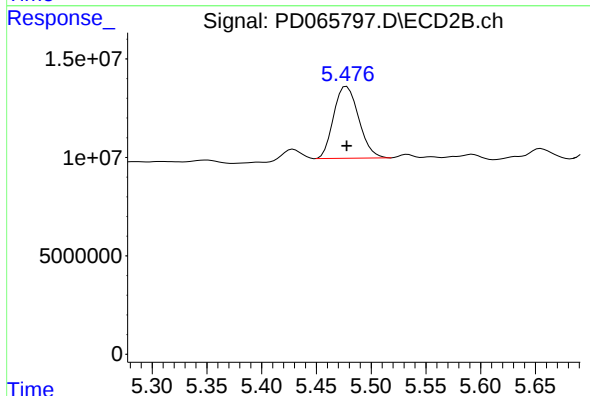


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 58218401
Conc: 267.92 ng/ml

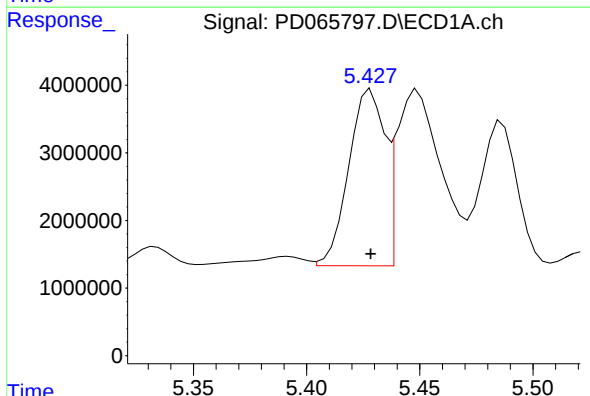


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 28788183
Conc: 245.88 ng/ml

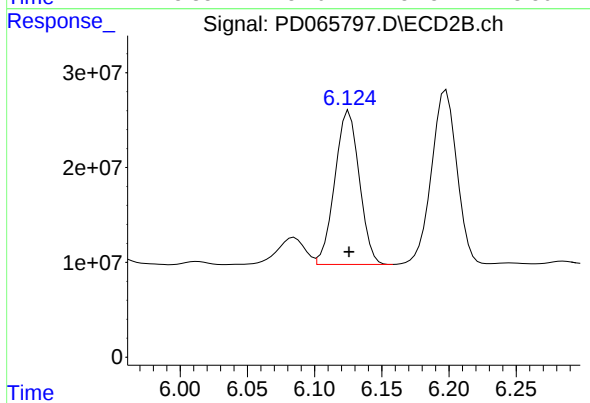

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 204640304
Conc: 256.91 ng/ml

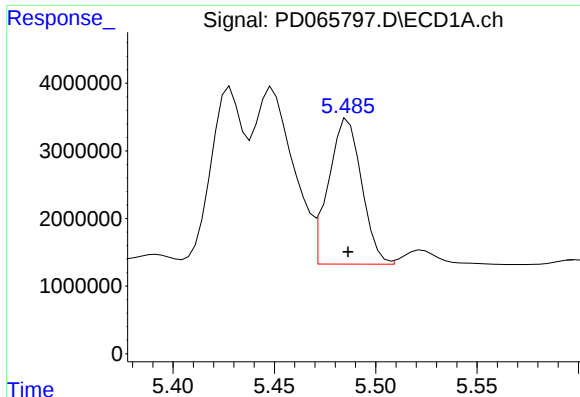

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 24404822
Conc: 248.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

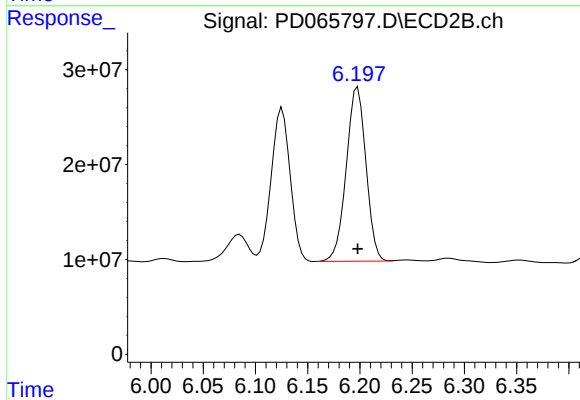


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 241009766
Conc: 259.58 ng/ml

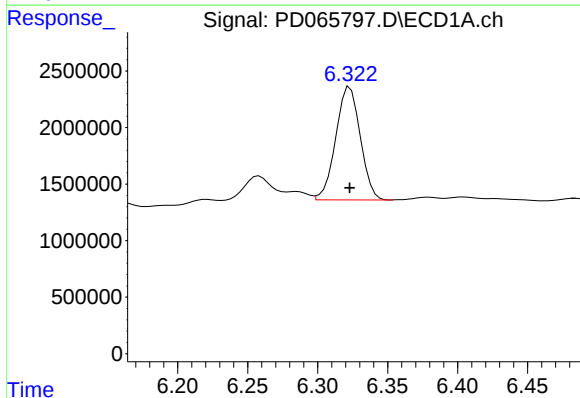


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 12194546
Conc: 260.79 ng/ml

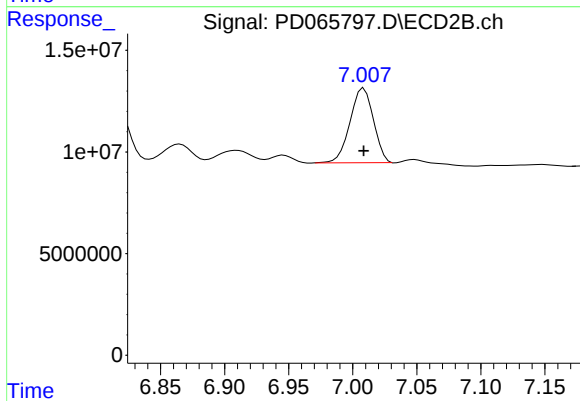

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 46732956
Conc: 254.88 ng/ml

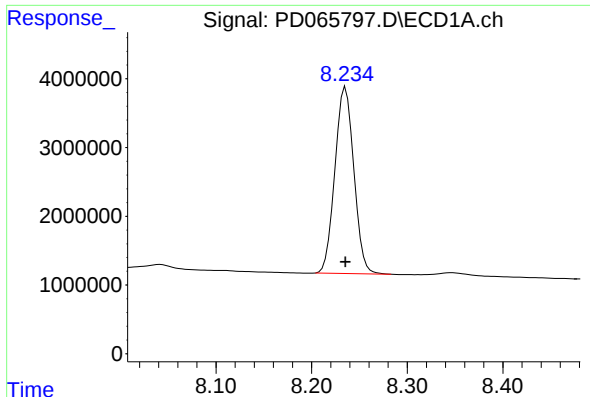

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 37327454
Conc: 26.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

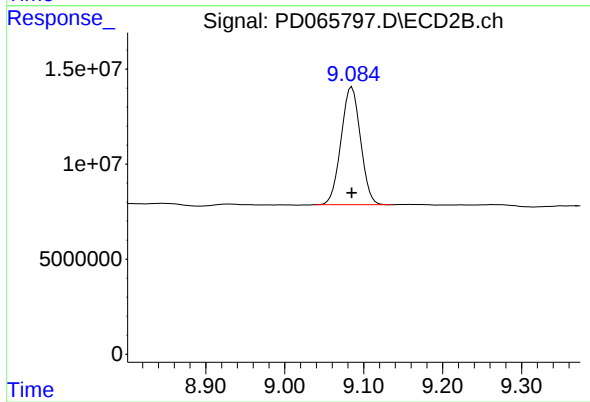

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 106172507
Conc: 26.60 ng/ml