

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
 Data File : PD065798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 18:50
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 04:12:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 04:04:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	4945989	33927950	5.163	5.535
28)	SA Decachlor...	8.235	9.084	8929465	23343248	6.042	5.656
Target Compounds							
23)	Chlordane-1	4.363	5.007	2011985	10223001	60.064	46.172
24)	Chlordane-2	4.862	5.477	2083473	14367849	51.302	62.115
25)	Chlordane-3	5.428	6.125	6037032	45707762	51.242	55.737
26)	Chlordane-4	5.486	6.197	5035290	54099690	50.983	56.403
27)	Chlordane-5	6.323	7.008	2797946	9789183	57.571	52.675



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
Data File : PD065798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 18:50
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 04:12:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 04:04:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

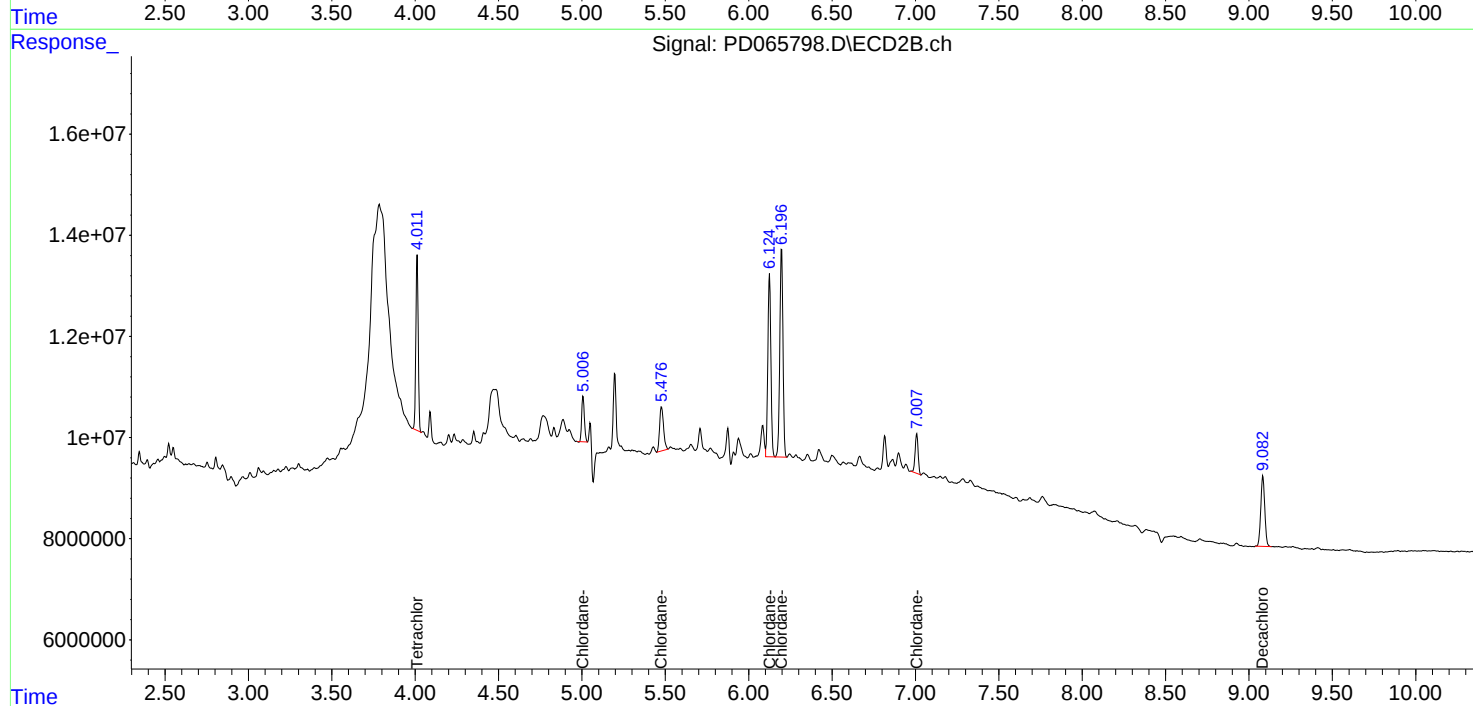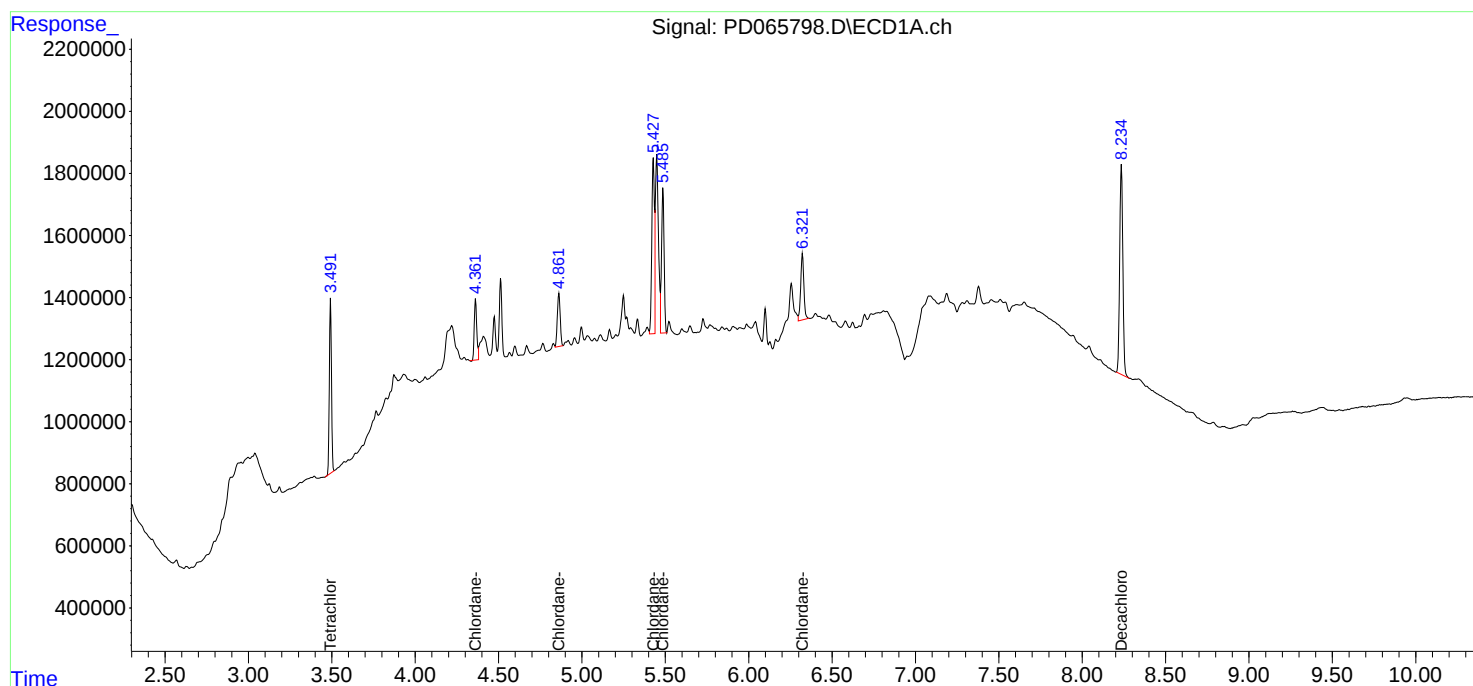


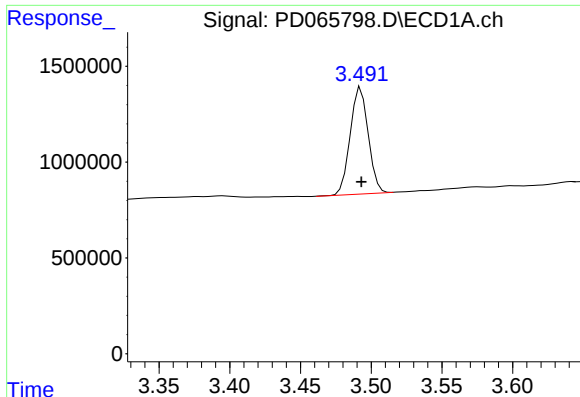

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 4945989
Conc: 5.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

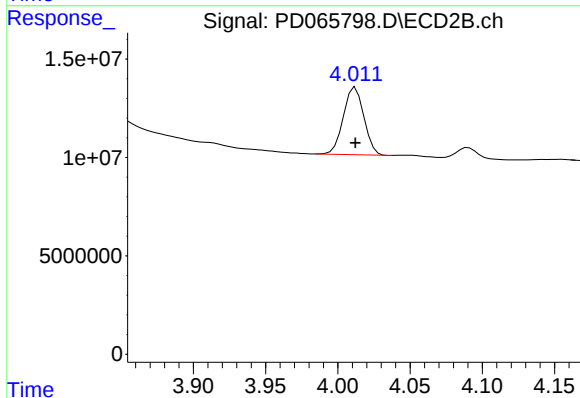


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 33927950
Conc: 5.54 ng/ml

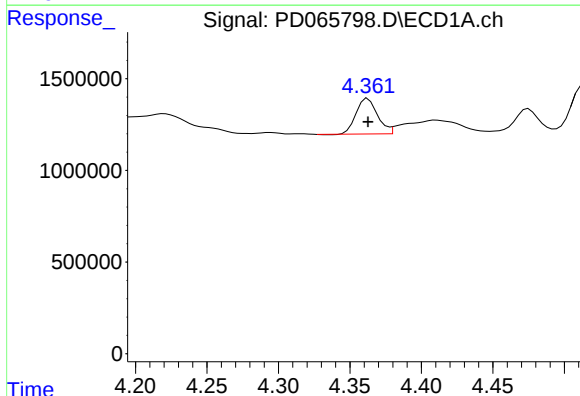


#23 Chlordane-1

R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 2011985
Conc: 60.06 ng/ml

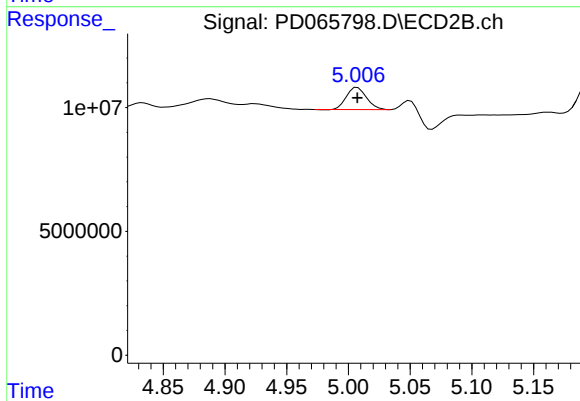

#23 Chlordane-1


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 10223001
Conc: 46.17 ng/ml

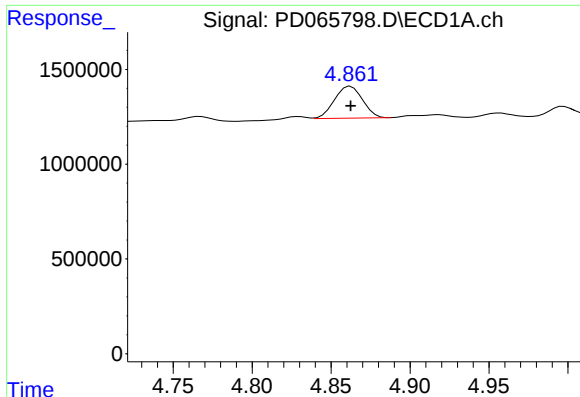

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 2083473
Conc: 51.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

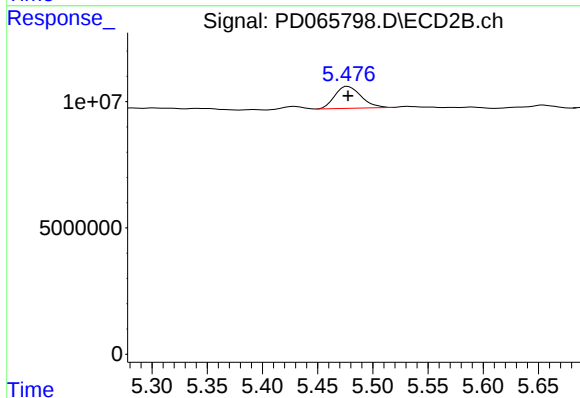


#24 Chlordane-2

R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 14367849
Conc: 62.11 ng/ml

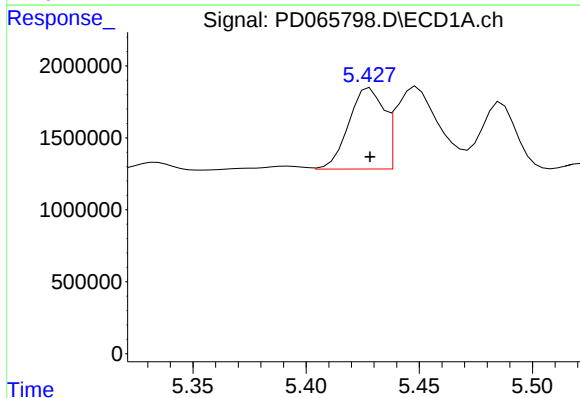


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 6037032
Conc: 51.24 ng/ml

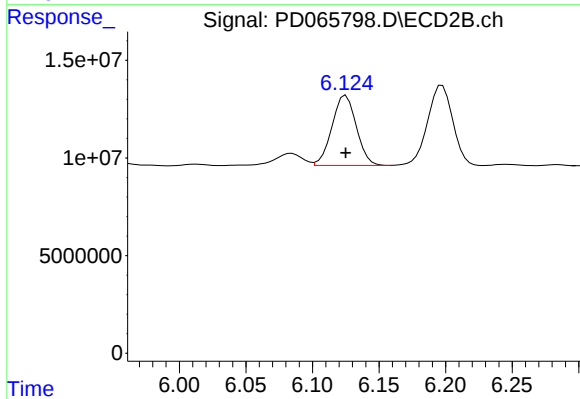

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 45707762
Conc: 55.74 ng/ml

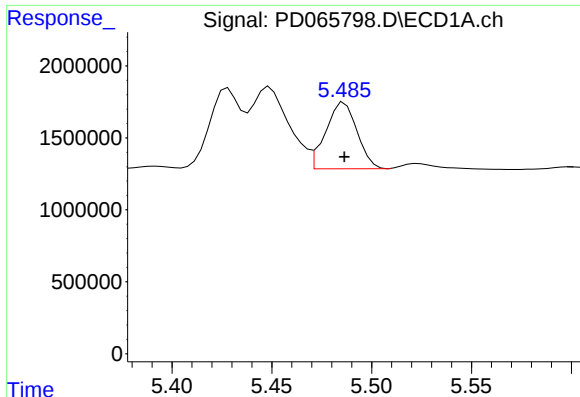

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 5035290
Conc: 50.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

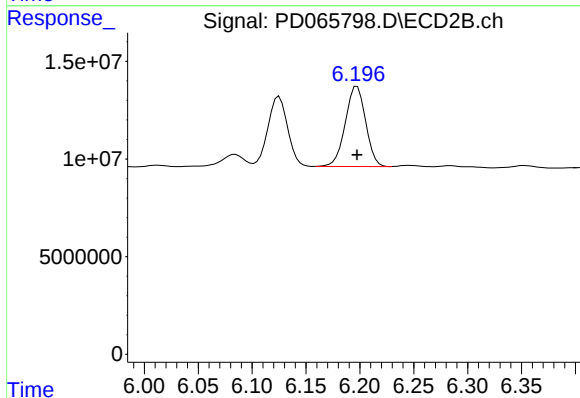


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 54099690
Conc: 56.40 ng/ml

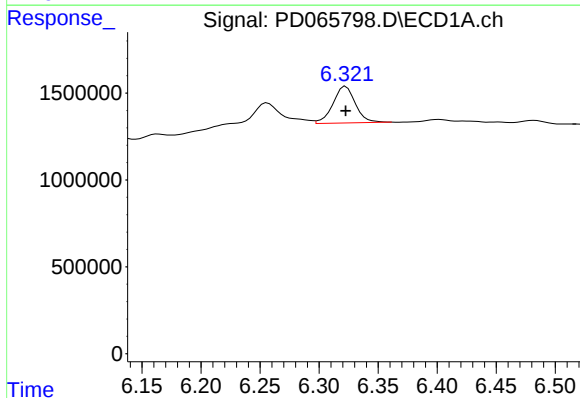


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 2797946
Conc: 57.57 ng/ml

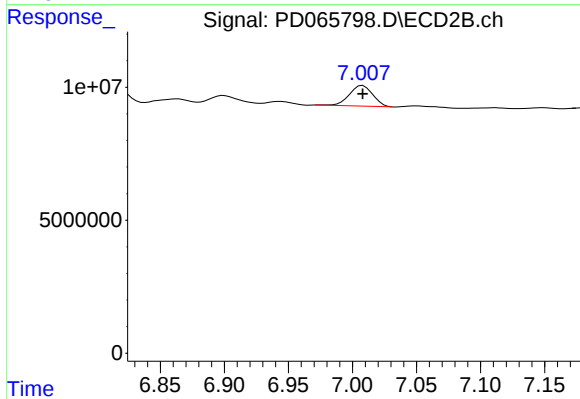

#27 Chlordane-5


R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 9789183
Conc: 52.68 ng/ml

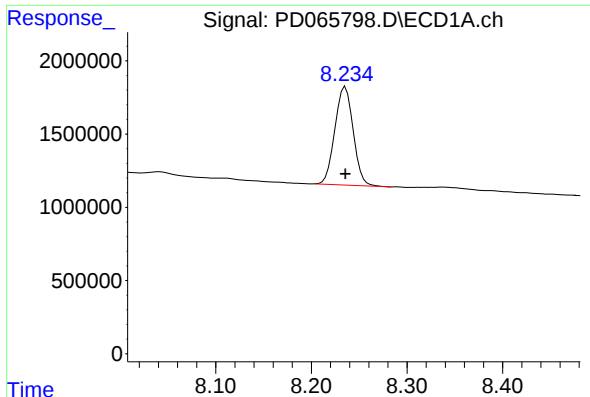

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 8929465
Conc: 6.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

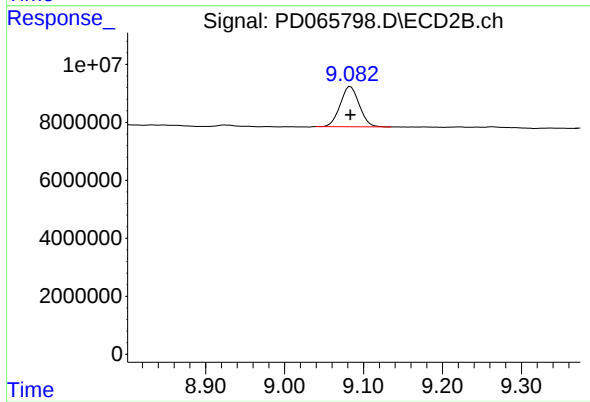

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 23343248
Conc: 5.66 ng/ml