

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
 Data File : PD065805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 20:27
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD092221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 04:14:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 04:13:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	4.012	50196810	317.2E6	52.396	51.760
28)	SA Decachlor...	8.235	9.084	74936588	215.5E6	50.702	52.208
Target Compounds							
23)	Chlordane-1	4.362	5.008	17660963	134.0E6	527.237	605.116
24)	Chlordane-2	4.862	5.477	23049370	124.8E6	567.556	539.417
25)	Chlordane-3	5.428	6.125	67452591	461.5E6	572.532	562.707
26)	Chlordane-4	5.486	6.198	56332688	536.8E6	570.374	559.633
27)	Chlordane-5	6.323	7.008	26573150	108.6E6	546.771	584.564



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092221\
Data File : PD065805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 20:27
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD092221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 04:14:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 04:13:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

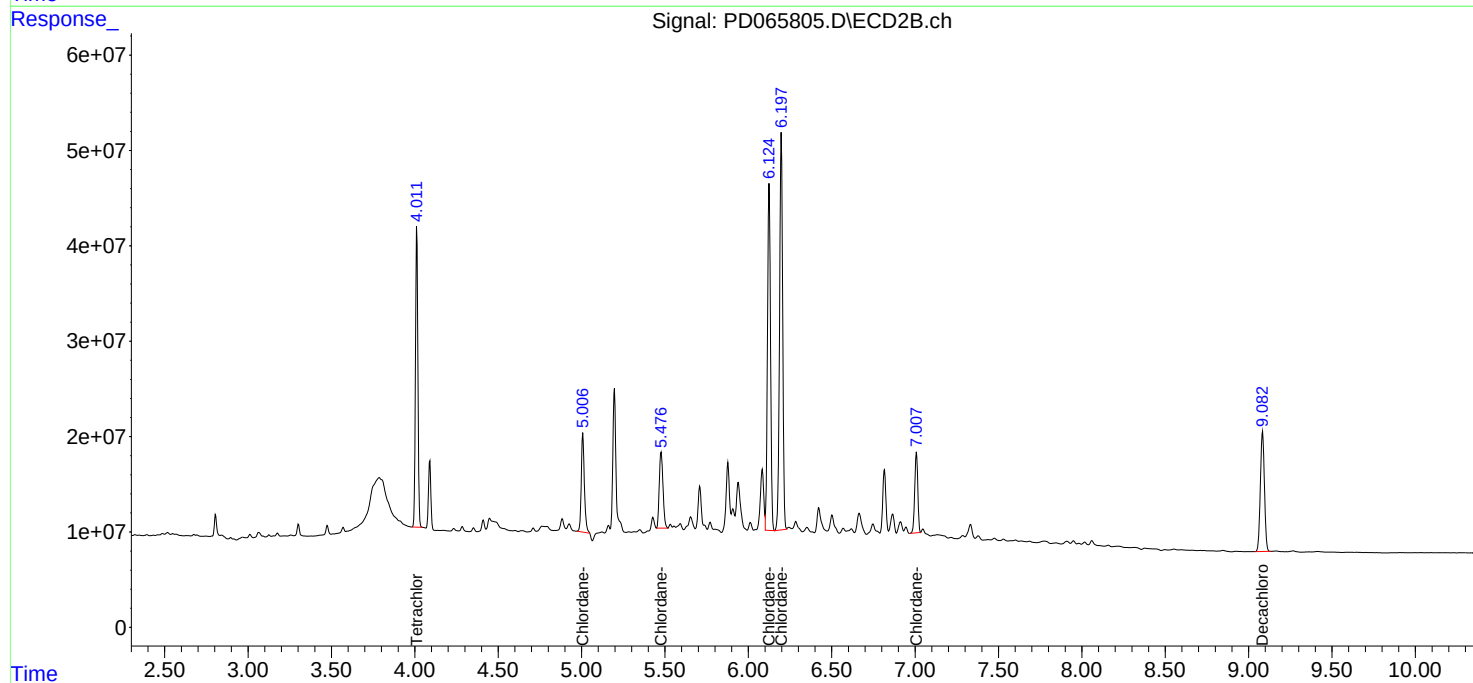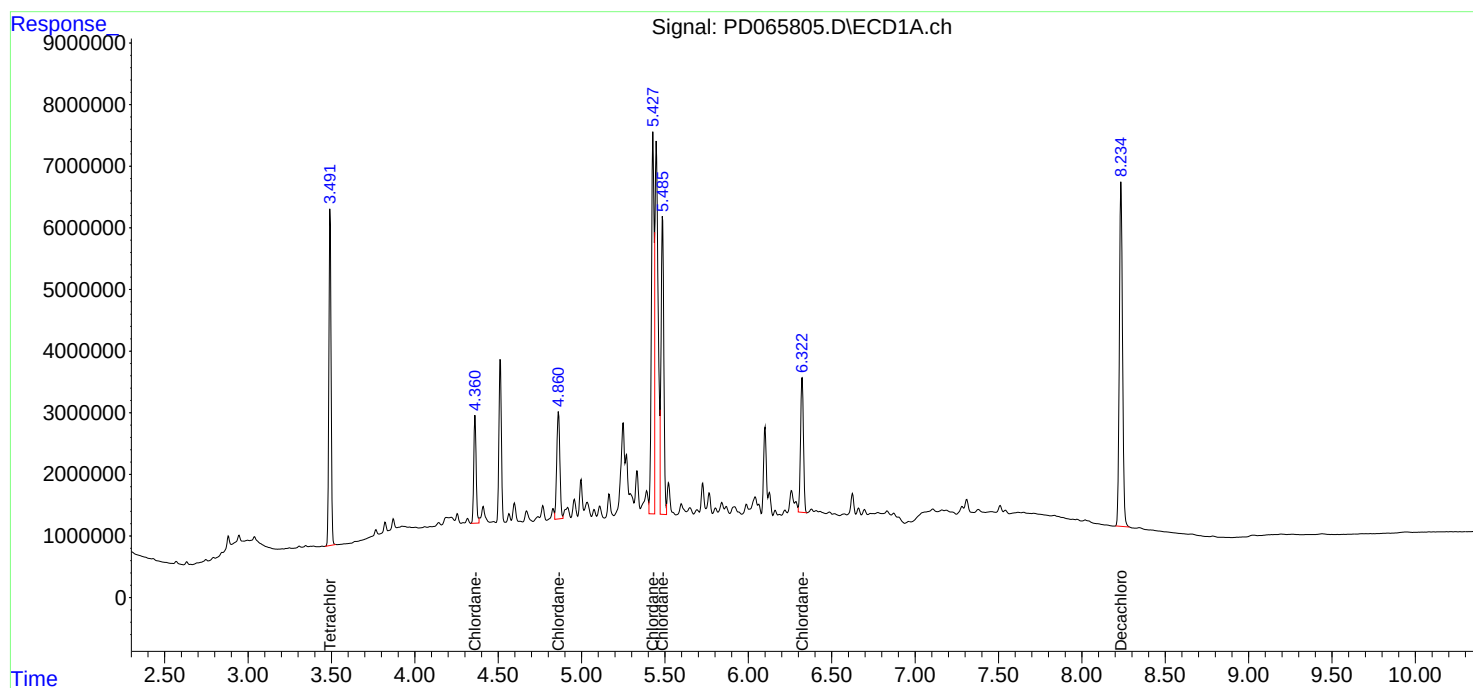


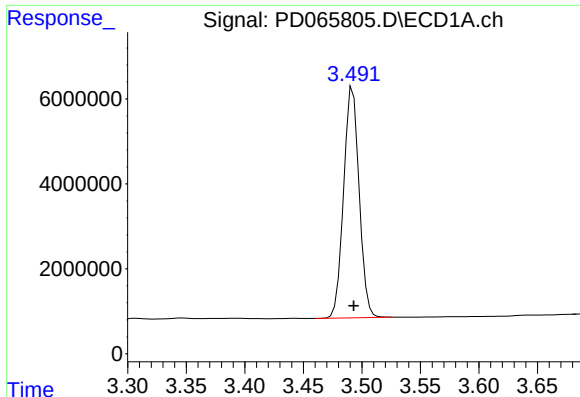

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.000 min
Response: 50196810
Conc: 52.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092221

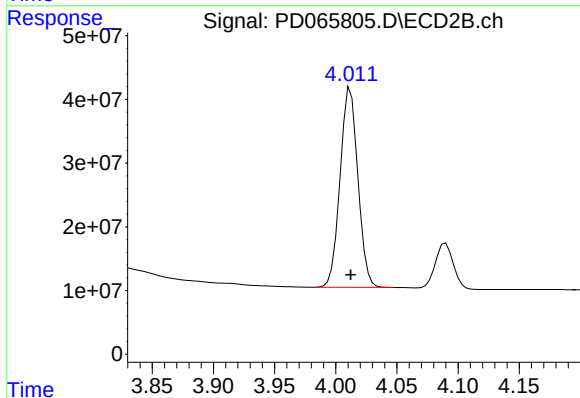


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 317249121
Conc: 51.76 ng/ml

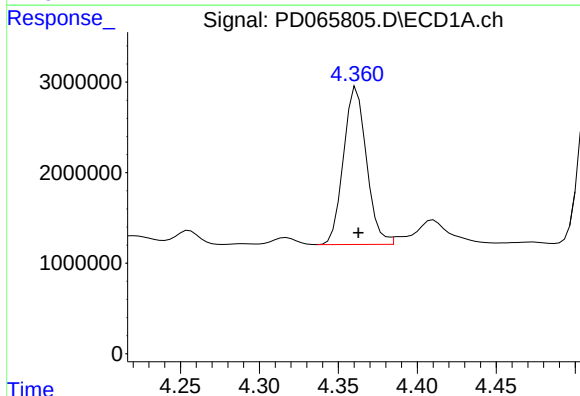


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 17660963
Conc: 527.24 ng/ml

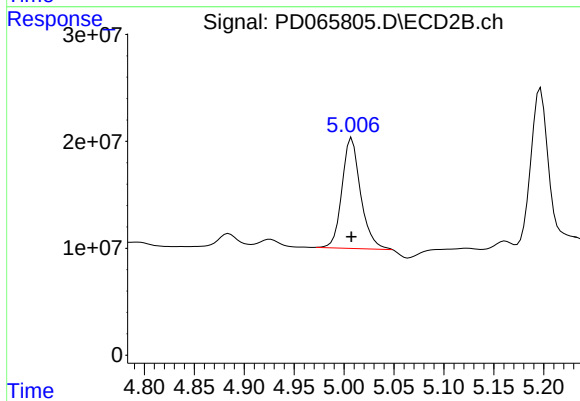

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 133980897
Conc: 605.12 ng/ml

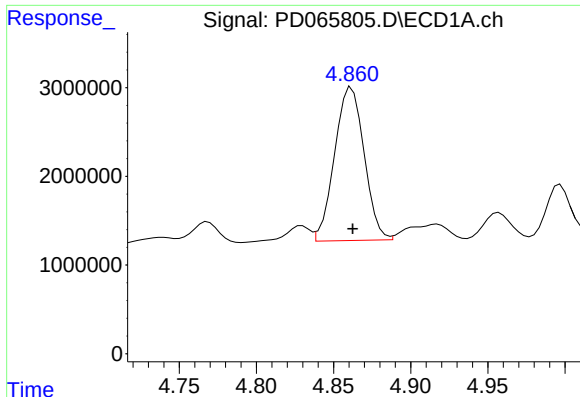

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 23049370
Conc: 567.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092221

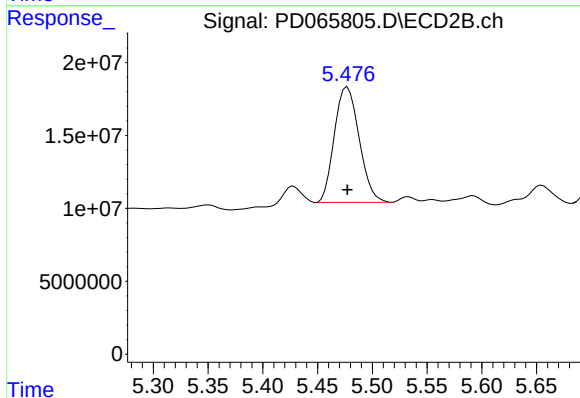


#24 Chlordane-2

R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 124773857
Conc: 539.42 ng/ml

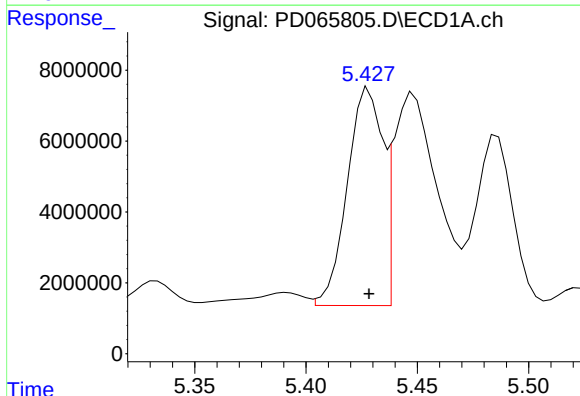


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 67452591
Conc: 572.53 ng/ml

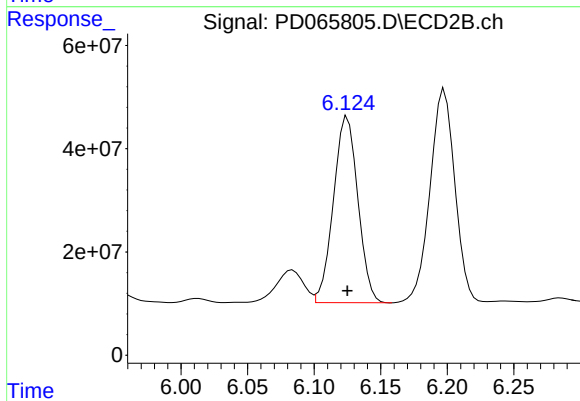

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 461451576
Conc: 562.71 ng/ml

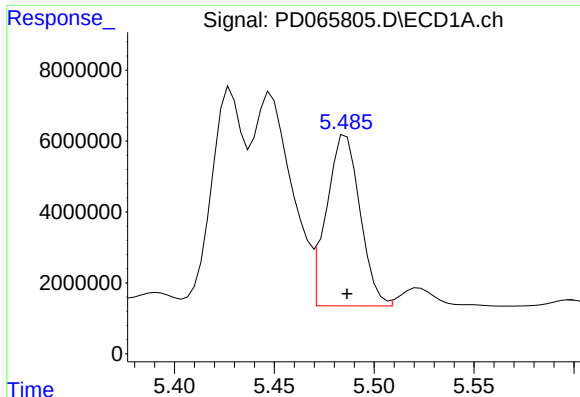

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 56332688
Conc: 570.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092221

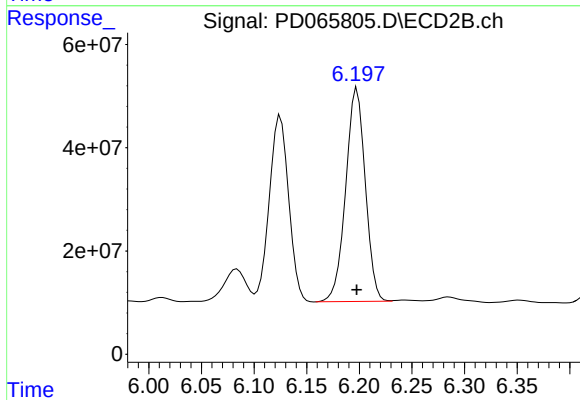


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 536778733
Conc: 559.63 ng/ml

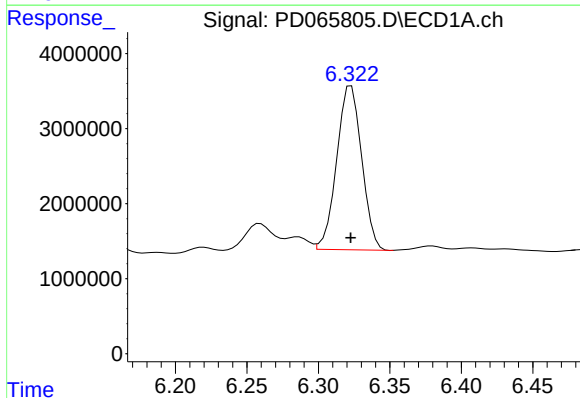


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 26573150
Conc: 546.77 ng/ml

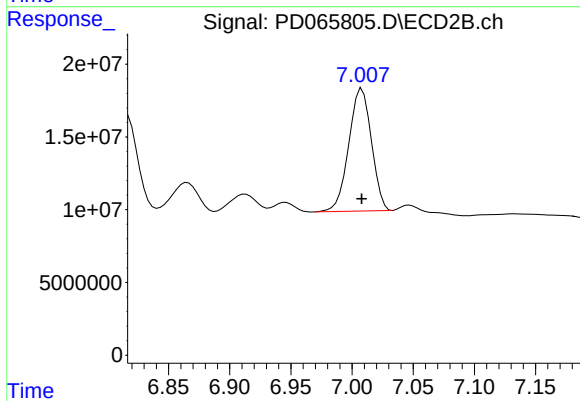

#27 Chlordane-5


R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 108635316
Conc: 584.56 ng/ml

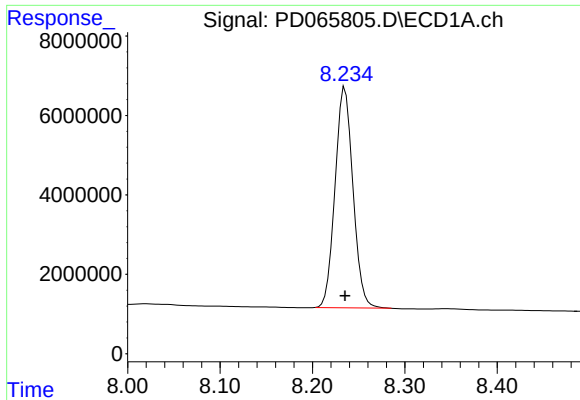

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 74936588
Conc: 50.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092221

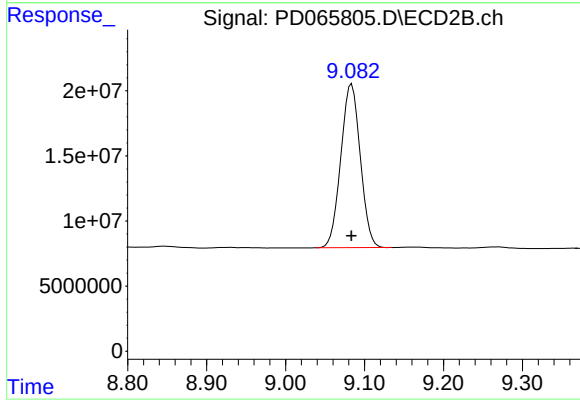

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 215464133
Conc: 52.21 ng/ml