

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092222\
 Data File : PD071979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 13:23
 Operator : AR\AJ
 Sample : EPA MDL SPIKE 10PPB
 Misc : PP20810 MDL SPIKE
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EPA MDL SPIKE 10PPB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 03:15:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	7.949	9.100	126874	159052	<MDL	<MDL #
Target Compounds							
2)	A alpha-BHC	3.323	4.030	33800590	398.8E6	8.763	9.038
3)	MA gamma-BHC...	3.657	4.366	32154444	340.0E6	8.709	9.142
4)	MA Heptachlor	4.003	4.944	32775649	267.2E6	8.611	9.896
5)	MB Aldrin	4.287	5.286	33624966	230.2E6	9.446	10.655
6)	B beta-BHC	3.956	4.573	15372480	132.7E6	9.677	9.275
7)	B delta-BHC	4.189	4.820	31102032	242.0E6	8.901	9.207
8)	B Heptachlo...	4.793	5.718	30619562	180.8E6	9.394	10.692
9)	A Endosulfan I	5.166	6.106	27822713	160.6E6	8.828	10.226
10)	B trans-Chl...	5.045	5.973	30704834	177.3E6	9.069	10.475
11)	B cis-Chlor...	5.110	6.050	30616752	171.3E6	9.179	10.512
12)	B 4,4'-DDE	5.301	6.223	27596961	163.4E6	8.997	11.197
13)	MA Dieldrin	5.433	6.383	30061753	174.1E6	8.681	10.877 #
14)	MA Endrin	5.710	6.616	27869528	148.0E6	9.306	11.248
15)	B Endosulfa...	6.006	6.842	27020202	145.4E6	10.165	12.060
16)	A 4,4'-DDD	5.859	6.748	24319788	138.5E6	9.240	11.320
17)	MA 4,4'-DDT	6.112	7.059	23144551	125.0E6	8.502	10.357
18)	B Endrin al...	6.186	6.973	22900093	115.7E6	9.900	11.336
19)	B Endosulfa...	6.411	7.205	26485609	129.9E6	9.942	11.441
20)	A Methoxychlor	6.691	7.536	14007541	72247045	9.753	13.167 #
21)	B Endrin ke...	6.920	7.698	29861181	146.5E6	9.979	11.836
22)	Toxaphene-1	5.433f	5.886	30061753	781951	1716.146	13.170 #
23)	Toxaphene-2	5.710f	6.308f	27869528	539976	1513.990	4.542 #
24)	Toxaphene-3	6.006	7.059	27020202	125.0E6	1270.416	684.203 #
25)	Toxaphene-4	6.830	7.205	1317693	129.9E6	15.018	494.762 #
26)	Toxaphene-5	0.000	7.615	0	503449	N.D.	3.376

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092222\
Data File : PD071979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 13:23
Operator : AR\AJ
Sample : EPA MDL SPIKE 10PPB
Misc : PP20810 MDL SPIKE
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 03:15:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

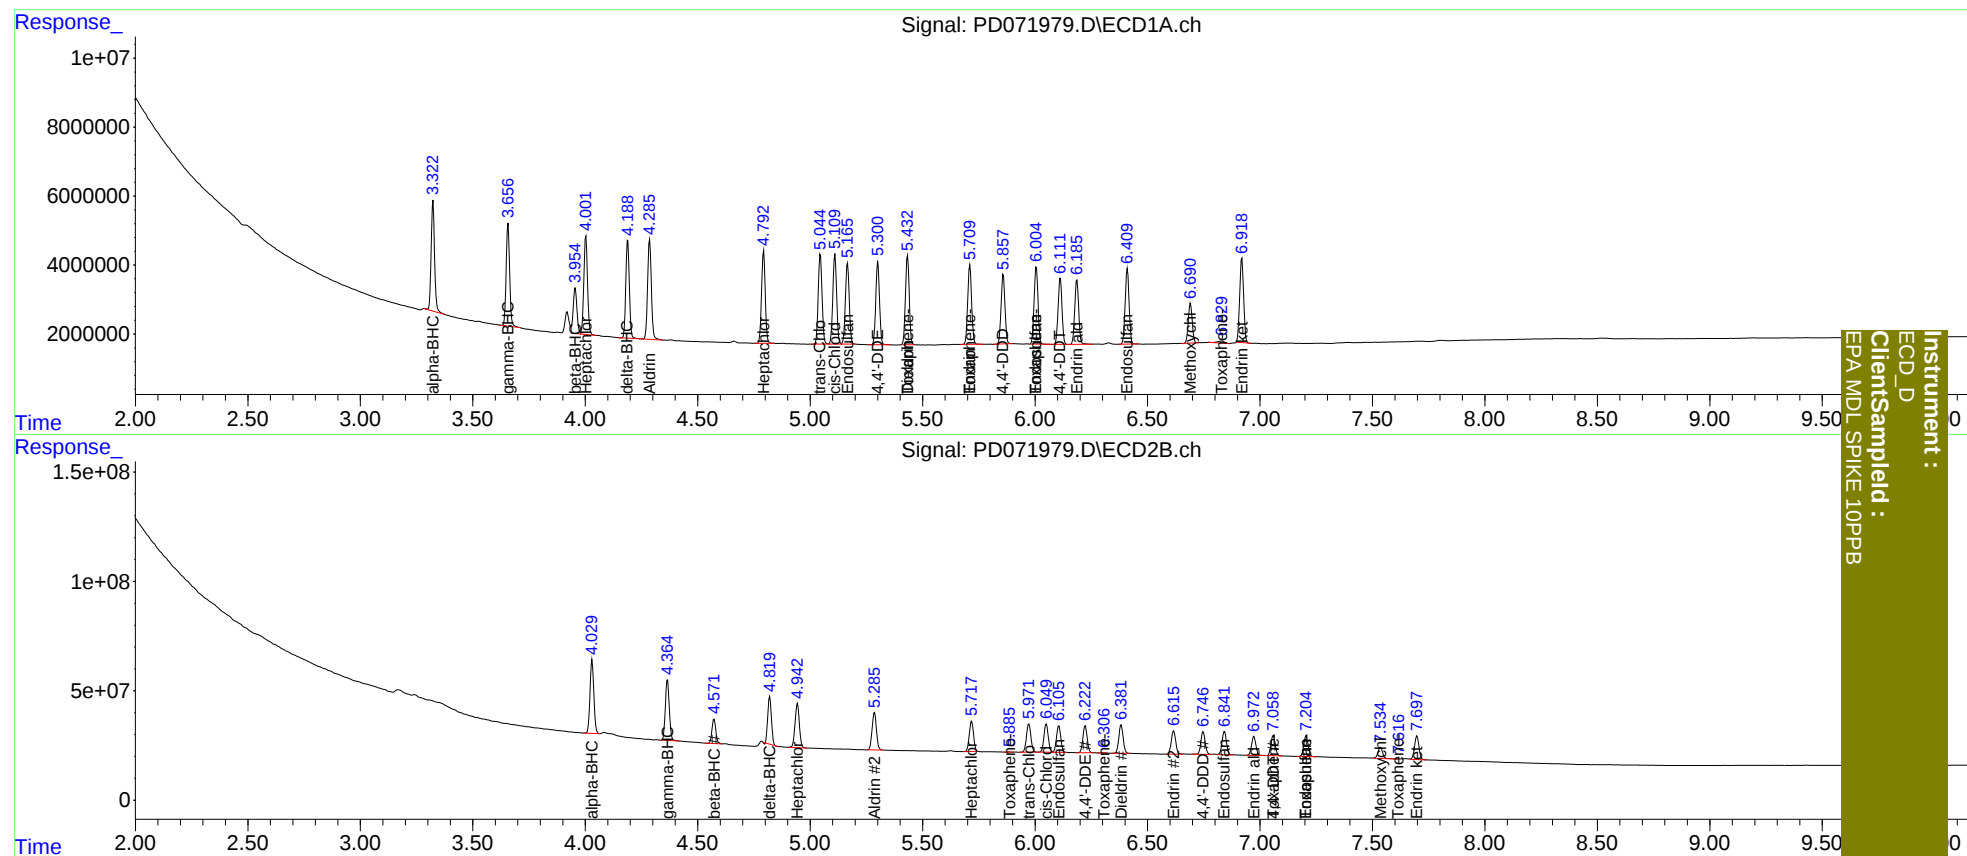

Instrument :
ECD_D
ClientSample :
EPA MDL SPIKE 10PPB