

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
 Data File : PD085492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2024 22:40
 Operator : AR\AJ
 Sample : PIBLK149
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK311

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:31:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	2.890	25931476	81721655	21.414	21.620
2)	SA Decachlor...	8.958	8.084	42242887	81348610	25.751	30.430
Target Compounds							
3)	MA gamma-BHC...	4.216f	0.000	30750847	0	12.291	N.D. #
7)	B delta-BHC	4.708	0.000	1592698	0	0.699	N.D. #
20)	A Methoxychlor	7.464f	0.000	2409441	0	3.293	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
Data File : PD085492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2024 22:40
Operator : AR\AJ
Sample : PIBLK149
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:31:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

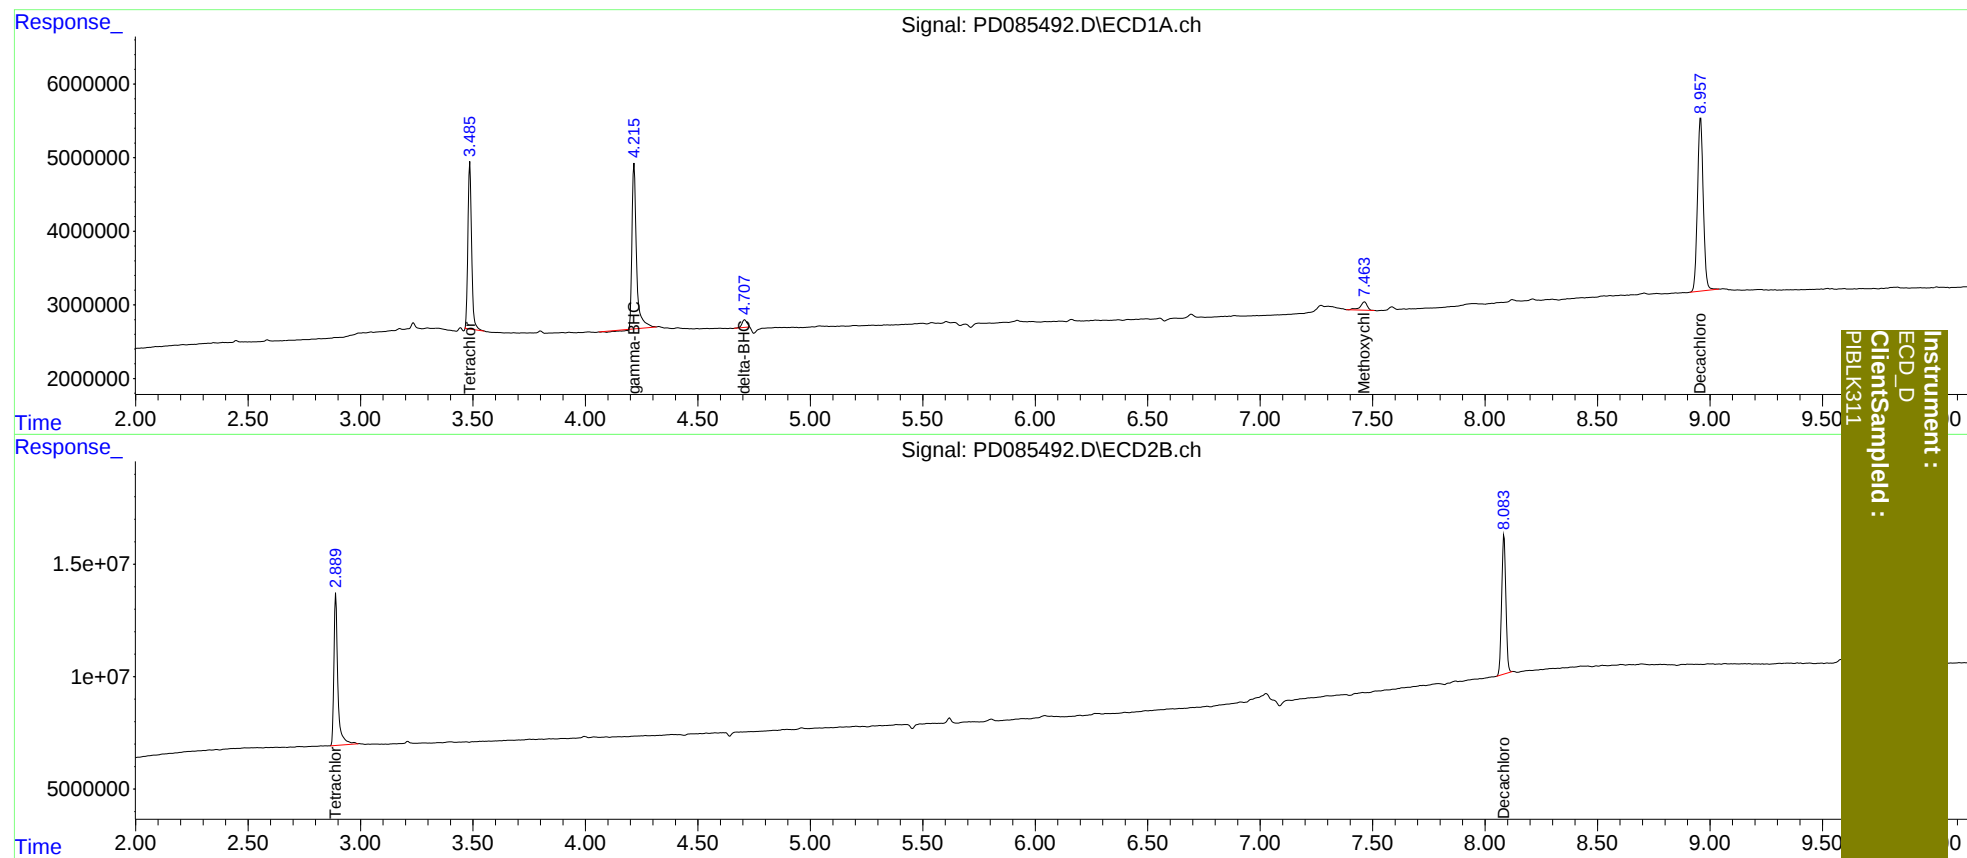


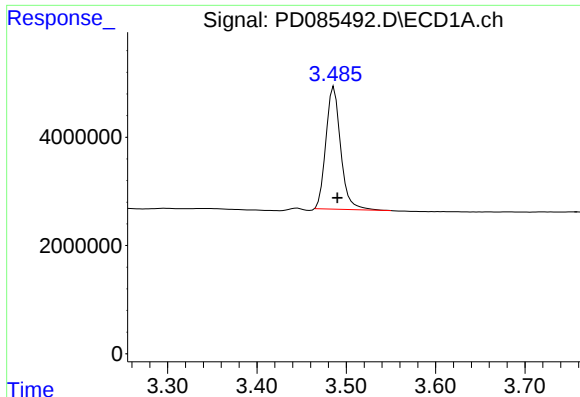

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: -0.004 min
Response: 25931476
Conc: 21.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK311

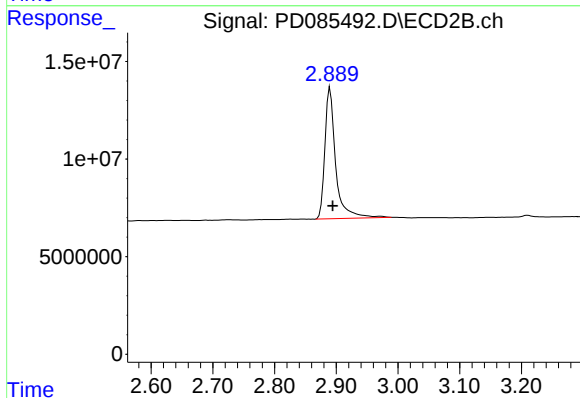


#1 Tetrachloro-m-xylene

R.T.: 2.890 min
Delta R.T.: -0.004 min
Response: 81721655
Conc: 21.62 ng/ml

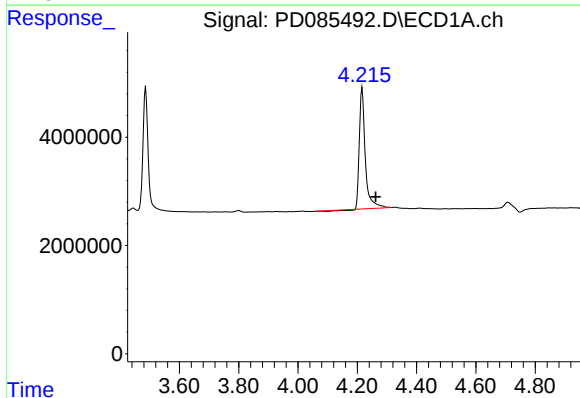


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: -0.046 min
Response: 30750847
Conc: 12.29 ng/ml

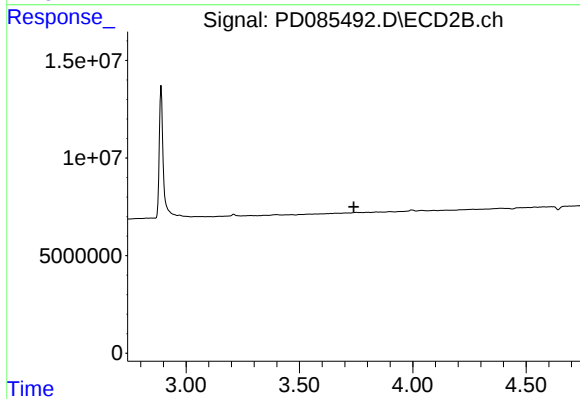

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.739 min
Response: 0
Conc: N.D.

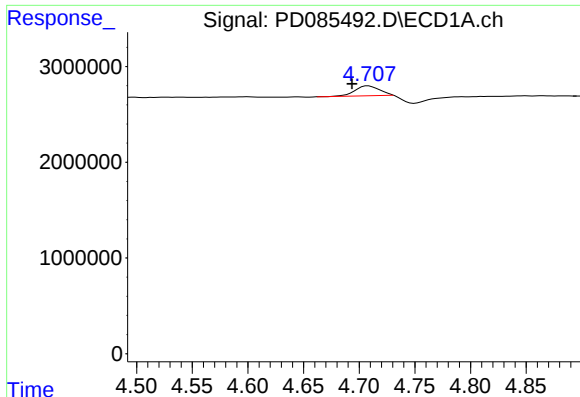

#7 delta-BHC


R.T.: 4.708 min
Delta R.T.: 0.015 min
Response: 1592698
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK311

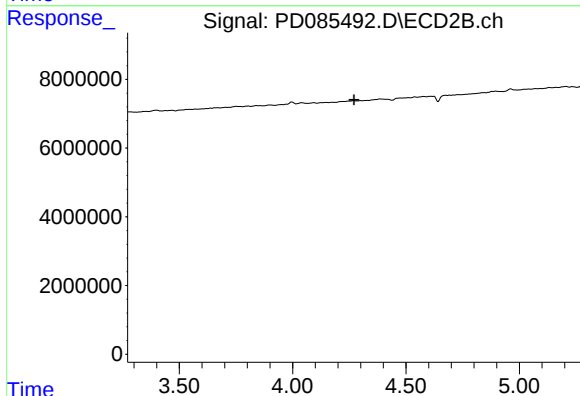


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.

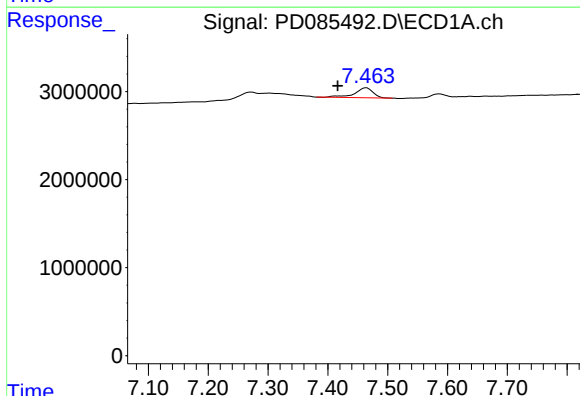


#20 Methoxychlor

R.T.: 7.464 min
Delta R.T.: 0.048 min
Response: 2409441
Conc: 3.29 ng/ml

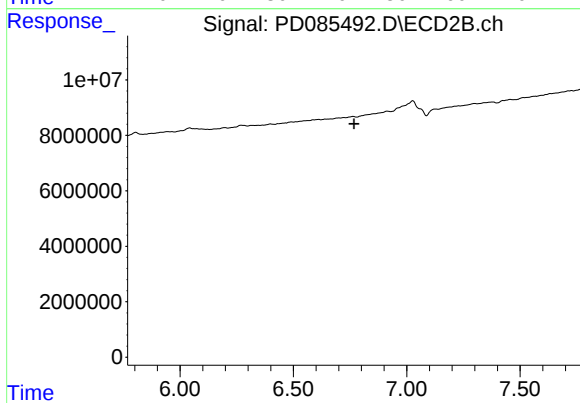

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

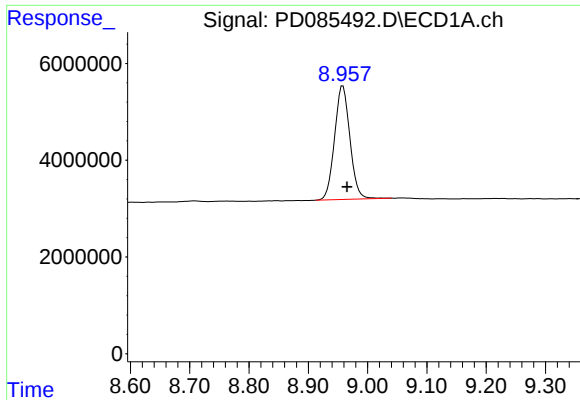

#27 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.007 min
Response: 42242887
Conc: 25.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK311

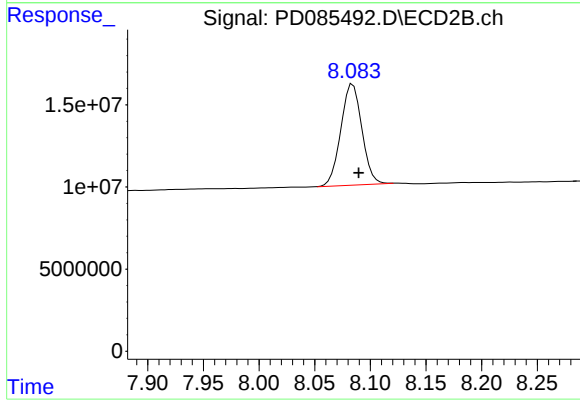

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.005 min
Response: 81348610
Conc: 30.43 ng/ml