

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
 Data File : PD085494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2024 23:20
 Operator : AR\AJ
 Sample : PB163490BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK490

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:32:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	2.890	21138478	68342444	17.456	18.081
2)	SA Decachlor...	8.959	8.084	35421920	68477131	21.593	25.615
Target Compounds							
3)	MA gamma-BHC...	4.217f	0.000	30204011	0	12.073	N.D. #
20)	A Methoxychlor	7.465f	0.000	2735748	0	3.739	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
Data File : PD085494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2024 23:20
Operator : AR\AJ
Sample : PB163490BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:32:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

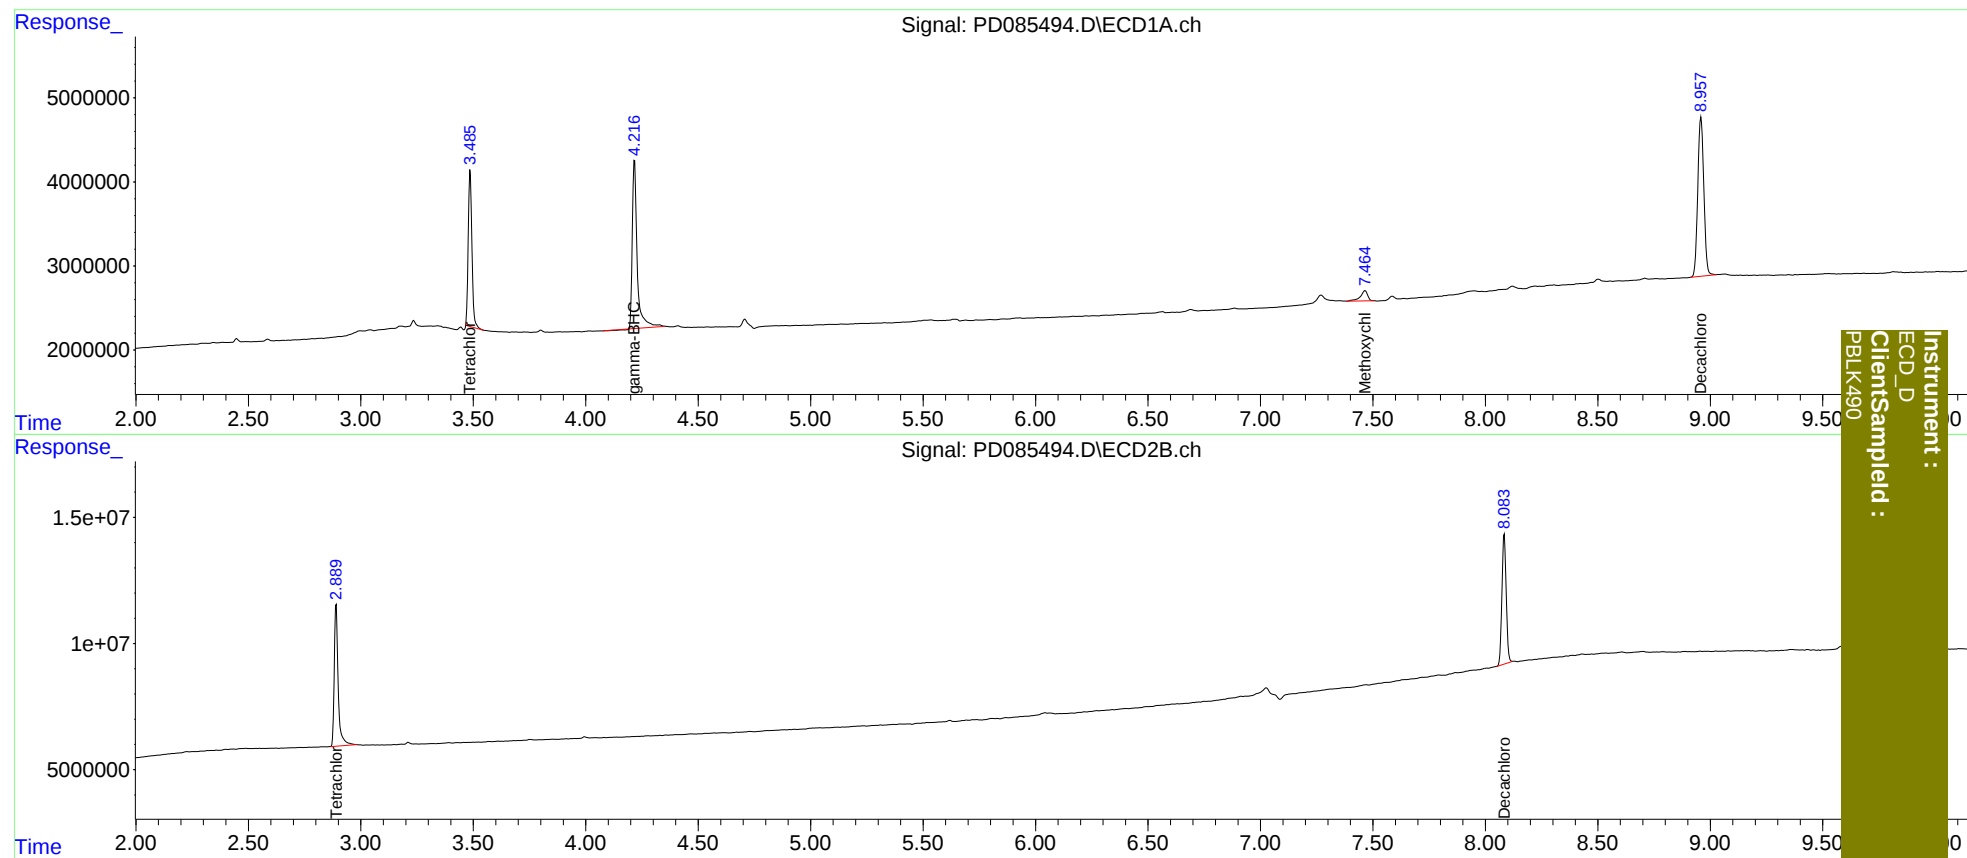


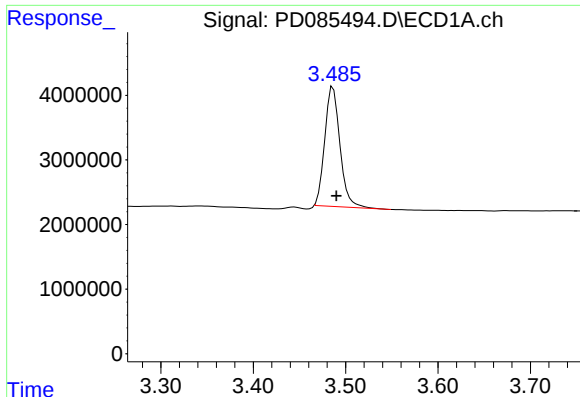

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: -0.004 min
Response: 21138478
Conc: 17.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK490

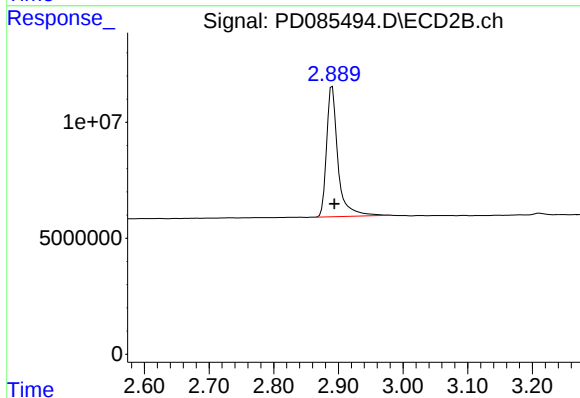


#1 Tetrachloro-m-xylene

R.T.: 2.890 min
Delta R.T.: -0.003 min
Response: 68342444
Conc: 18.08 ng/ml

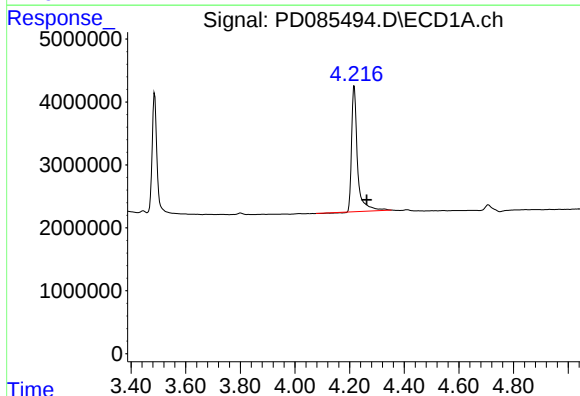


#3 gamma-BHC (Lindane)

R.T.: 4.217 min
Delta R.T.: -0.045 min
Response: 30204011
Conc: 12.07 ng/ml

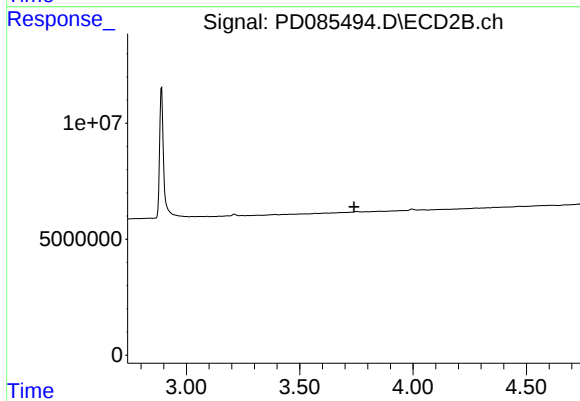

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.739 min
Response: 0
Conc: N.D.

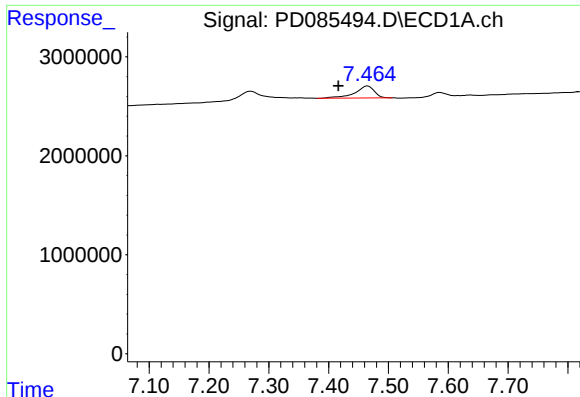

#20 Methoxychlor


R.T.: 7.465 min
Delta R.T.: 0.049 min
Response: 2735748
Conc: 3.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK490

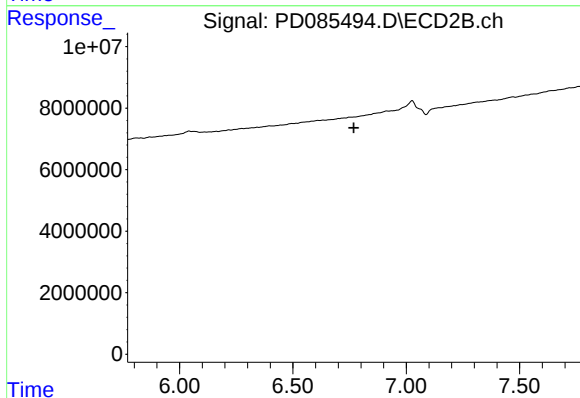


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

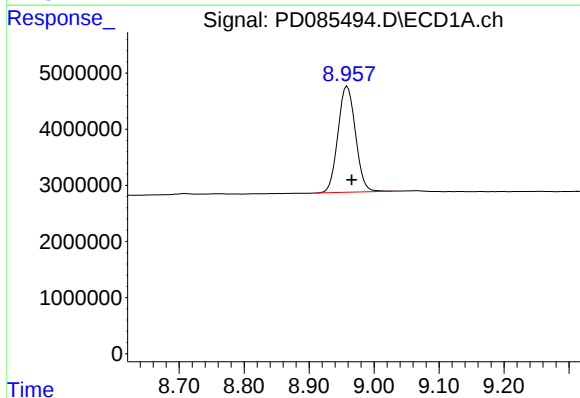

#27 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.007 min
Response: 35421920
Conc: 21.59 ng/ml

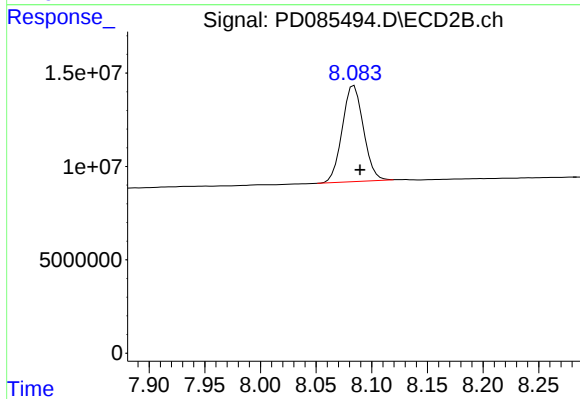

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.005 min
Response: 68477131
Conc: 25.62 ng/ml