

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
 Data File : PD085498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 00:14
 Operator : AR\AJ
 Sample : P4017-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC42

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:33:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	2.904	35993130	454.1E6	29.722m	120.131m#
27)	SA Decachlor...	8.949	8.082	46009168	17969768	28.047m	6.722m#
Target Compounds							
2)	A alpha-BHC	3.933	3.402	1026.2E6	1484.1E6	434.345	268.751 #
7)	B delta-BHC	4.691	4.269	1301.9E6	1800.7E6	571.114	341.844 #
9)	A Endosulfan I	5.997	5.261	125.2E6	63864503	70.626m	15.541m#
11)	B cis-Chlor...	5.937	5.201	110.2E6	234.6E6	54.955m	50.572m
13)	MA Dieldrin	6.268	5.516	151.6E6	48532717	78.403m	10.426m#
14)	MA Endrin	6.469	5.799	101.4E6	261.2E6	63.082m	62.968m
16)	A 4,4'-DDD	6.624	5.938	384.5E6	557.7E6	291.802m	166.521m#
20)	A Methoxychlor	7.410	6.751	297.6E6	371.3E6	406.710m	228.809m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
Data File : PD085498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 00:14
Operator : AR\AJ
Sample : P4017-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:33:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

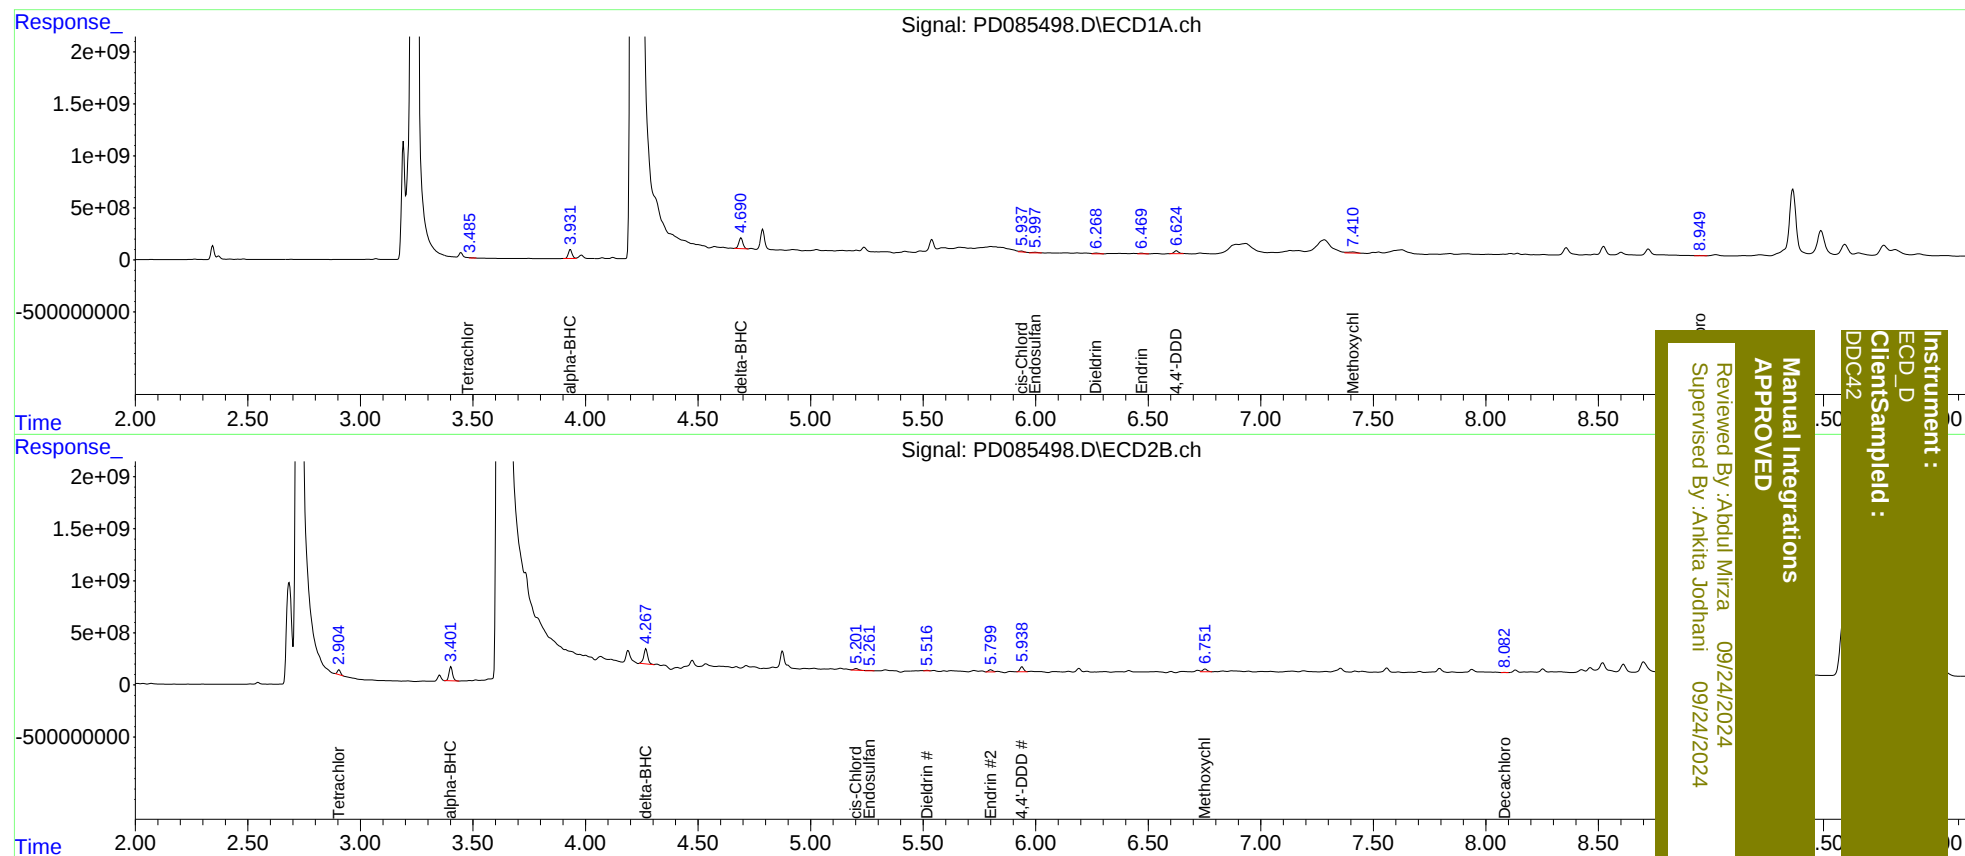

Reviewed By: Abdul Mirza 09/24/2024
Supervised By: Ankita Jodhani 09/24/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC42