

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
 Data File : PD085495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2024 23:33
 Operator : AR\AJ
 Sample : PB163490BS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS490

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:32:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	2.891	20150960	60172438	16.640m	15.919
27)	SA Decachlor...	8.958	8.084	32334266	62476133	19.711	23.370
Target Compounds							
2)	A alpha-BHC	3.931	3.402	9212016	24426702	3.899	4.423
3)	MA gamma-BHC...	4.259	3.737	11952995	24302110	4.778	4.663
4)	MA Heptachlor	4.853	4.089	8920883	21421278	4.225	4.513
5)	MB Aldrin	5.193	4.375	9499399	24778692	4.376	4.888
6)	B beta-BHC	4.443	4.029	4066950	10592993	4.265	4.555m
7)	B delta-BHC	4.688	4.268	10673516	22523994	4.682m	4.276
8)	B Heptachlo...	5.612	4.879	9053808	23382457	4.533	5.037
9)	A Endosulfan I	5.993	5.255	8469373	21217180	4.779	5.163
10)	B trans-Chl...	5.865	5.133	8659419	23078267	4.550	5.100
11)	B cis-Chlor...	5.946	5.197	8994401	23484561	4.487	5.062
12)	B 4,4'-DDE	6.116	5.382	14484865	39385404	8.286	9.193
13)	MA Dieldrin	6.266	5.521	17319315	46371484	8.958	9.962
14)	MA Endrin	6.492	5.798	13929880	41547532	8.664	10.017
15)	B Endosulfa...	6.703	6.090	15412786	38646691	8.406	10.445
16)	A 4,4'-DDD	6.623	5.938	11343922	32947693	8.610m	9.838
17)	MA 4,4'-DDT	6.939	6.192	11287689	33339262	9.260m	10.526
18)	B Endrin al...	6.832	6.269	11789626	31509575	9.954	11.395
19)	B Endosulfa...	7.066	6.493	14246291	36684062	9.436	10.681
20)	A Methoxychlor	7.412	6.764	36374574	93380316	49.716	57.538
21)	B Endrin ke...	7.544	7.004	14812471	50210967	9.265	10.810

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092224\
Data File : PD085495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2024 23:33
Operator : AR\AJ
Sample : PB163490BS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:32:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

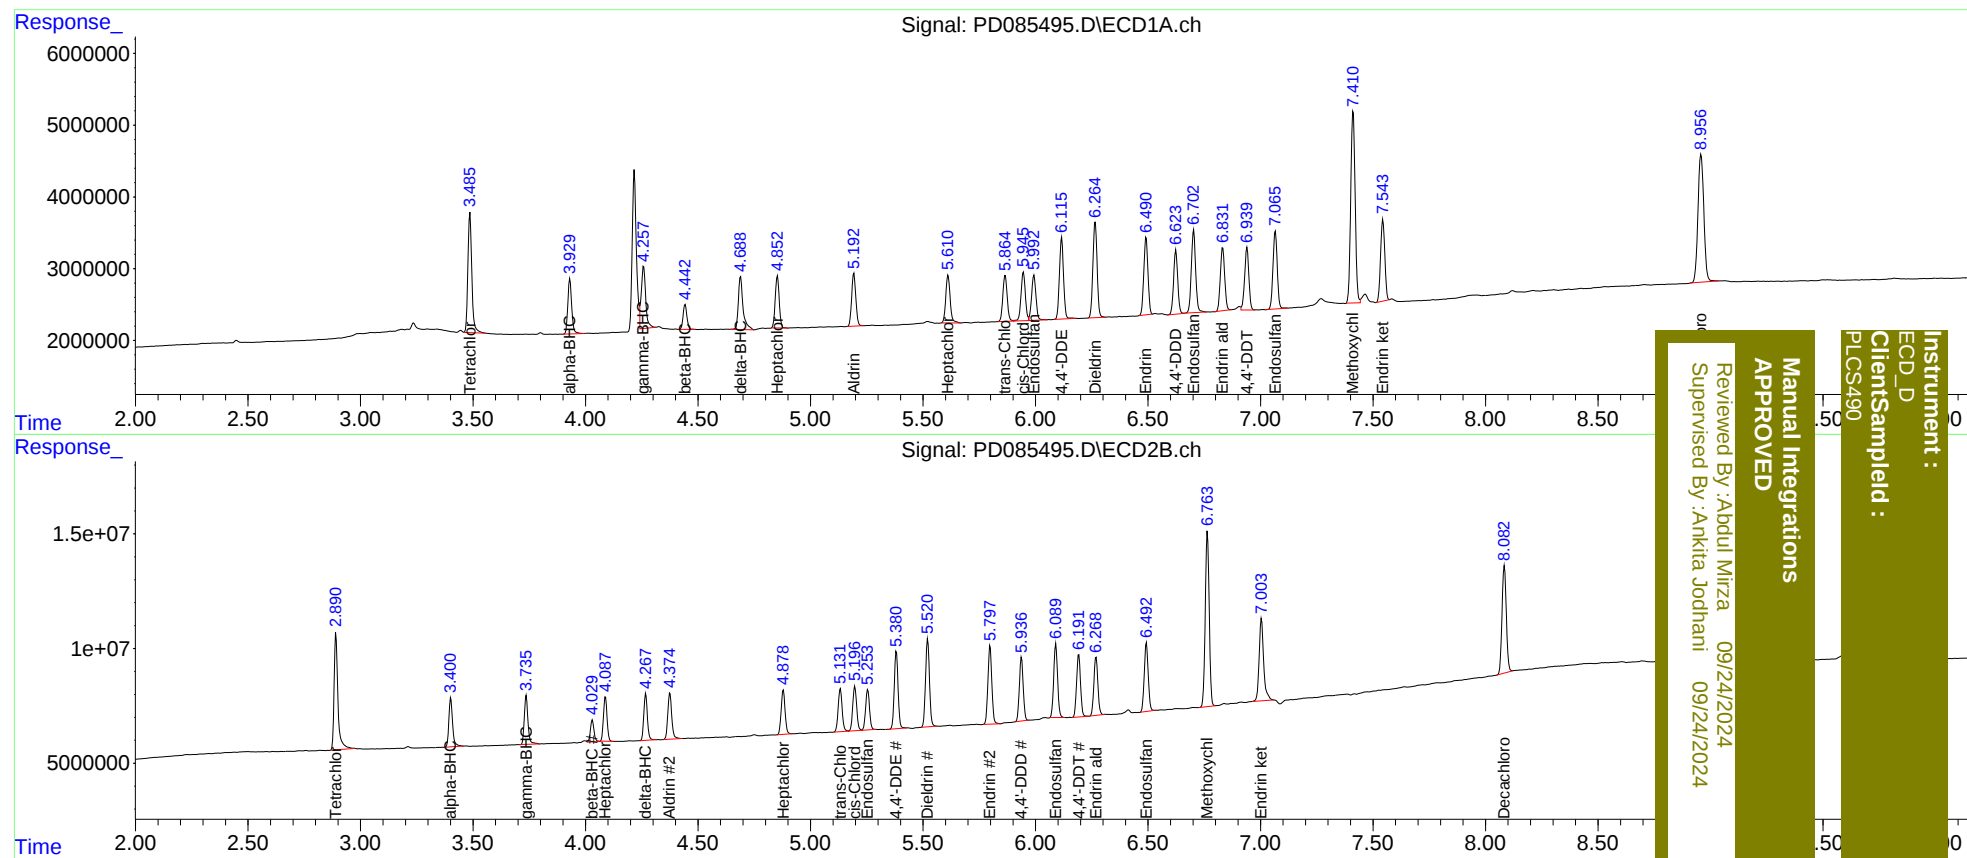

Reviewed By: Abdul Miza 09/24/2024
Supervised By: Ankita Jodhani 09/24/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS490