

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092225\
 Data File : PD090367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2025 11:18
 Operator : AR\AJ
 Sample : PB169574BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK574

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 08:01:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:48:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	49627131	456.3E6	19.038	20.021
27)	SA Decachlor...	9.066	8.062	101.2E6	684.0E6	25.446	27.606
Target Compounds							
3)	MA gamma-BHC...	4.337	0.000	327246	0	<MDL	N.D. #
6)	B beta-BHC	0.000	3.984f	0	14408290	N.D.	0.958
7)	B delta-BHC	4.775	0.000	1267516	0	0.258	N.D. #
9)	A Endosulfan I	6.008f	0.000	538194	0	0.120	N.D. #
10)	B trans-Chl...	6.008f	0.000	538194	0	0.118	N.D. #
11)	B cis-Chlor...	6.008	0.000	538194	0	0.114	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092225\
Data File : PD090367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2025 11:18
Operator : AR\AJ
Sample : PB169574BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 08:01:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:48:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

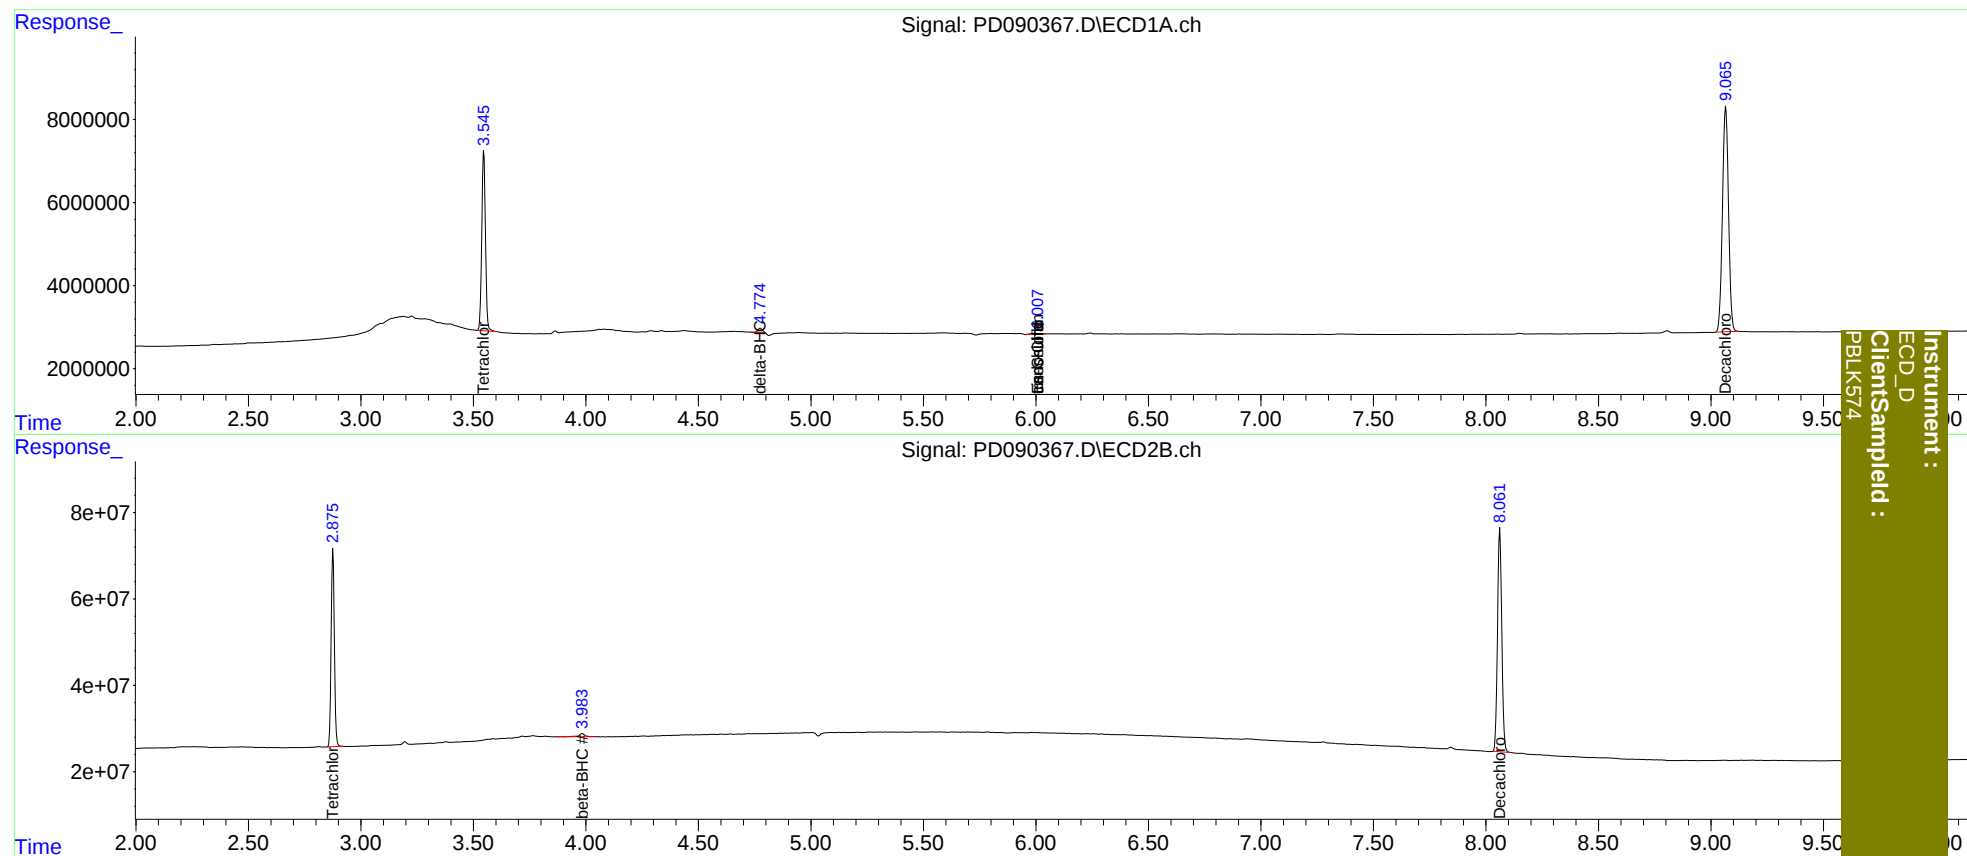


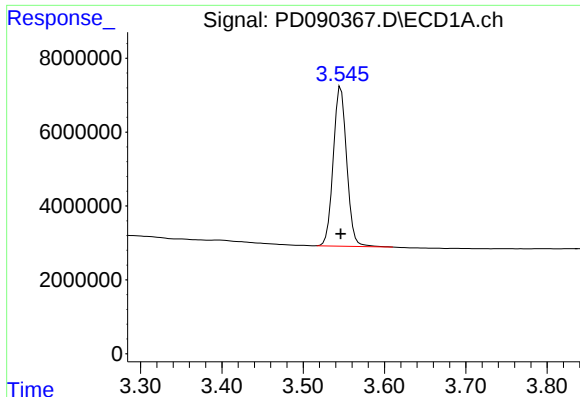

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 49627131
Conc: 19.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK574

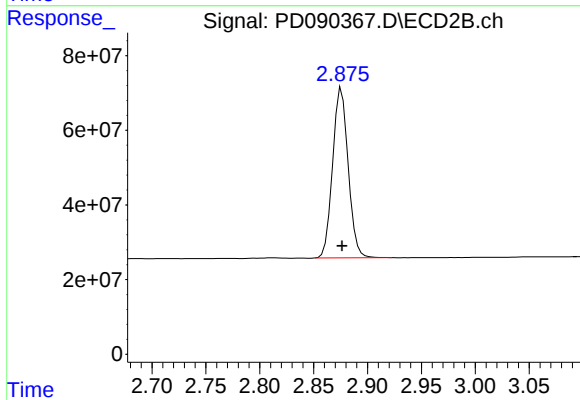


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 456313773
Conc: 20.02 ng/ml

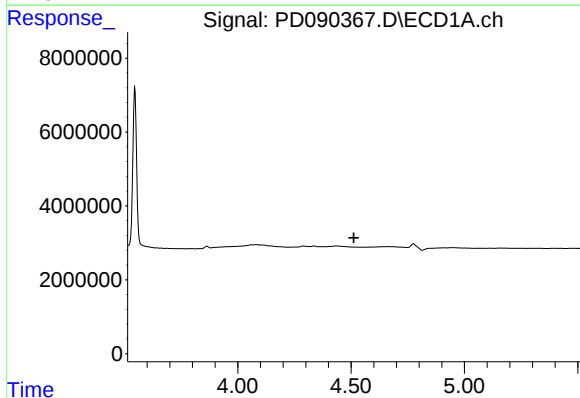


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.513 min
Response: 0
Conc: N.D.

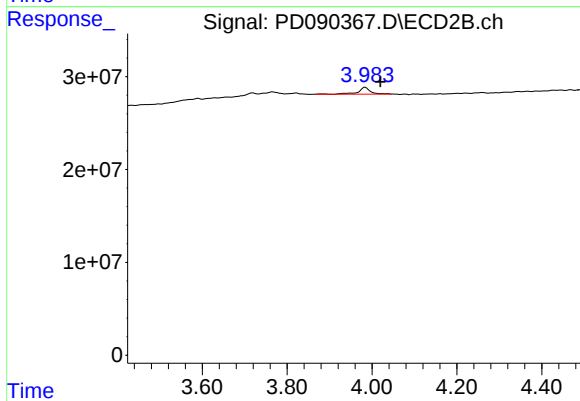

#6 beta-BHC


R.T.: 3.984 min
Delta R.T.: -0.036 min
Response: 14408290
Conc: 0.96 ng/ml

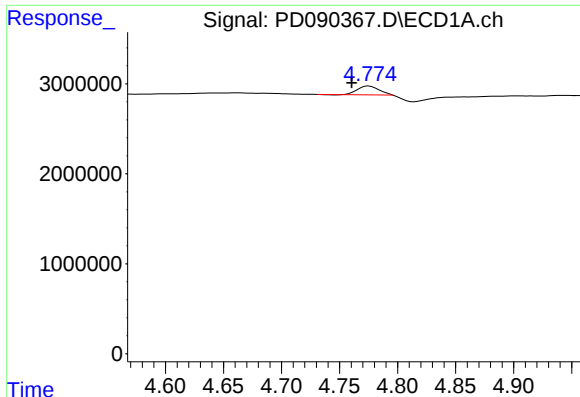

#7 delta-BHC


R.T.: 4.775 min
Delta R.T.: 0.015 min
Response: 1267516
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK574

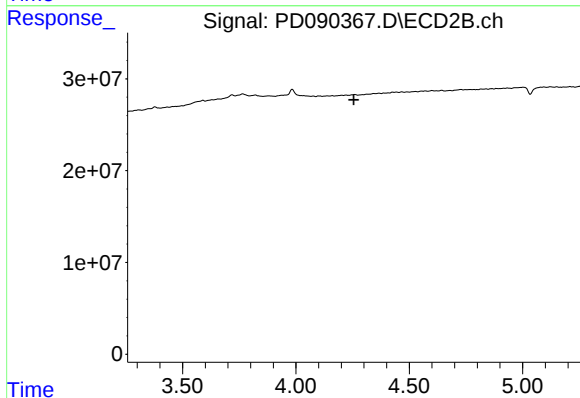


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.256 min
Response: 0
Conc: N.D.

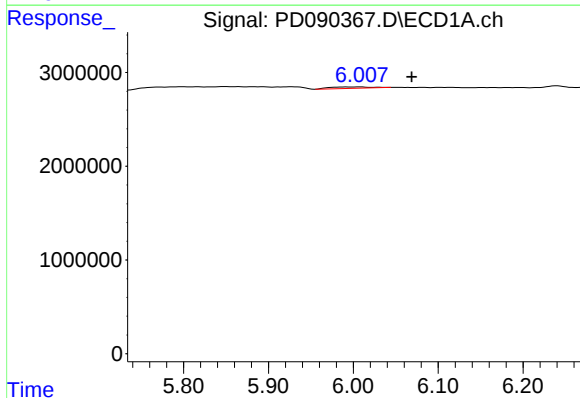


#9 Endosulfan I

R.T.: 6.008 min
Delta R.T.: -0.061 min
Response: 538194
Conc: 0.12 ng/ml

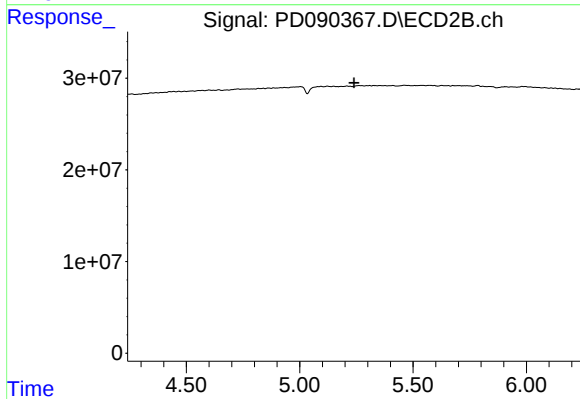

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

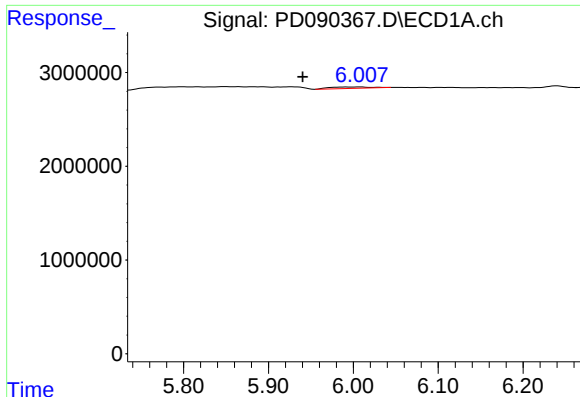

#10 trans-Chlordane


R.T.: 6.008 min
Delta R.T.: 0.067 min
Response: 538194
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK574

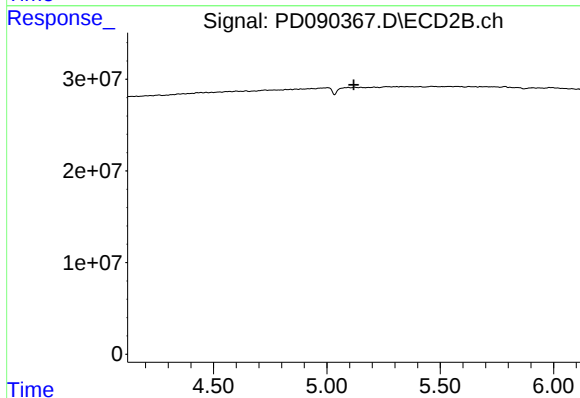


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

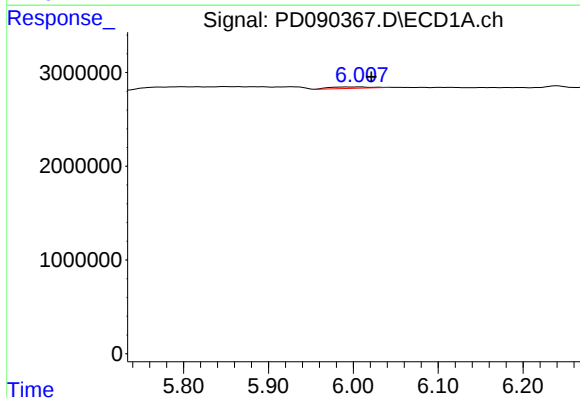


#11 cis-Chlordane

R.T.: 6.008 min
Delta R.T.: -0.014 min
Response: 538194
Conc: 0.11 ng/ml

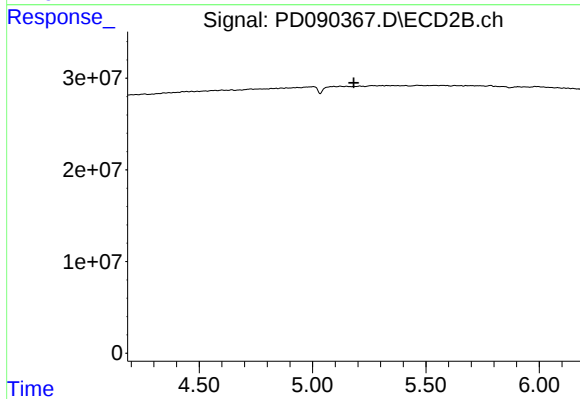

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

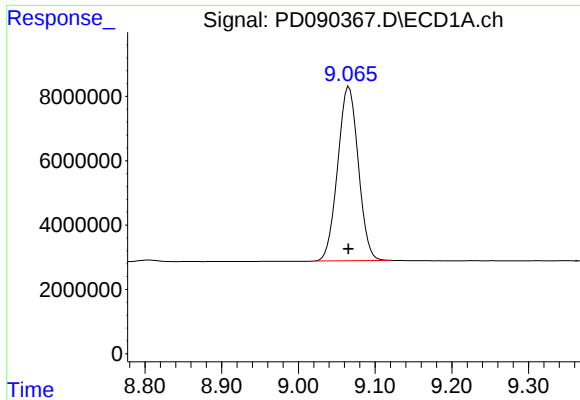

#27 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 101201246
Conc: 25.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK574

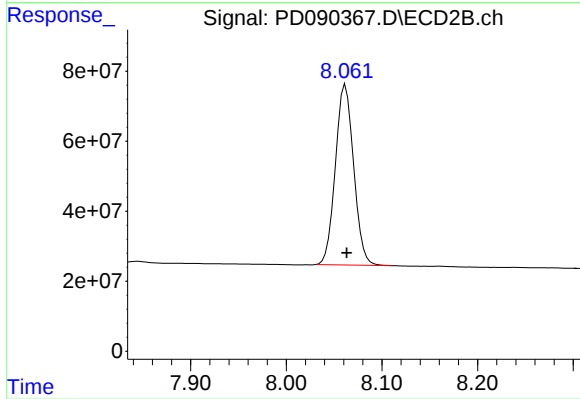

#27 Decachlorobiphenyl

R.T.: 8.062 min
Delta R.T.: -0.001 min
Response: 684034201
Conc: 27.61 ng/ml