

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
 Data File : PD049362.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2018 2:57
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:39:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 24 01:38:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.913	26989331	231.9E6	24.490	25.963
28)	SA Decachlor...	7.953	8.903	27324499	85743460	25.083	25.714
Target Compounds							
23)	Chlordane-1	4.133	4.890	12007977	107.4E6	248.095	257.433
24)	Chlordane-2	4.619	5.351	12842820	103.6E6	248.492m	261.830
25)	Chlordane-3	5.171	5.987	40387649	335.6E6	246.777	257.490
26)	Chlordane-4	5.228	6.063	36772401	394.1E6	242.505	259.629
27)	Chlordane-5	6.048	6.853	13497094	77617762	250.177	255.677



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
Data File : PD049362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2018 2:57
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:39:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
Quant Title : GC Extractables
QLast Update : Mon Sep 24 01:38:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

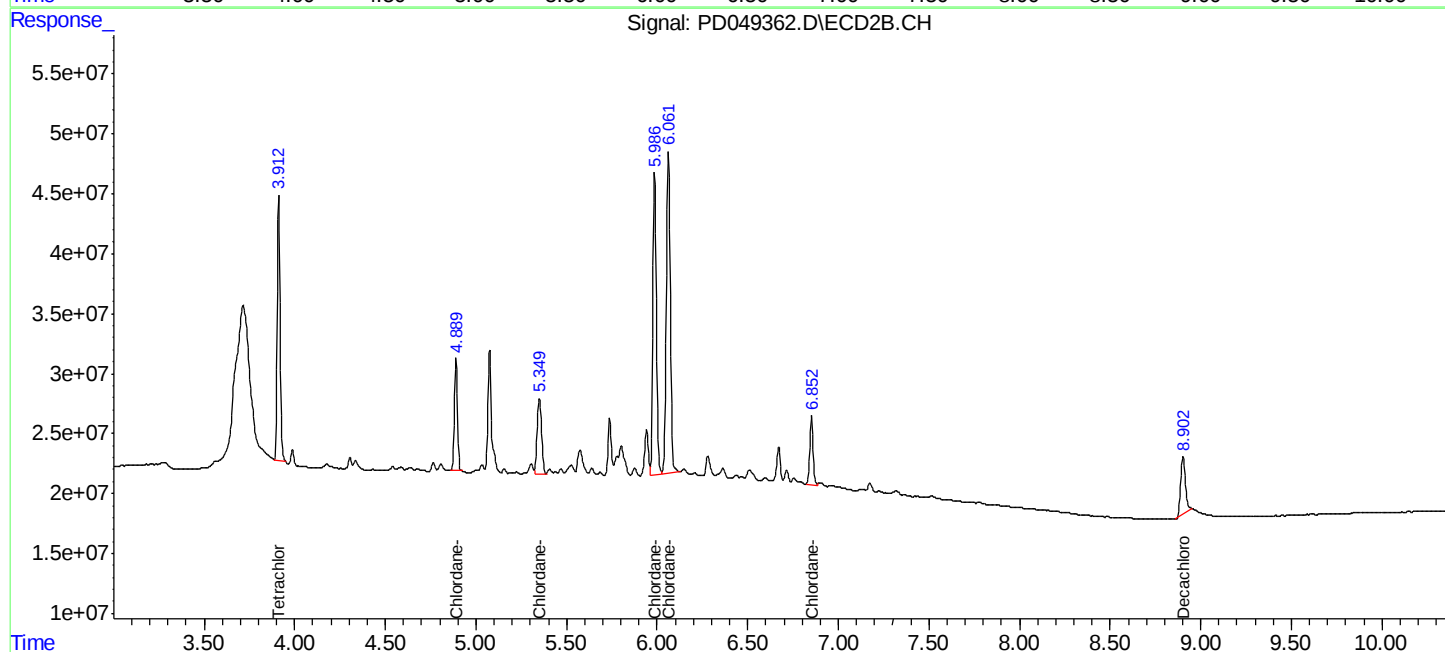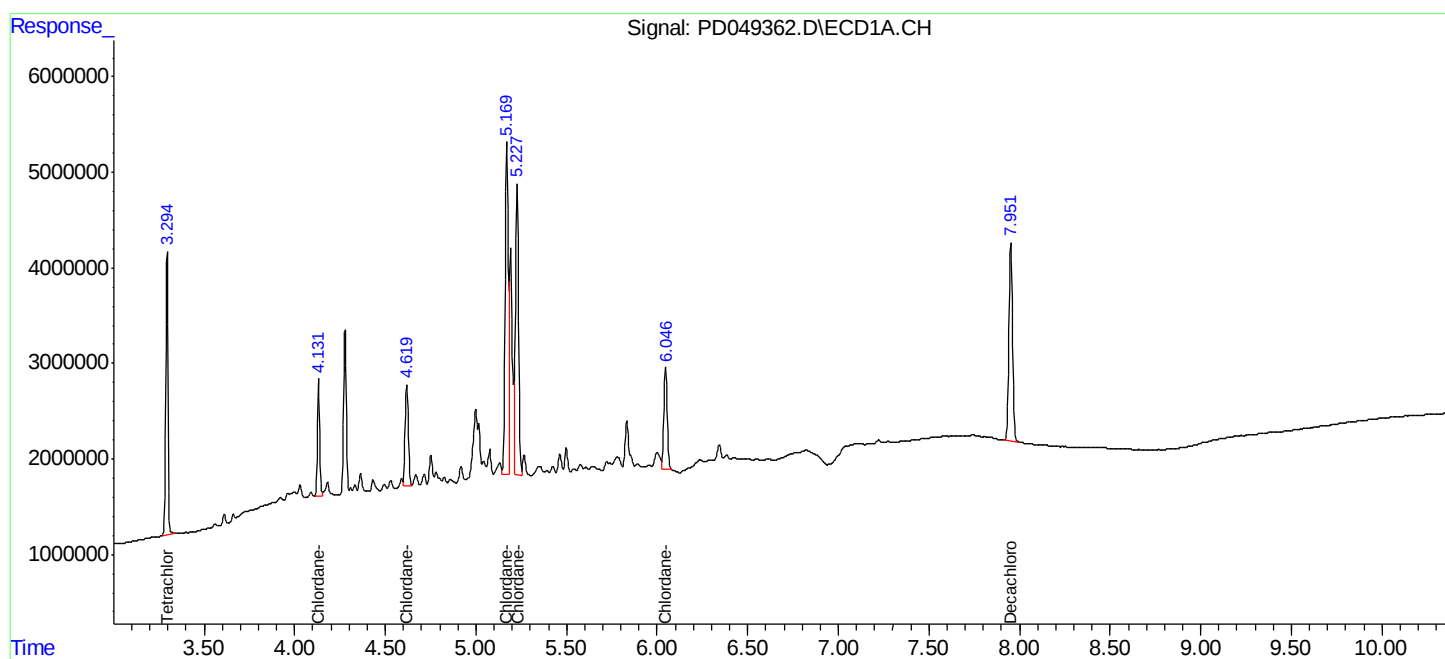


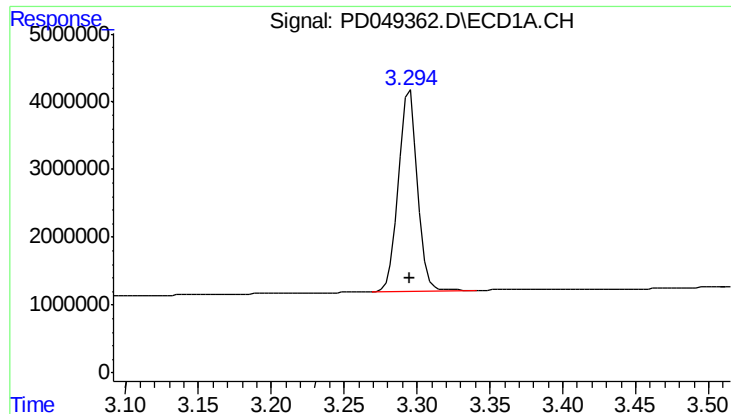

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 26989331
Conc: 24.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

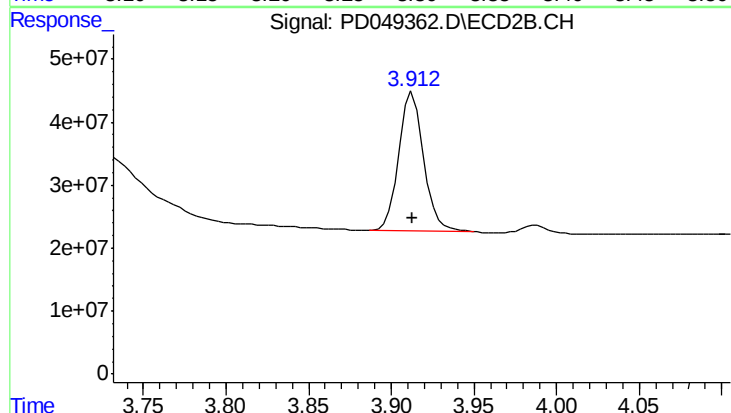


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 231892136
Conc: 25.96 ng/ml

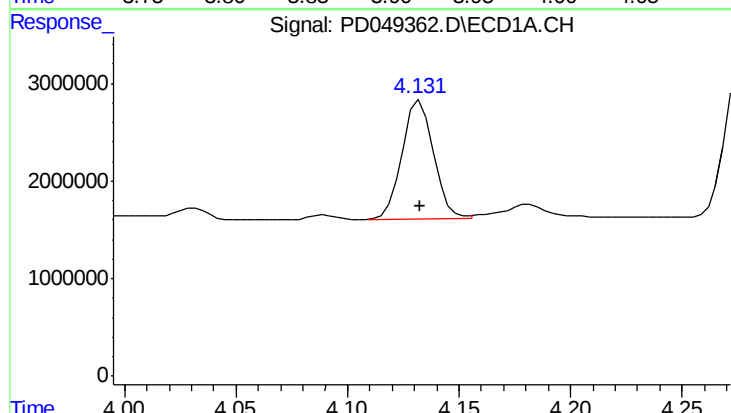


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 12007977
Conc: 248.10 ng/ml

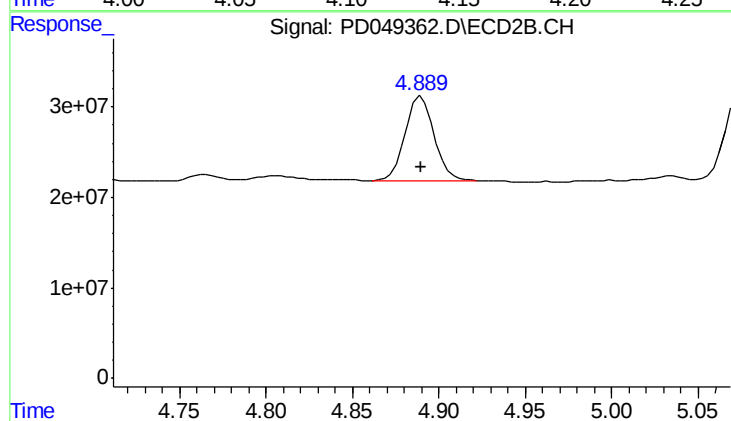

#23 Chlordane-1


R.T.: 4.890 min
Delta R.T.: 0.000 min
Response: 107393050
Conc: 257.43 ng/ml

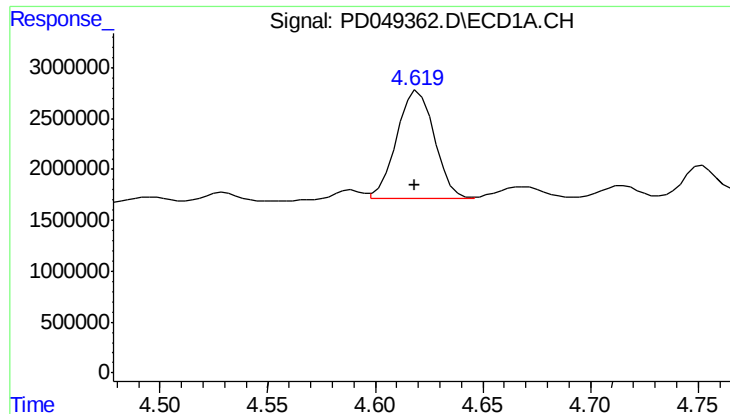

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 12842820
Conc: 248.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

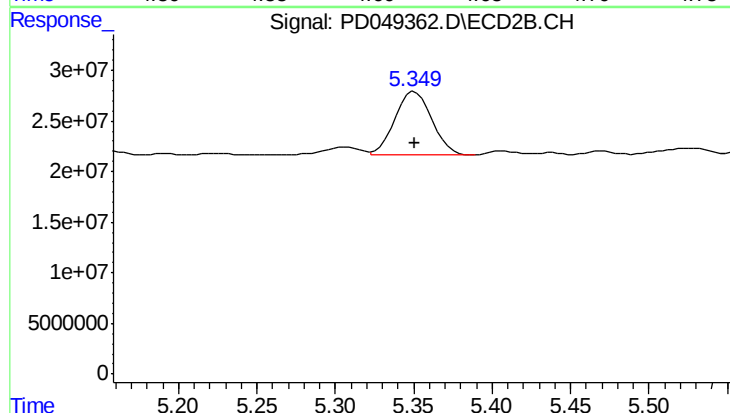


#24 Chlordane-2

R.T.: 5.351 min
Delta R.T.: 0.000 min
Response: 103649809
Conc: 261.83 ng/ml

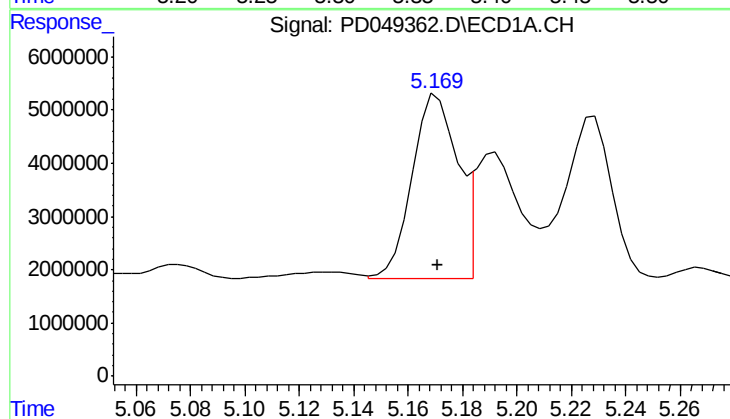


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 40387649
Conc: 246.78 ng/ml

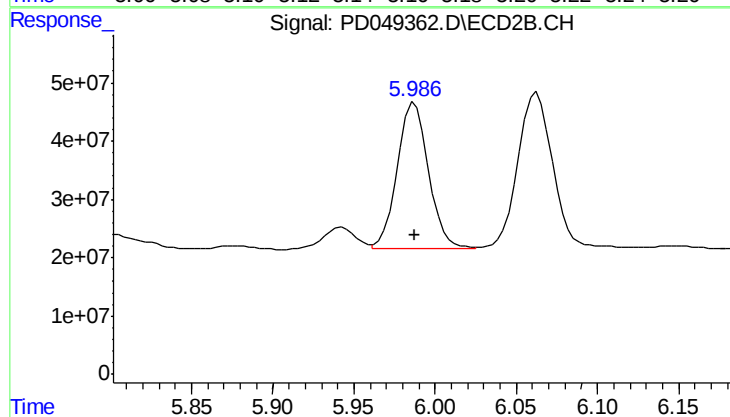

#25 Chlordane-3


R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 335647257
Conc: 257.49 ng/ml

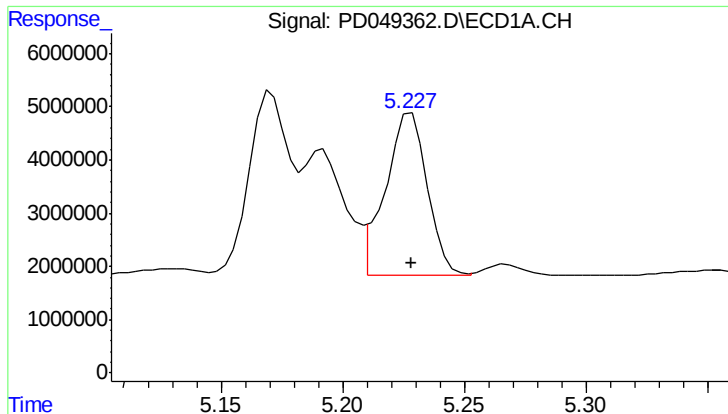

#26 Chlordane-4


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 36772401
Conc: 242.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

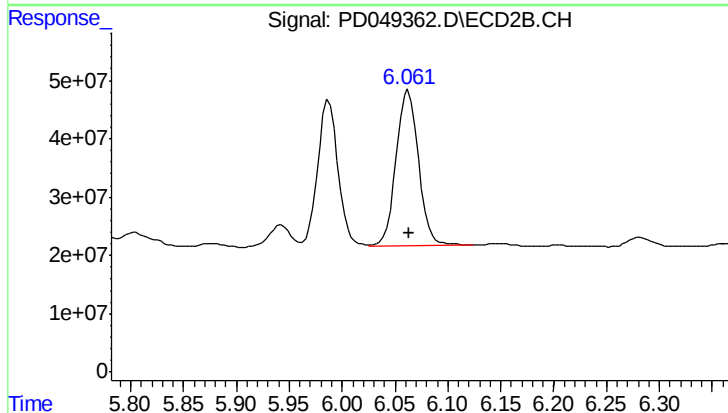


#26 Chlordane-4

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 394071988
Conc: 259.63 ng/ml

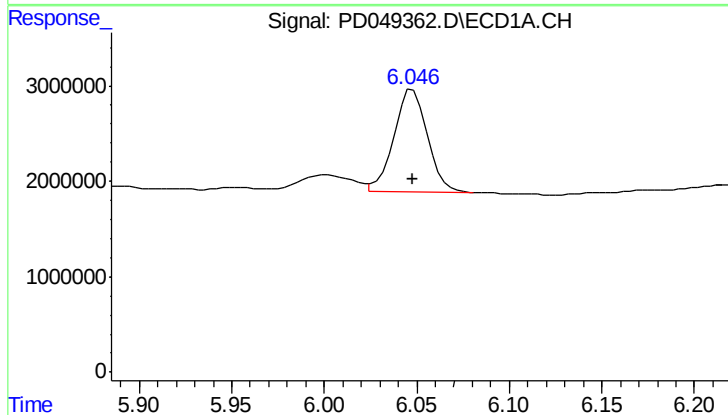


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 13497094
Conc: 250.18 ng/ml

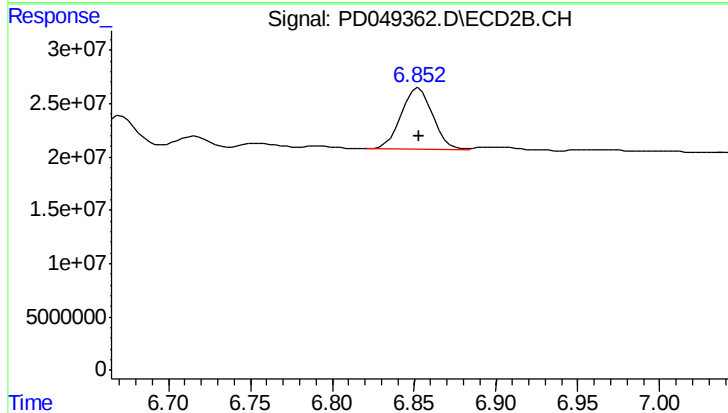

#27 Chlordane-5


R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 77617762
Conc: 255.68 ng/ml

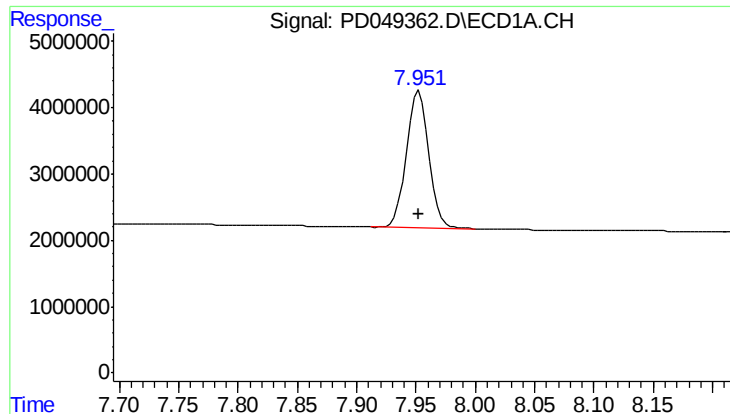

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.000 min
Response: 27324499
Conc: 25.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

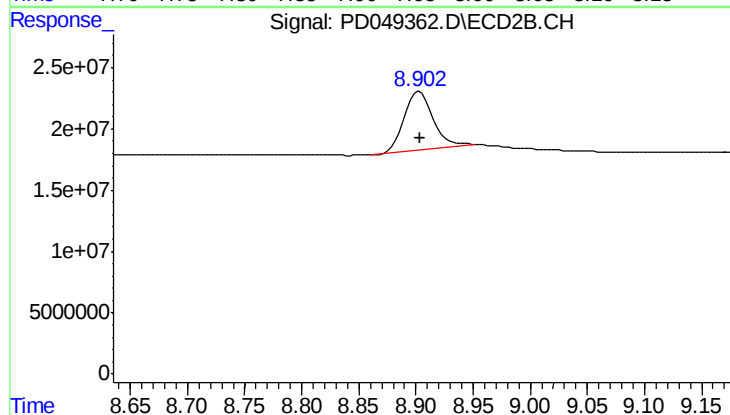

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.000 min
Response: 85743460
Conc: 25.71 ng/ml