

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
 Data File : PD049363.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2018 3:11
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:41:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 24 01:40:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.295	3.913	5884880	51022248	5.268	5.554
28) SA Decachlor...	7.953	8.903	5906875	19052297	5.332	5.555
Target Compounds						
23) Chlordane-1	4.133	4.891	2370795	22496111	49.183	53.092
24) Chlordane-2	4.619	5.351	2853448	24286335	53.949m	58.685
25) Chlordane-3	5.171	5.988	8240380	75290894	50.280	56.020
26) Chlordane-4	5.228	6.063	7678830	89420894	50.511	56.886
27) Chlordane-5	6.046	6.854	2525092	16610953	47.113m	53.704



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
Data File : PD049363.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2018 3:11
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:41:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
Quant Title : GC Extractables
QLast Update : Mon Sep 24 01:40:42 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

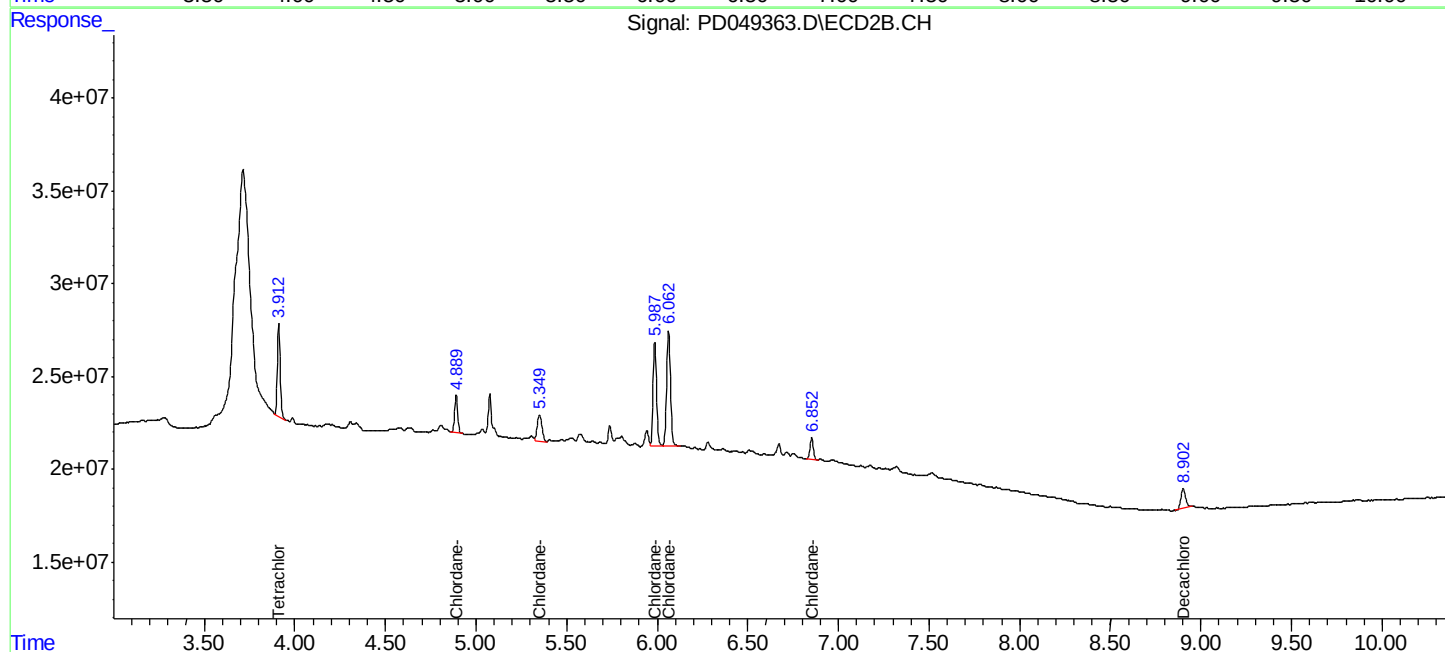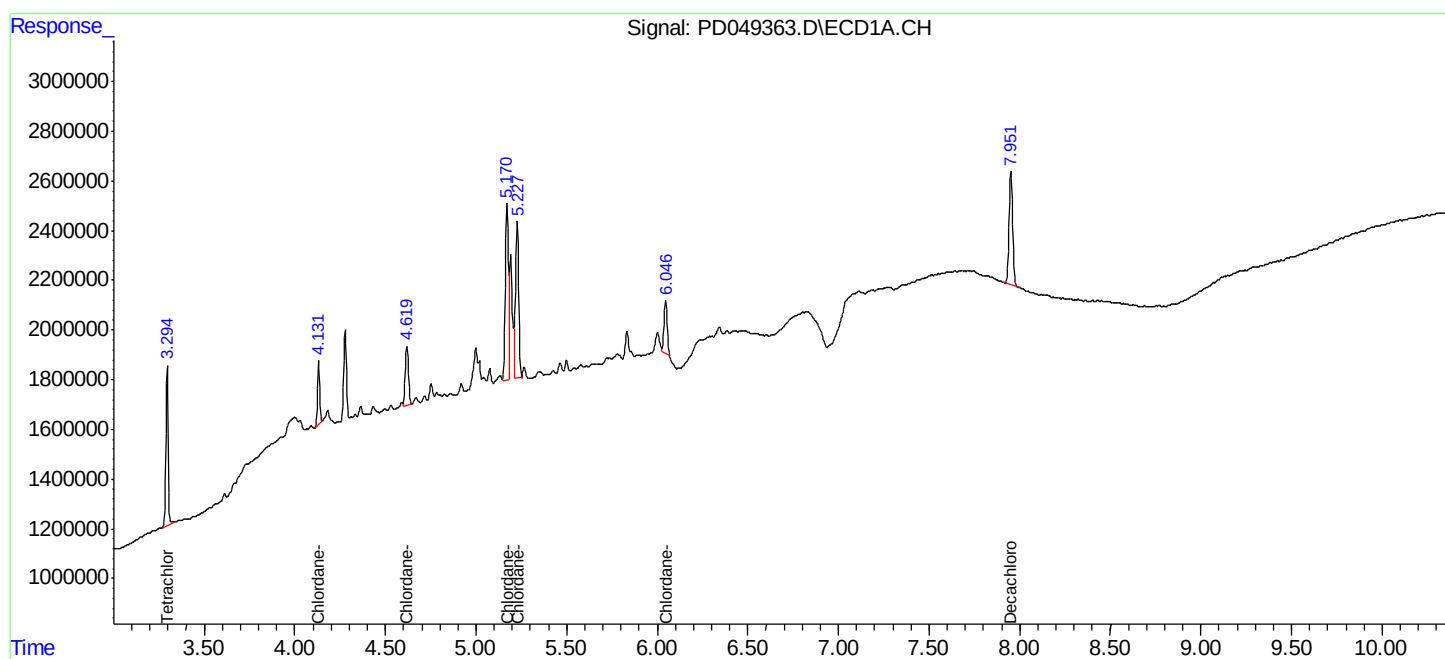


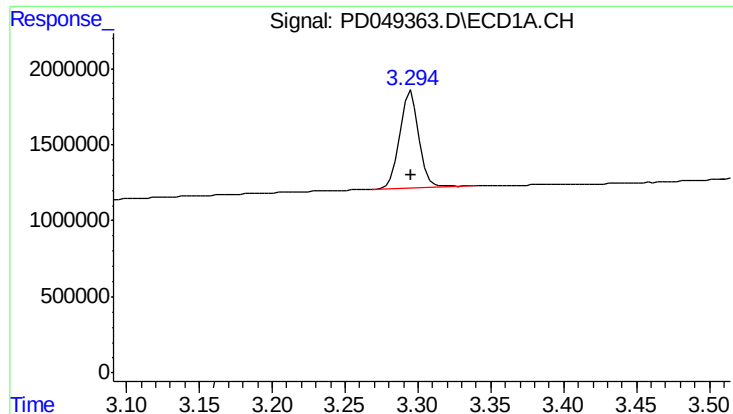

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 5884880
Conc: 5.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

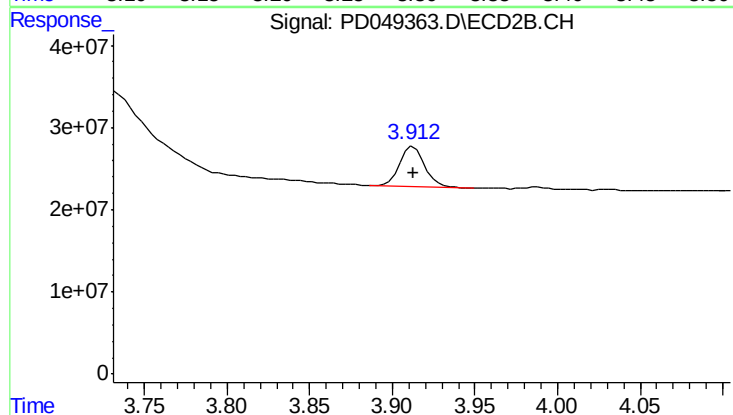


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 51022248
Conc: 5.55 ng/ml

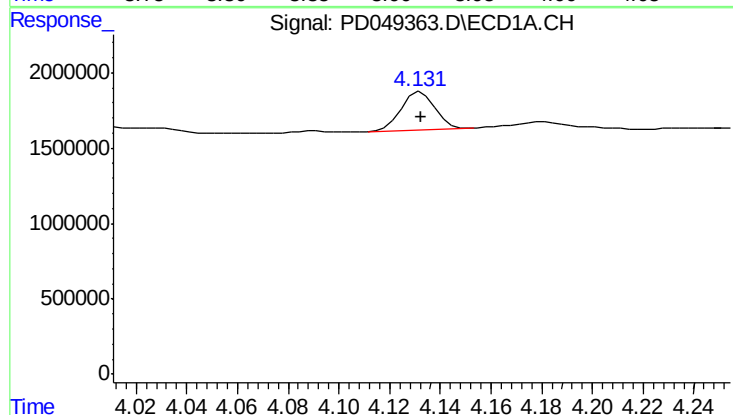


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 2370795
Conc: 49.18 ng/ml

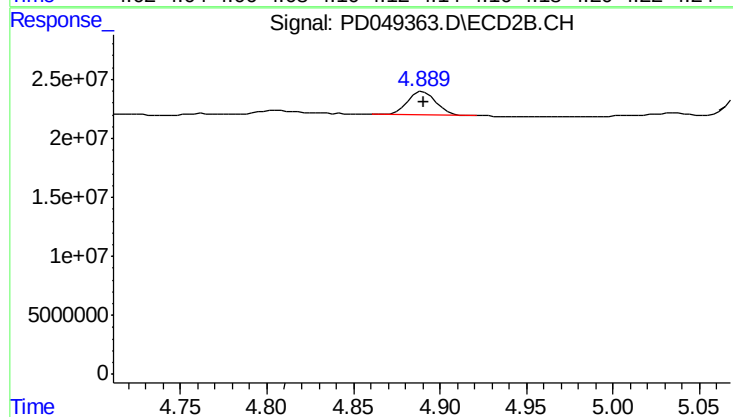

#23 Chlordane-1


R.T.: 4.891 min
Delta R.T.: 0.000 min
Response: 22496111
Conc: 53.09 ng/ml

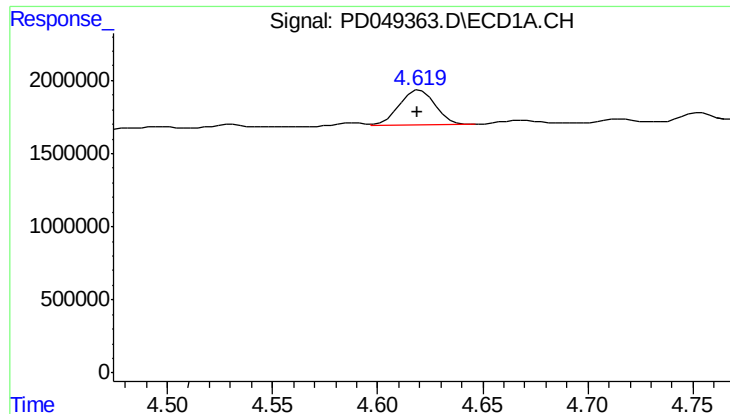

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 2853448
Conc: 53.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

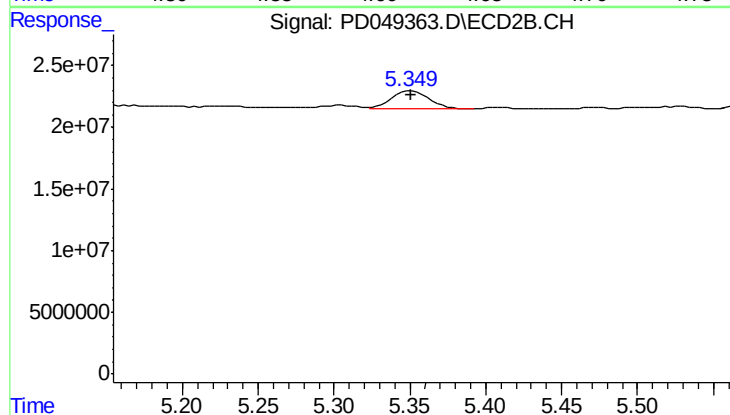


#24 Chlordane-2

R.T.: 5.351 min
Delta R.T.: 0.000 min
Response: 24286335
Conc: 58.69 ng/ml

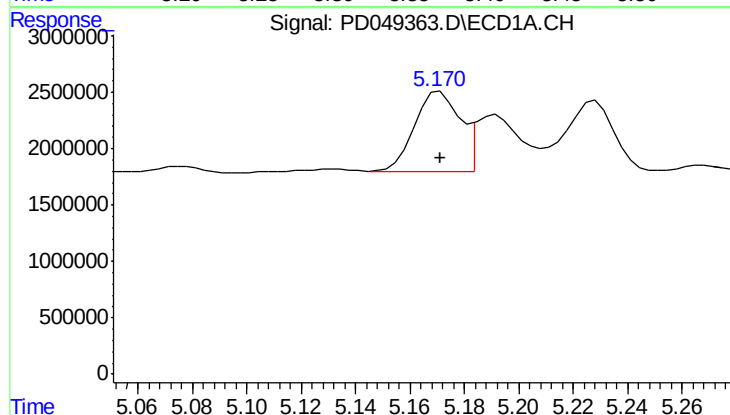


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 8240380
Conc: 50.28 ng/ml

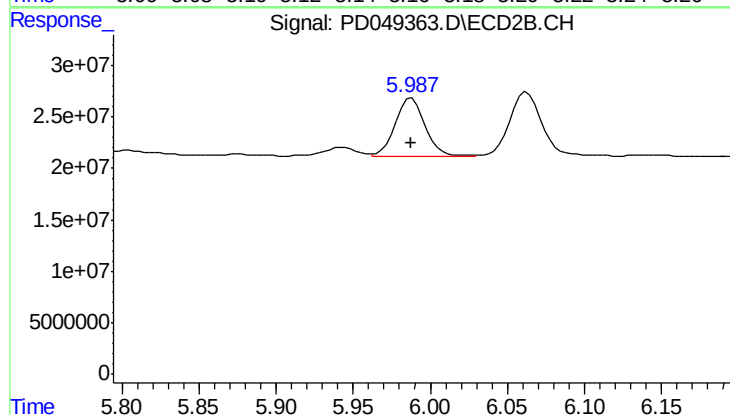

#25 Chlordane-3


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 75290894
Conc: 56.02 ng/ml

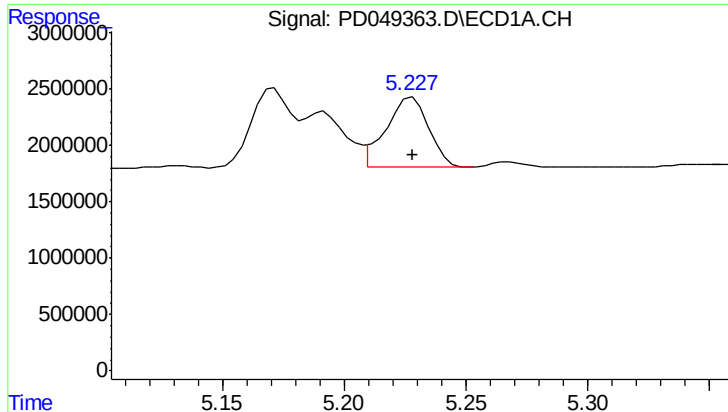

#26 Chlordane-4


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 7678830
Conc: 50.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

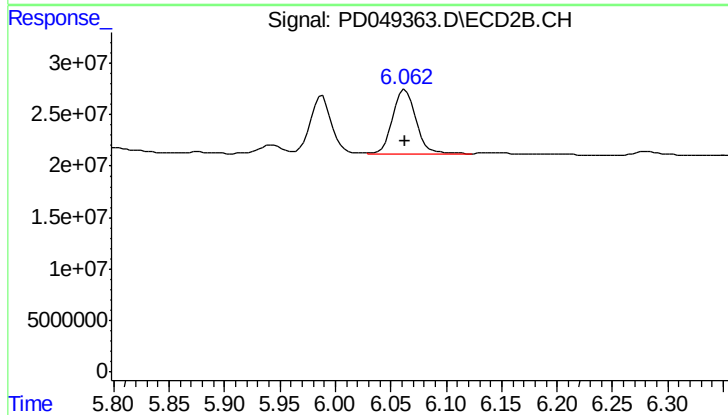


#26 Chlordane-4

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 89420894
Conc: 56.89 ng/ml

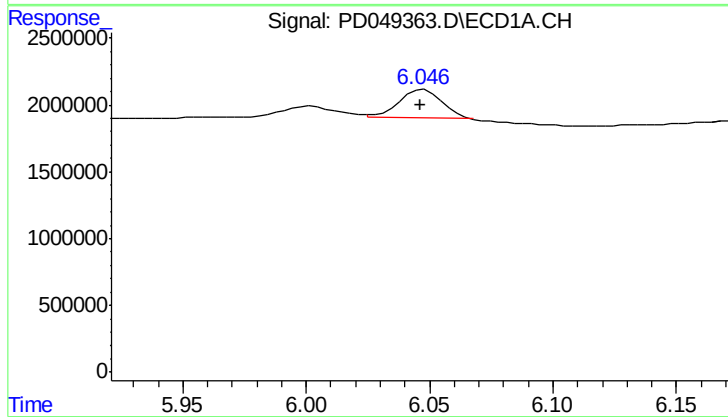


#27 Chlordane-5

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 2525092
Conc: 47.11 ng/ml m

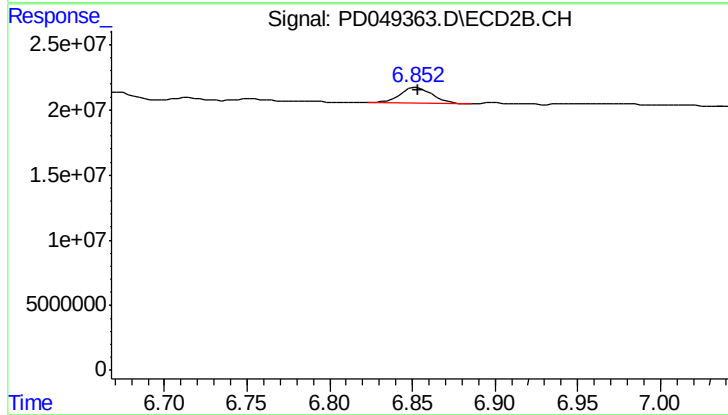

#27 Chlordane-5


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 16610953
Conc: 53.70 ng/ml

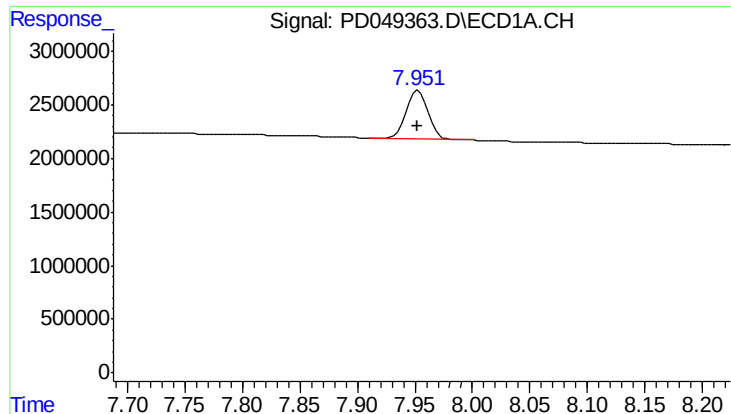

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.000 min
Response: 5906875
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

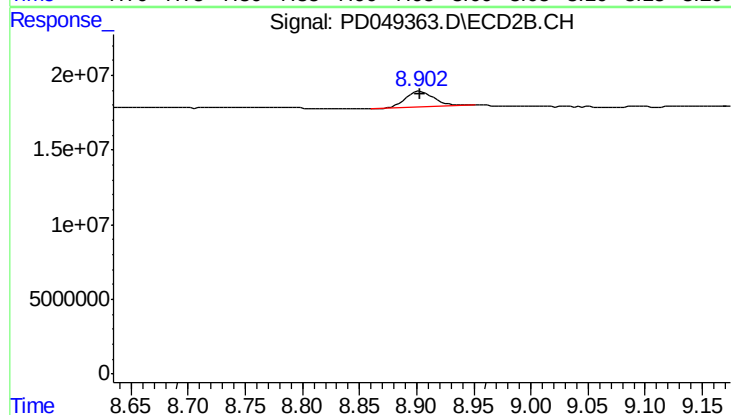

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.000 min
Response: 19052297
Conc: 5.56 ng/ml