

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
 Data File : PD049370.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2018 4:49
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD092318CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:42:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 24 01:41:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.295	3.913	55532871	452.2E6	49.714	49.228
28) SA Decachlor...	7.952	8.902	54668162	165.8E6	49.349	48.332
Target Compounds						
23) Chlordane-1	4.132	4.890	24561210	212.2E6	509.530	500.903
24) Chlordane-2	4.619	5.350	26447205	202.5E6	501.299	489.386
25) Chlordane-3	5.170	5.987	84520325	661.2E6	515.714	491.938
26) Chlordane-4	5.227	6.062	76137215	769.2E6	500.824	489.341
27) Chlordane-5	6.047	6.852	27072730	154.5E6	508.308	499.583



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
Data File : PD049370.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2018 4:49
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD092318CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:42:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
Quant Title : GC Extractables
QLast Update : Mon Sep 24 01:41:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

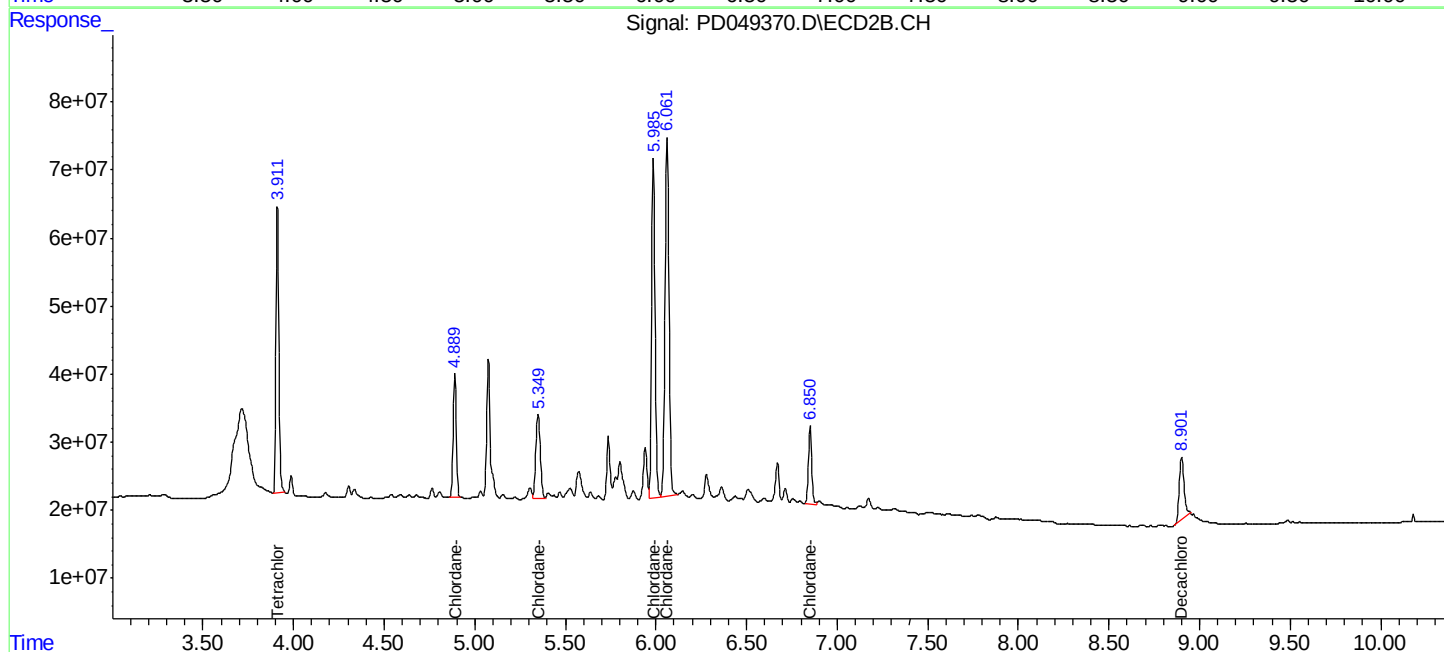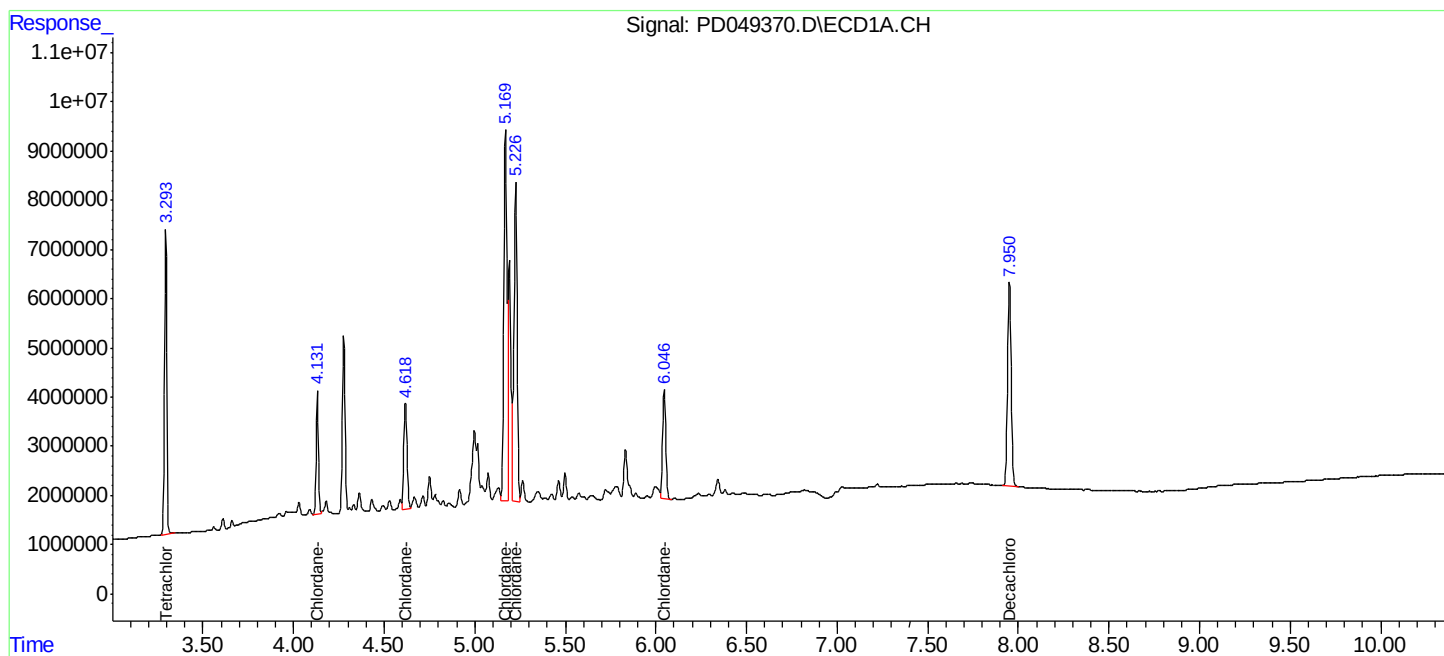


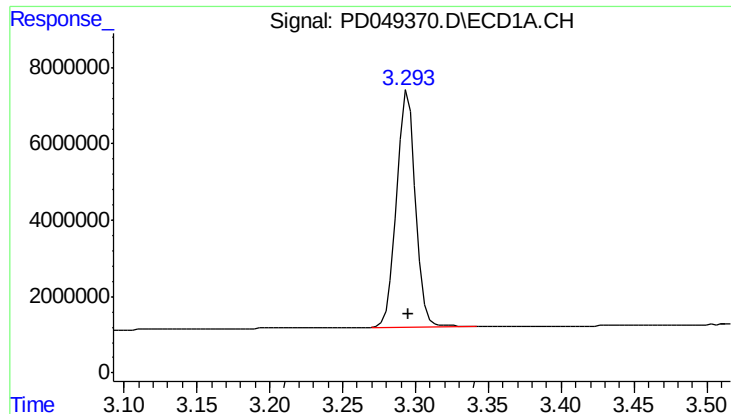

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 55532871
Conc: 49.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092318CHLOR

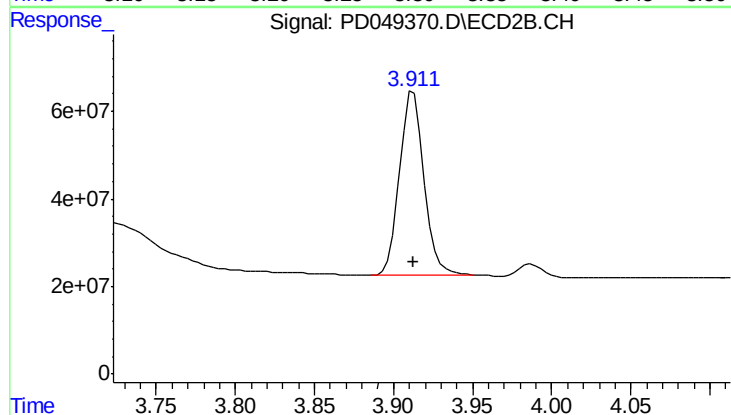


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 452223033
Conc: 49.23 ng/ml

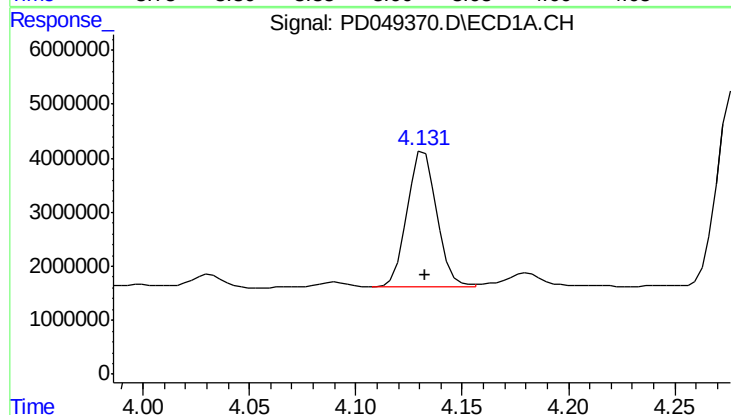


#23 Chlordane-1

R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 24561210
Conc: 509.53 ng/ml

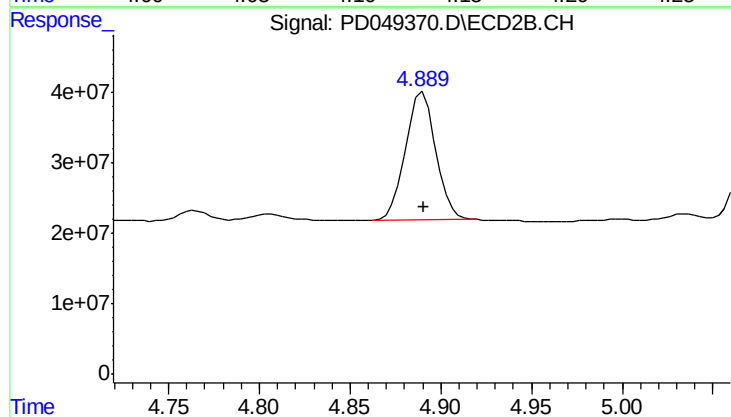

#23 Chlordane-1


R.T.: 4.890 min
Delta R.T.: 0.000 min
Response: 212241958
Conc: 500.90 ng/ml

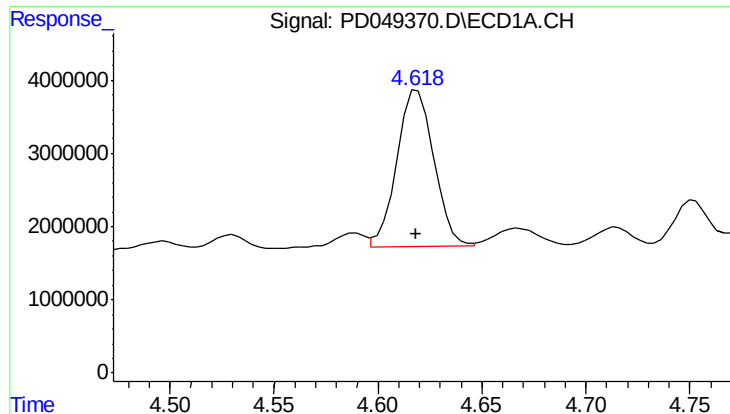

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 26447205
Conc: 501.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092318CHLOR

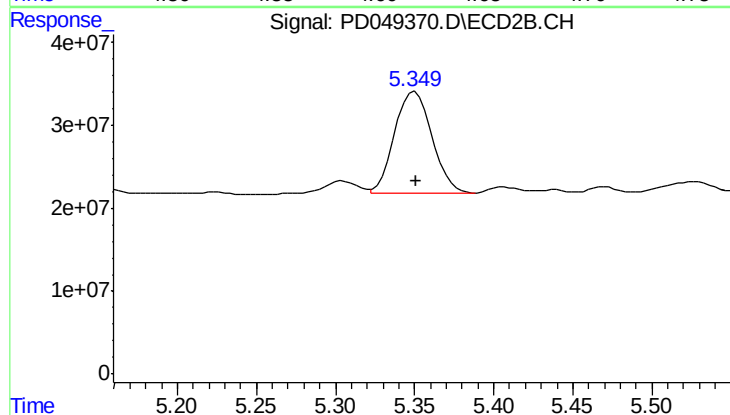


#24 Chlordane-2

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 202527145
Conc: 489.39 ng/ml

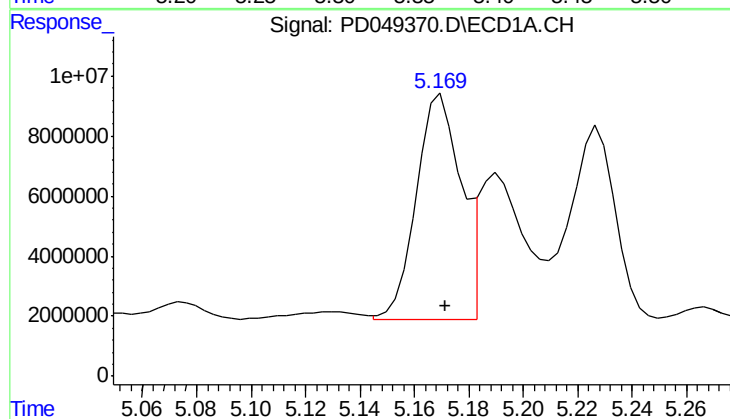


#25 Chlordane-3

R.T.: 5.170 min
Delta R.T.: -0.001 min
Response: 84520325
Conc: 515.71 ng/ml

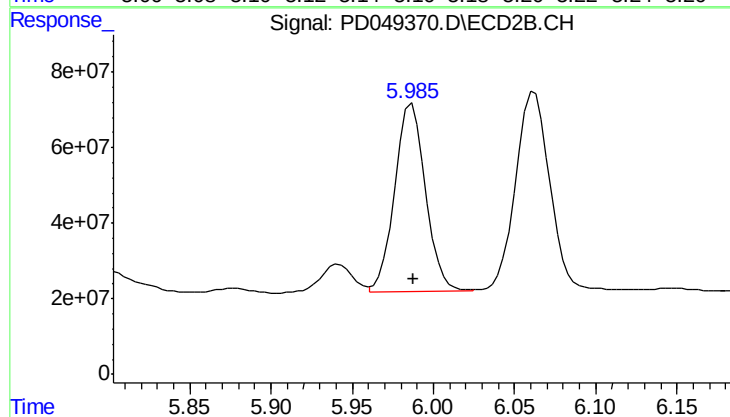

#25 Chlordane-3


R.T.: 5.987 min
Delta R.T.: -0.001 min
Response: 661160084
Conc: 491.94 ng/ml

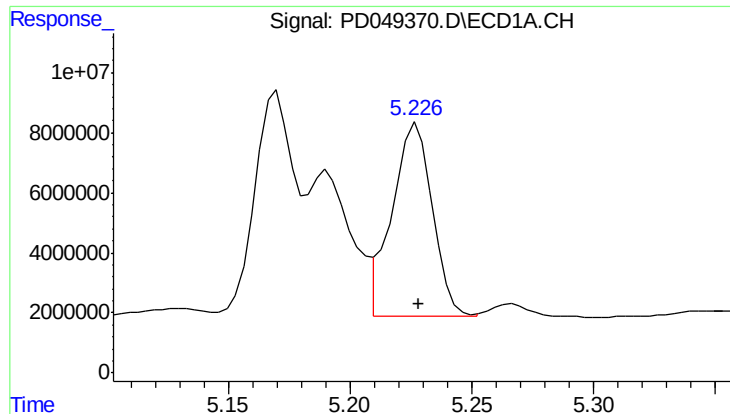

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 76137215
Conc: 500.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092318CHLOR

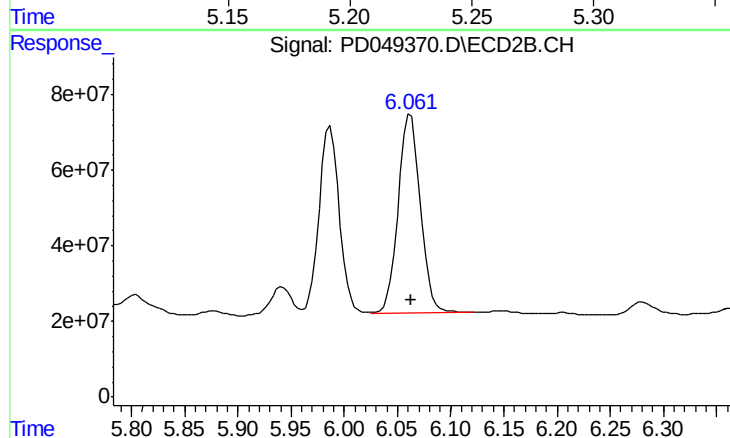


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 769217342
Conc: 489.34 ng/ml

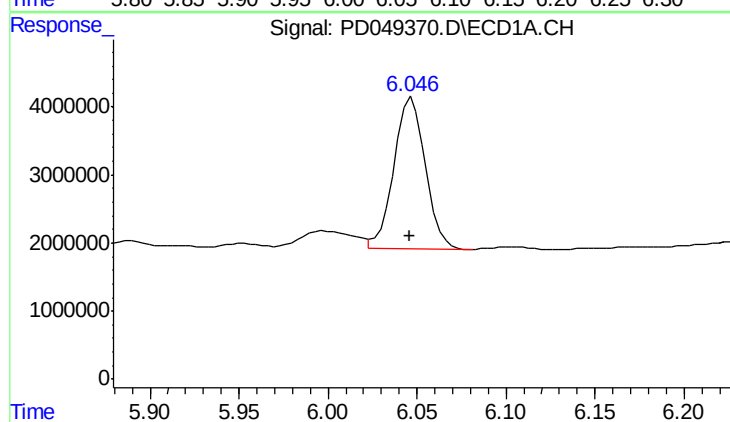


#27 Chlordane-5

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 27072730
Conc: 508.31 ng/ml

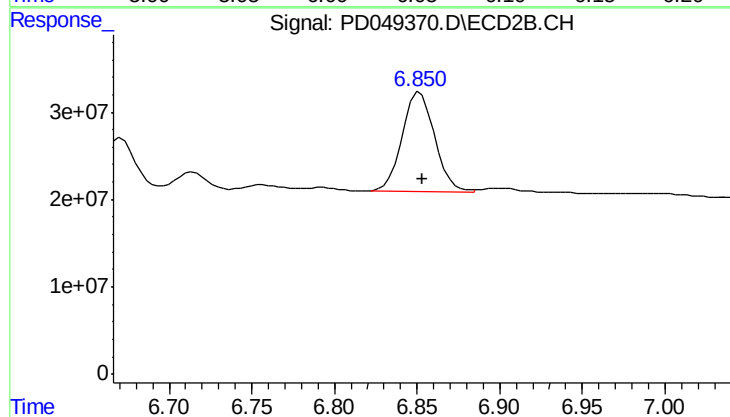

#27 Chlordane-5


R.T.: 6.852 min
Delta R.T.: -0.002 min
Response: 154523744
Conc: 499.58 ng/ml

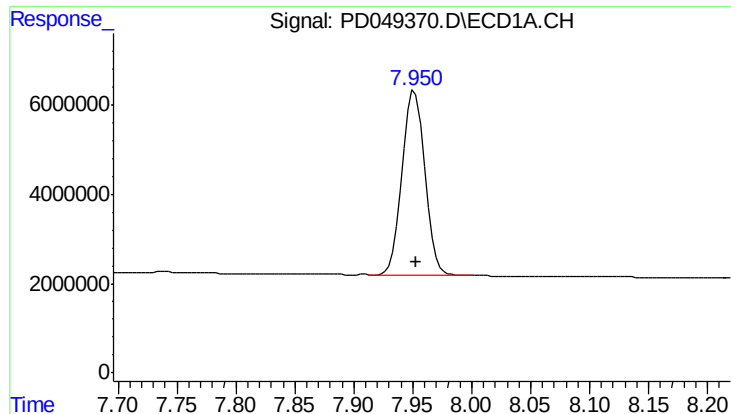

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 54668162
Conc: 49.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD092318CHLOR

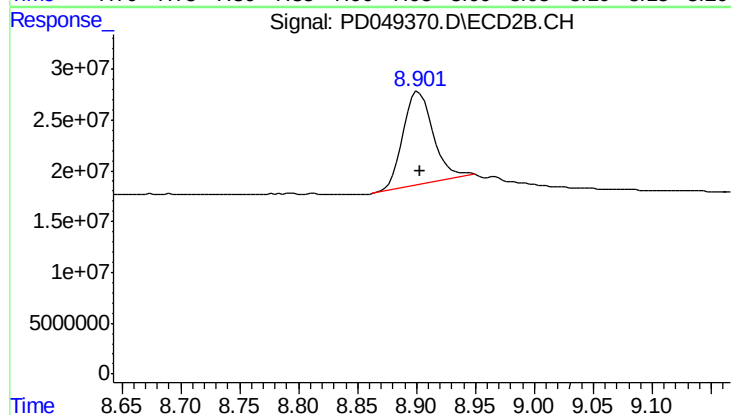

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: -0.001 min
Response: 165763450
Conc: 48.33 ng/ml