

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
 Data File : PD049382.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2018 7:36
 Operator : AJ\SJ
 Sample : PB113034BS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB113034BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:28:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 24 01:44:23 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.912	18265280	153.3E6	18.177	17.076
28)	SA Decachlor...	7.950	8.901	19721295	63123958	18.238	18.727
Target Compounds							
23)	Chlordane-1	4.131	4.888	3868315	35213195	80.249	83.105m
24)	Chlordane-2	4.617	5.349	4676508	34984879	88.642m	84.537
25)	Chlordane-3	5.168	5.985	11890097	107.8E6	72.549m	80.228m
26)	Chlordane-4	5.226	6.061	11955141	132.0E6	78.640	83.983
27)	Chlordane-5	6.044	6.850	4643608	24815908	87.187m	80.231m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
Data File : PD049382.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2018 7:36
Operator : AJ\SJ
Sample : PB113034BS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB113034BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:28:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
Quant Title : GC Extractables
QLast Update : Mon Sep 24 01:44:23 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

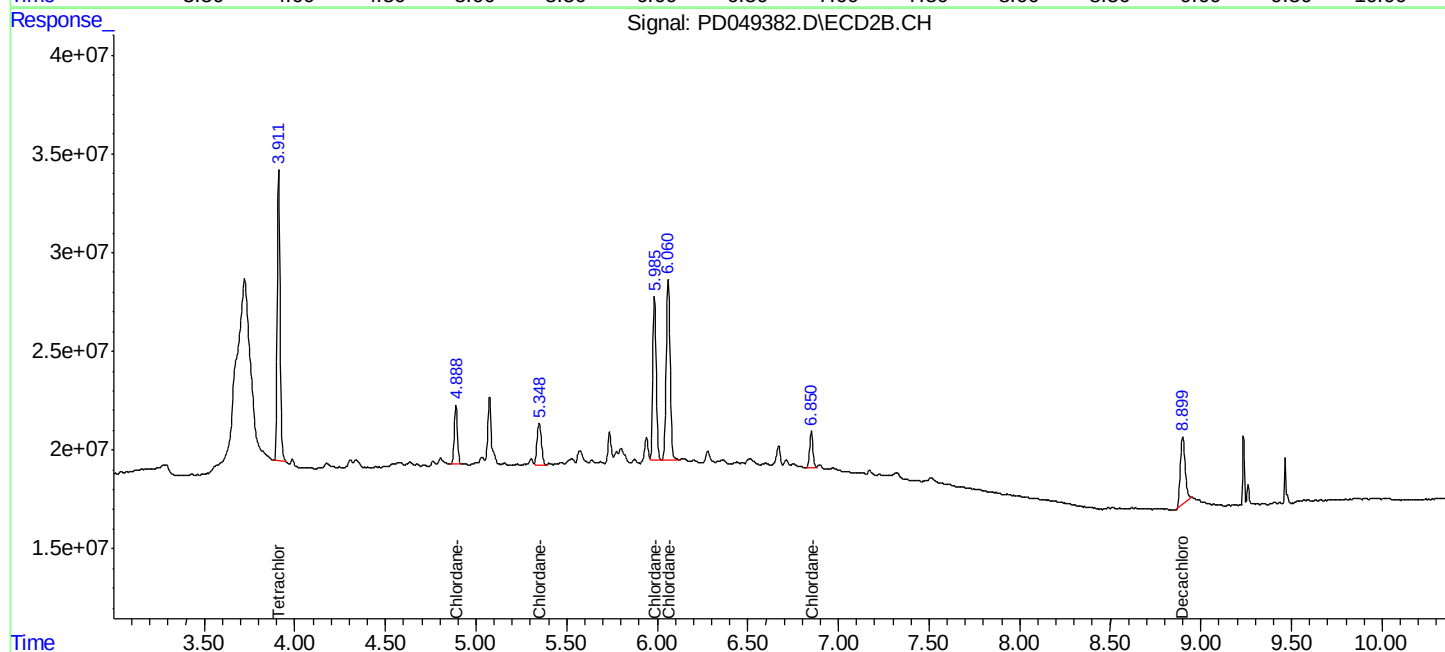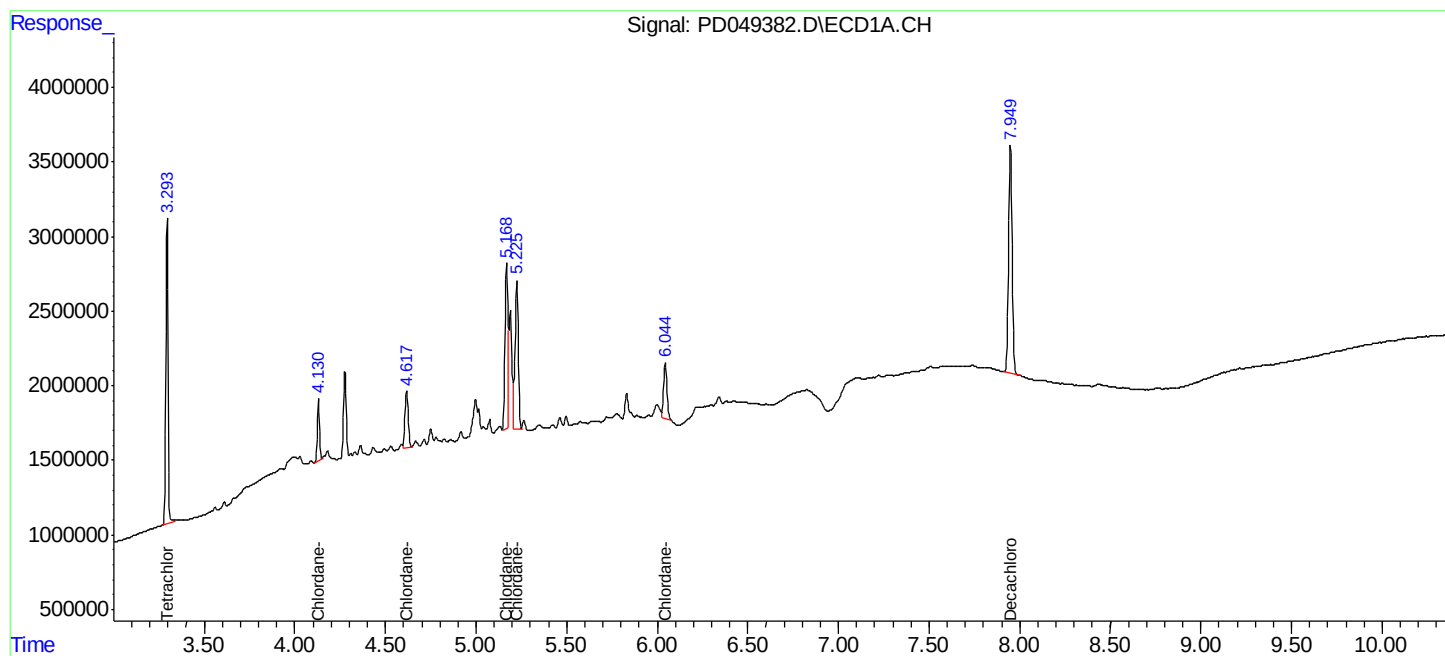


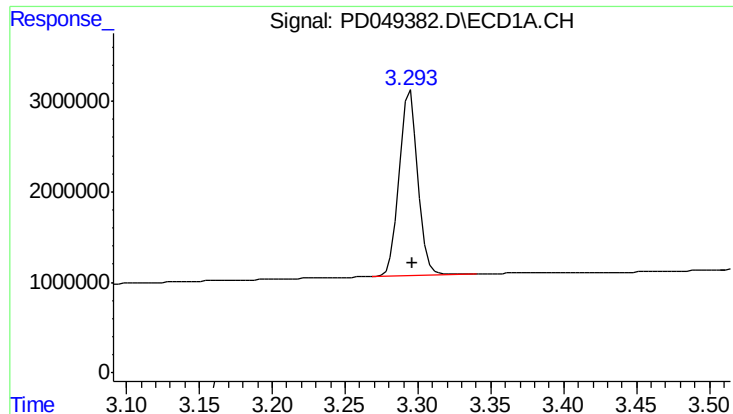

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: -0.001 min
Response: 18265280
Conc: 18.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB113034BS

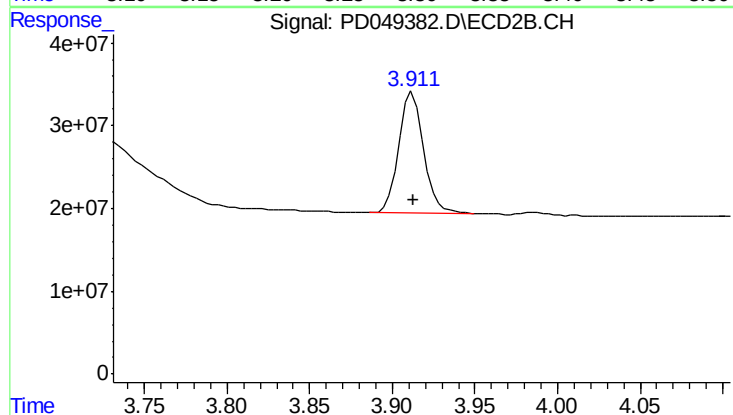


#1 Tetrachloro-m-xylene

R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 153310819
Conc: 17.08 ng/ml

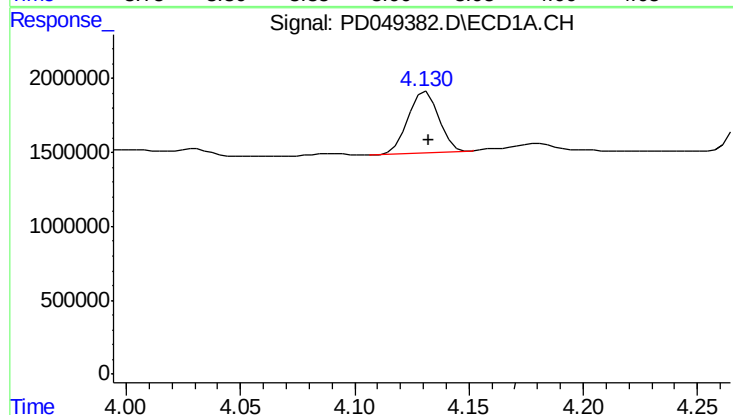


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: -0.001 min
Response: 3868315
Conc: 80.25 ng/ml

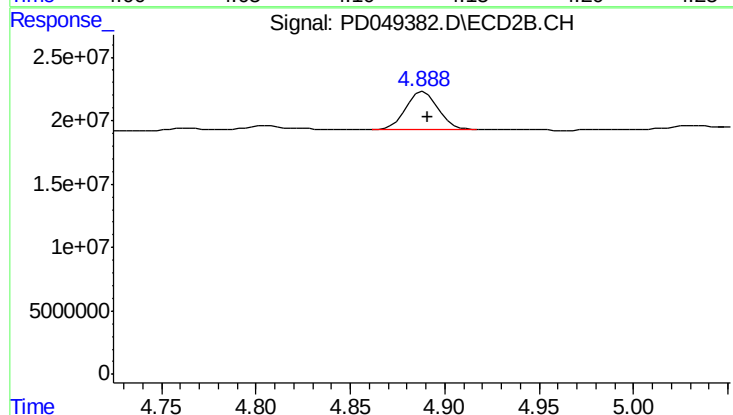

#23 Chlordane-1


R.T.: 4.888 min
Delta R.T.: -0.003 min
Response: 35213195
Conc: 83.11 ng/ml m

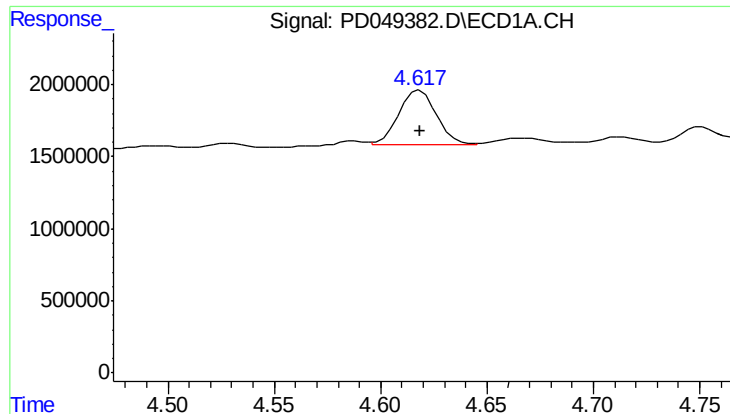

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: -0.002 min
Response: 4676508
Conc: 88.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB113034BS

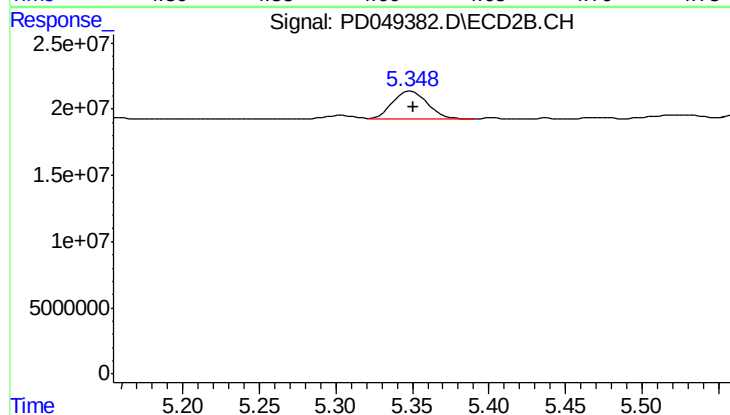


#24 Chlordane-2

R.T.: 5.349 min
Delta R.T.: -0.002 min
Response: 34984879
Conc: 84.54 ng/ml

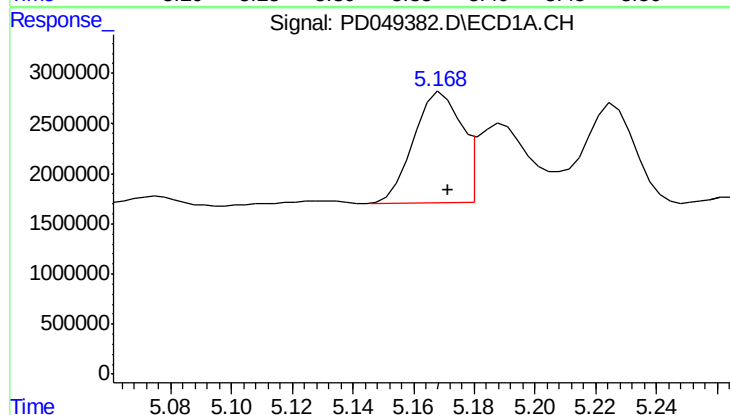


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: -0.003 min
Response: 11890097
Conc: 72.55 ng/ml m

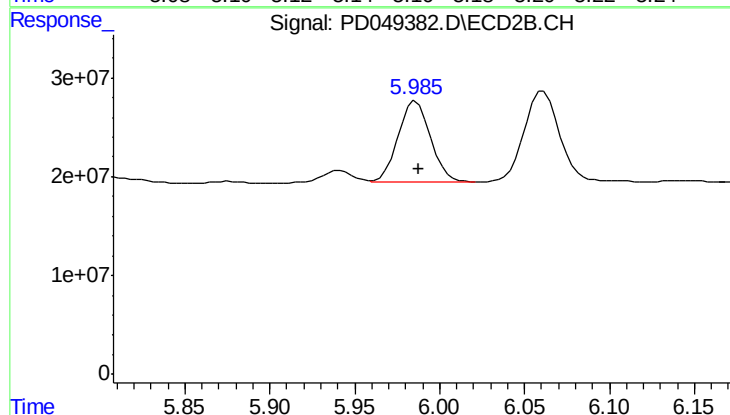

#25 Chlordane-3


R.T.: 5.985 min
Delta R.T.: -0.003 min
Response: 107826311
Conc: 80.23 ng/ml m

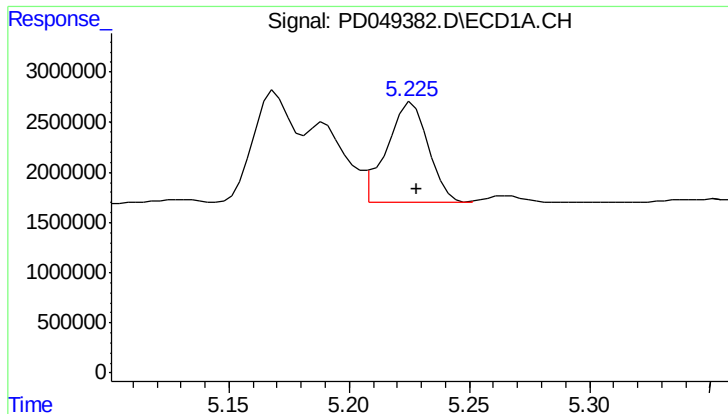

#26 Chlordane-4


R.T.: 5.226 min
Delta R.T.: -0.002 min
Response: 11955141
Conc: 78.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB113034BS

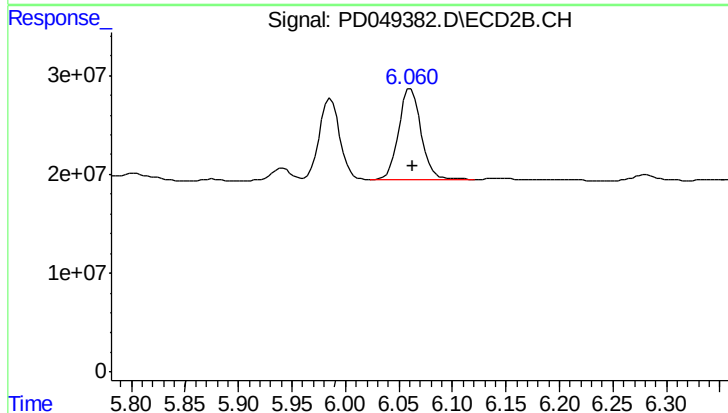


#26 Chlordane-4

R.T.: 6.061 min
Delta R.T.: -0.002 min
Response: 132016369
Conc: 83.98 ng/ml

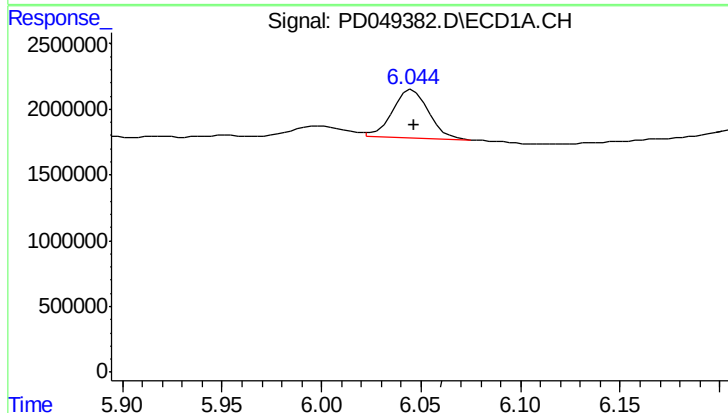


#27 Chlordane-5

R.T.: 6.044 min
Delta R.T.: -0.002 min
Response: 4643608
Conc: 87.19 ng/ml m

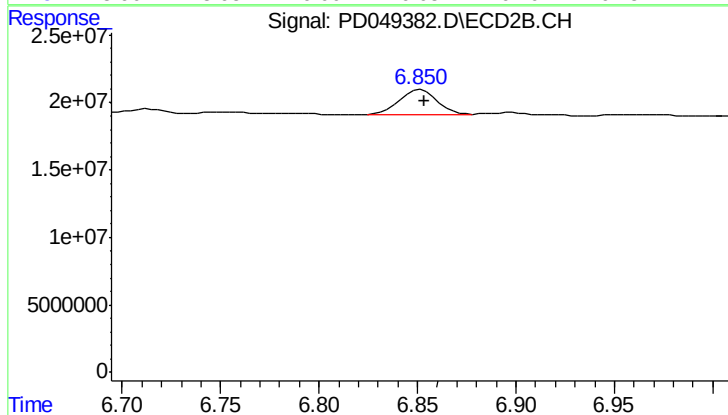

#27 Chlordane-5


R.T.: 6.850 min
Delta R.T.: -0.003 min
Response: 24815908
Conc: 80.23 ng/ml m

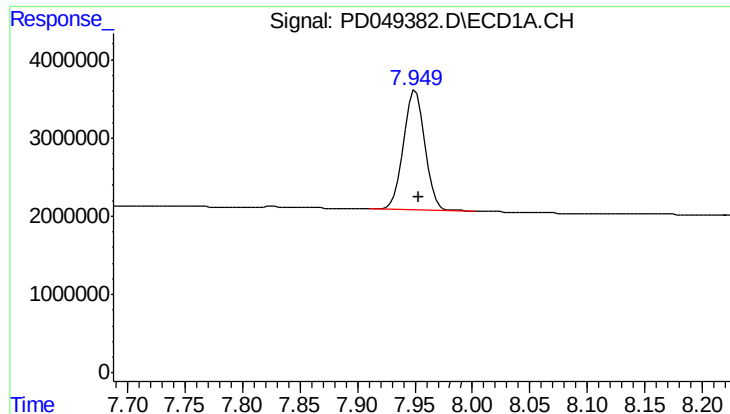

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: -0.003 min
Response: 19721295
Conc: 18.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB113034BS

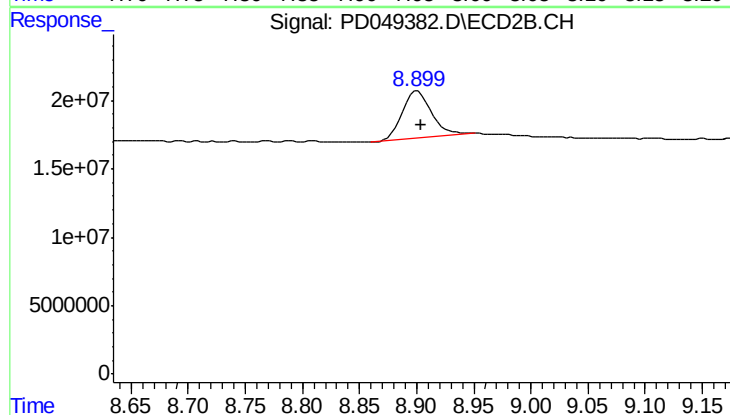

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: -0.004 min
Response: 63123958
Conc: 18.73 ng/ml