

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
 Data File : PD049404.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2018 13:11
 Operator : AJ\SJ
 Sample : J4777-20
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PL-03-092018-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 03:50:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 24 01:44:23 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.913	19519910	193.3E6	19.426	21.528
28)	SA Decachlor...	7.949	8.900	21475446	74354793	19.860	22.059

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092318\
Data File : PD049404.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2018 13:11
Operator : AJ\SJ
Sample : J4777-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PL-03-092018-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 03:50:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092318.M
Quant Title : GC Extractables
QLast Update : Mon Sep 24 01:44:23 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

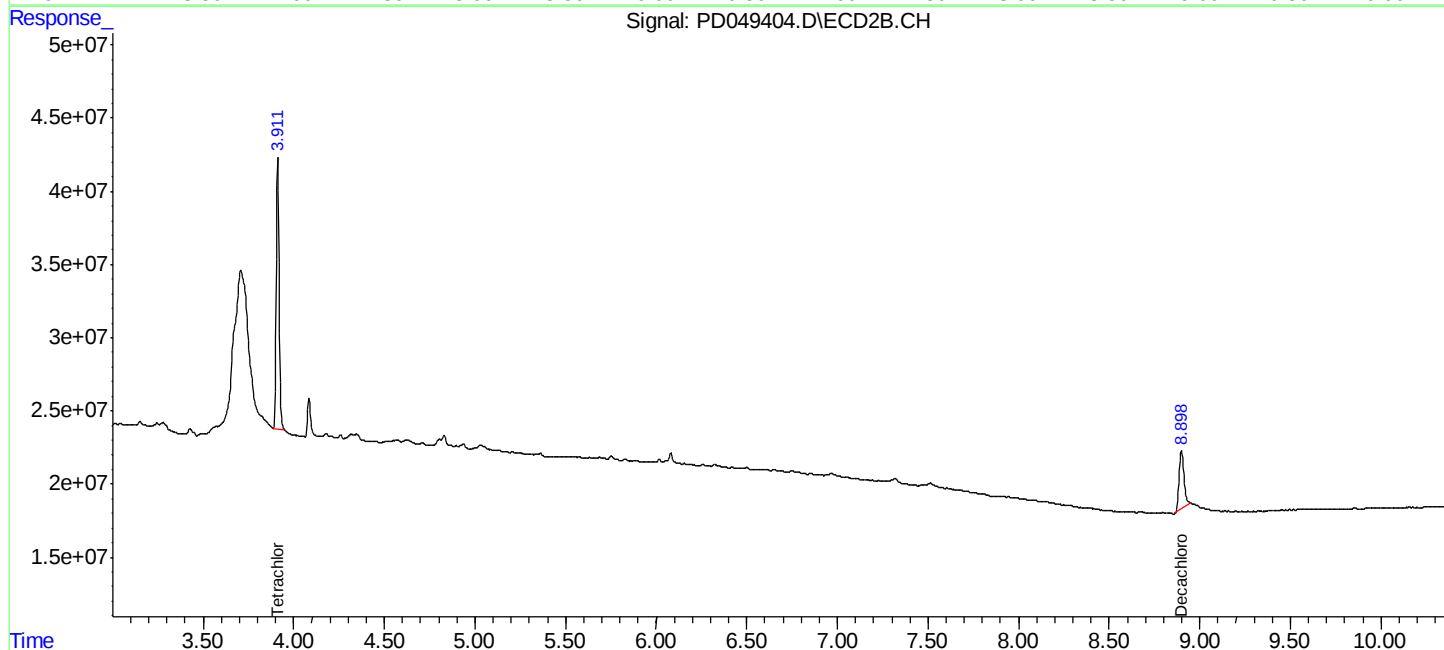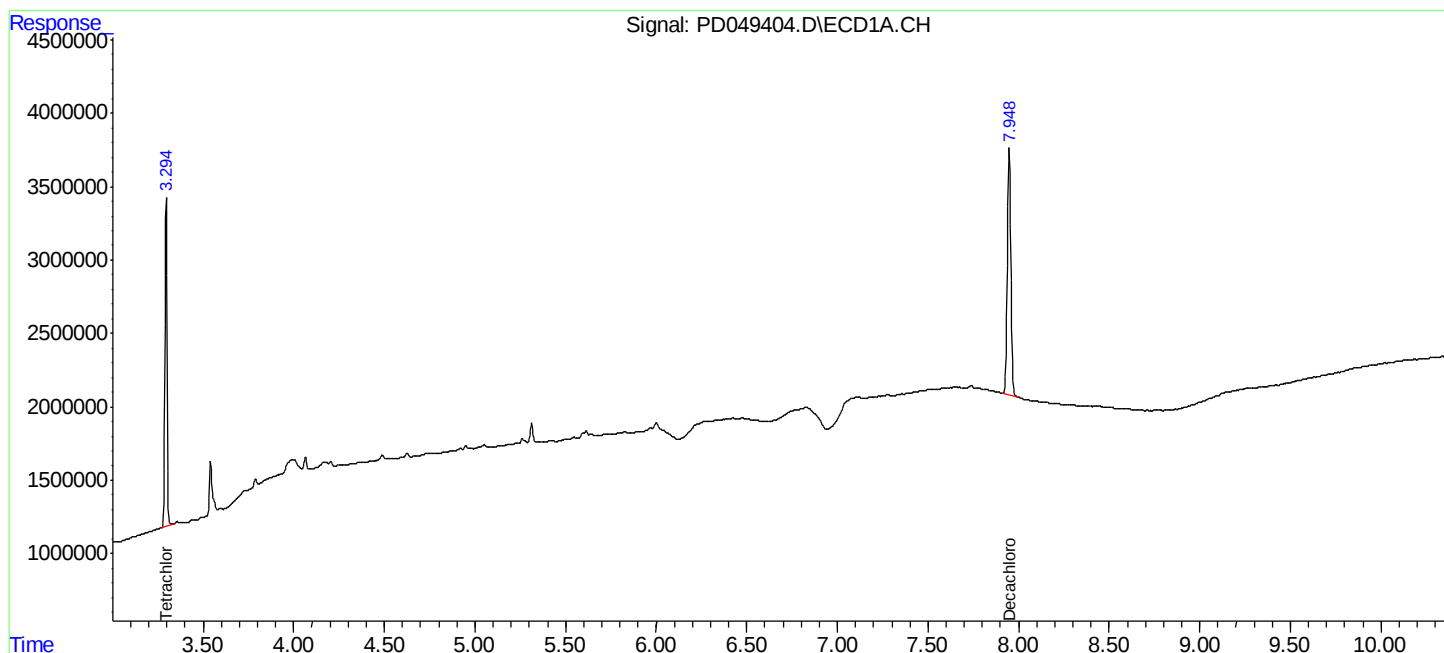


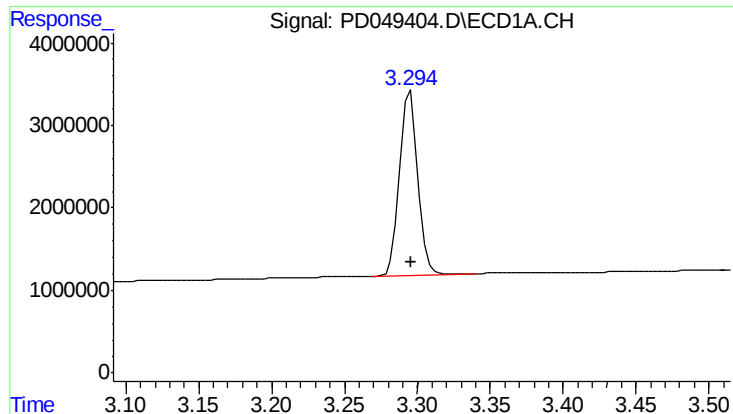

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 19519910
Conc: 19.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PL-03-092018-A

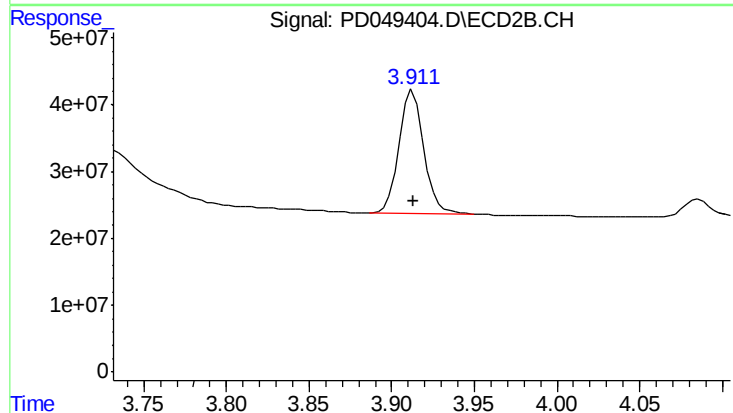


#1 Tetrachloro-m-xylene

R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 193283815
Conc: 21.53 ng/ml

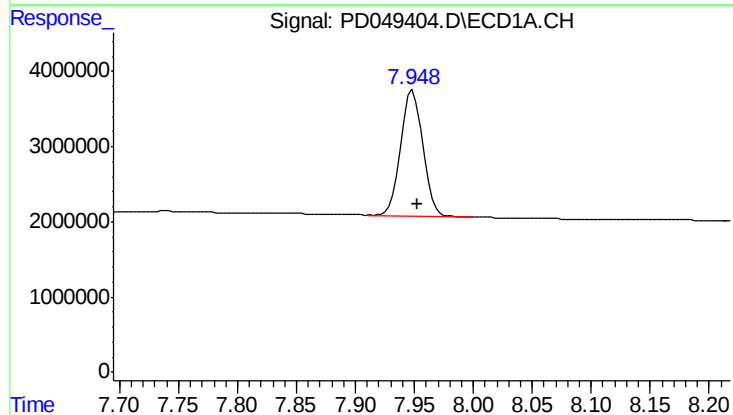

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.004 min
Response: 21475446
Conc: 19.86 ng/ml

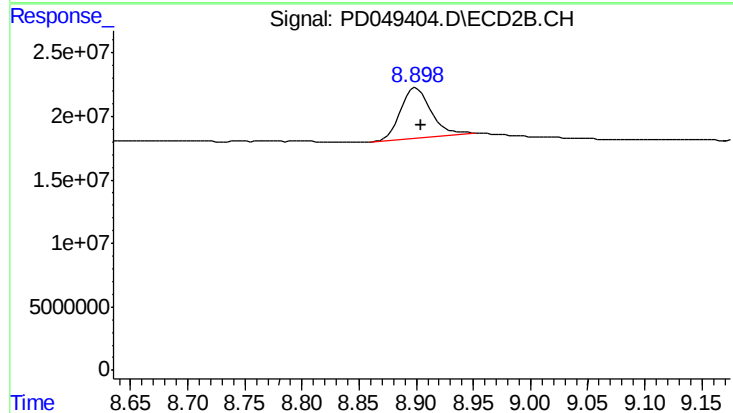

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.005 min
Response: 74354793
Conc: 22.06 ng/ml