

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
 Data File : PD059283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 10:33
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 11:57:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 11:55:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	4855563	8768806	5.082	4.921
27)	SA Decachlor...	7.838	8.861	10927504	16077345	10.545	10.448
Target Compounds							
2)	A alpha-BHC	3.627	4.247	6655897	11905266	4.699	4.696
3)	MA gamma-BHC...	3.898	4.528	7234398	11029456	5.322	4.744
4)	MA Heptachlor	4.177	5.028	6086270	10902425	4.962	4.823
9)	A Endosulfan I	5.171	6.065	5483218	9095692	5.057	5.009
13)	MA Dieldrin	5.408	6.320	11356684	19118933	9.451	9.572
14)	MA Endrin	5.659	6.535	8868402	14292590	9.607	9.229
16)	A 4,4'-DDD	5.797	6.665	8736814	14891990	9.664	9.537
17)	MA 4,4'-DDT	6.030	6.961	8187339	14088110	8.867	8.925
20)	A Methoxychlor	6.579	7.421	21667271	39267762	48.252	45.130
21)	B Endrin ke...	6.790	7.558	956458	1266173	13.535	16.823

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
Data File : PD059283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 10:33
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 11:57:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 11:55:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

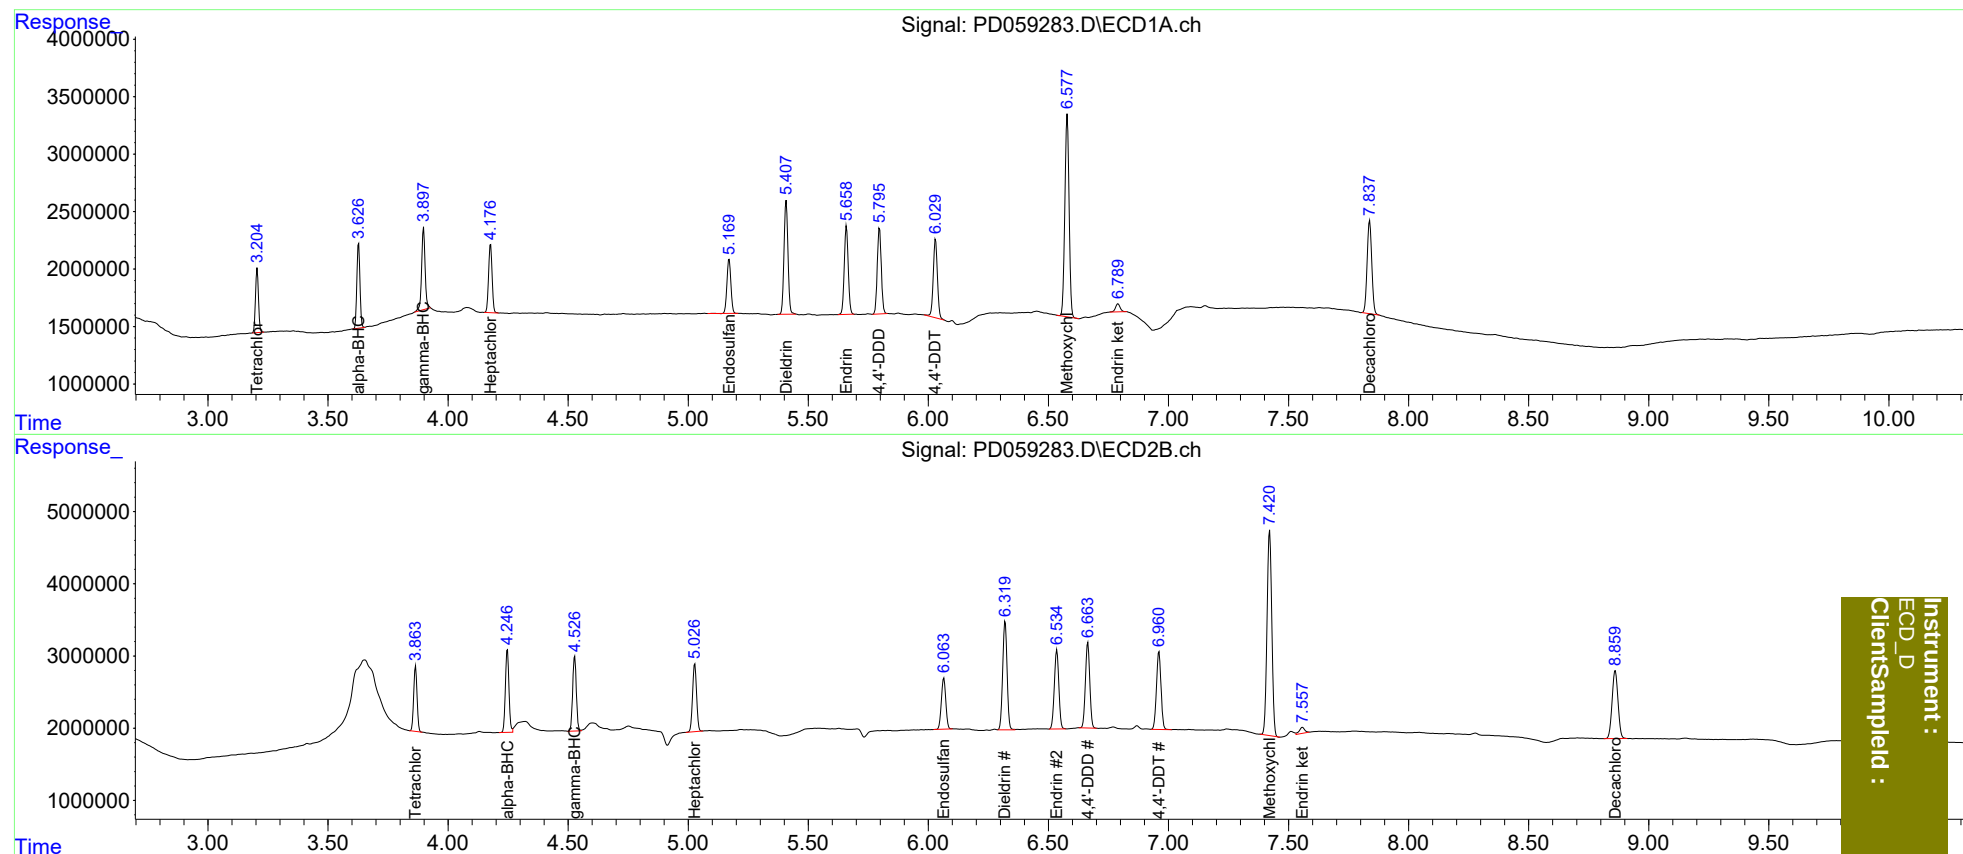


Instrument :
ECD_D
ClientSampled :

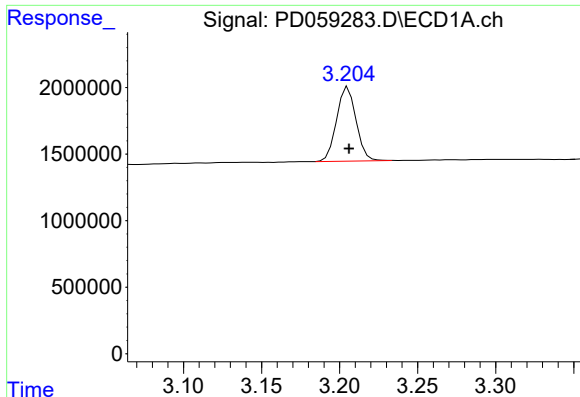

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 4855563
Conc: 5.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

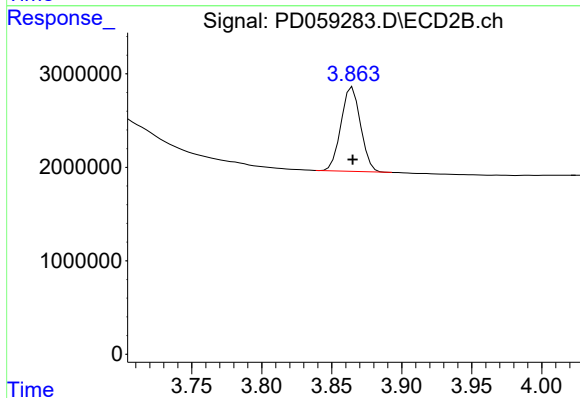


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 8768806
Conc: 4.92 ng/ml

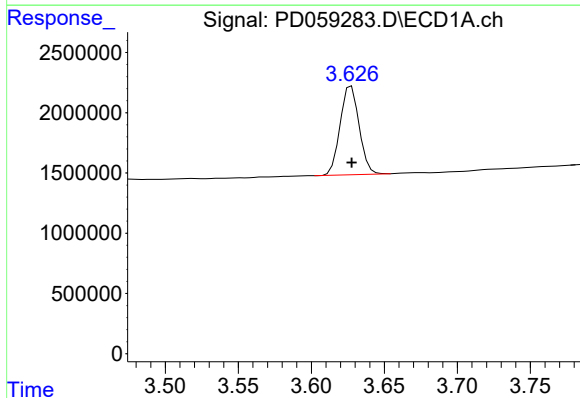


#2 alpha-BHC

R.T.: 3.627 min
Delta R.T.: 0.000 min
Response: 6655897
Conc: 4.70 ng/ml

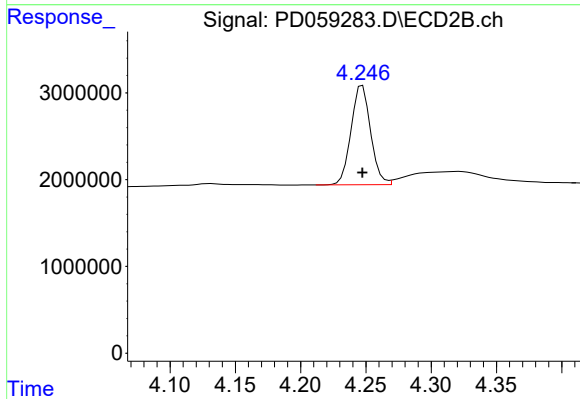

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 11905266
Conc: 4.70 ng/ml

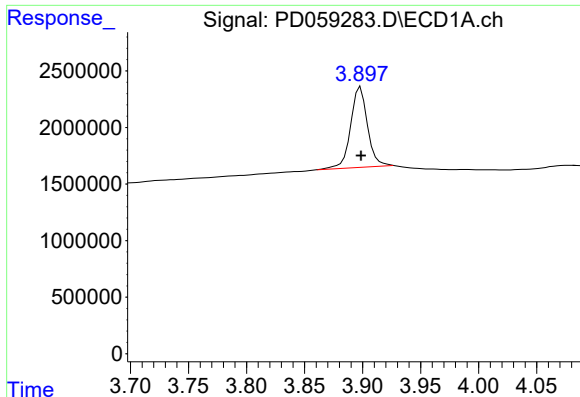

#3 gamma-BHC (Lindane)


R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 7234398
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

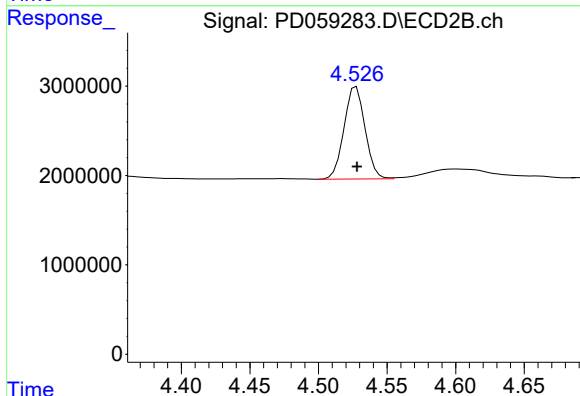


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 11029456
Conc: 4.74 ng/ml

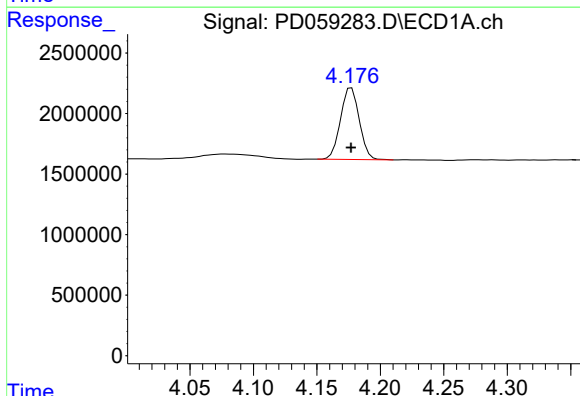


#4 Heptachlor

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 6086270
Conc: 4.96 ng/ml

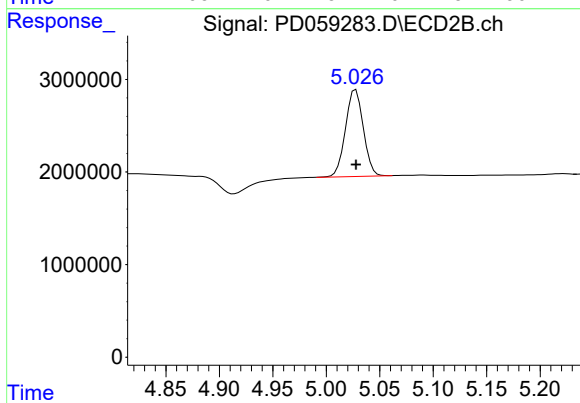

#4 Heptachlor


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 10902425
Conc: 4.82 ng/ml

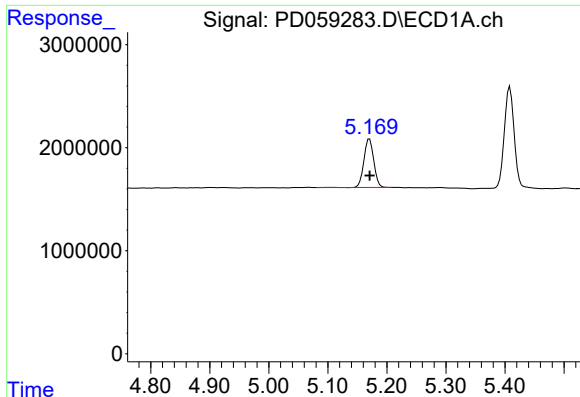

#9 Endosulfan I


R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 5483218
Conc: 5.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

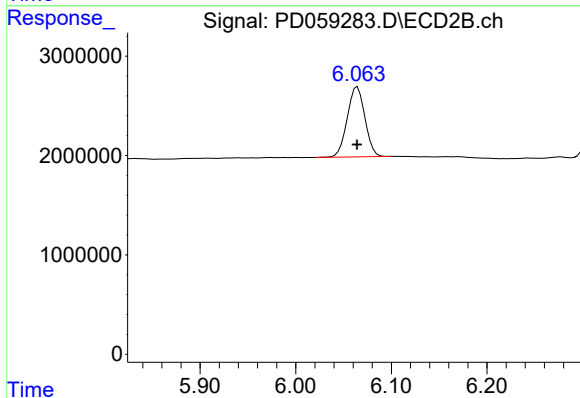


#9 Endosulfan I

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 9095692
Conc: 5.01 ng/ml

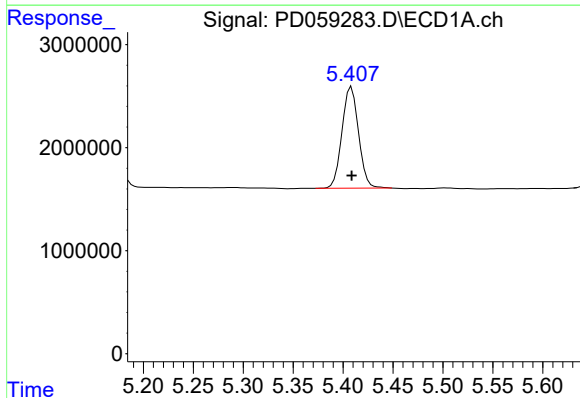


#13 Dieldrin

R.T.: 5.408 min
Delta R.T.: 0.000 min
Response: 11356684
Conc: 9.45 ng/ml

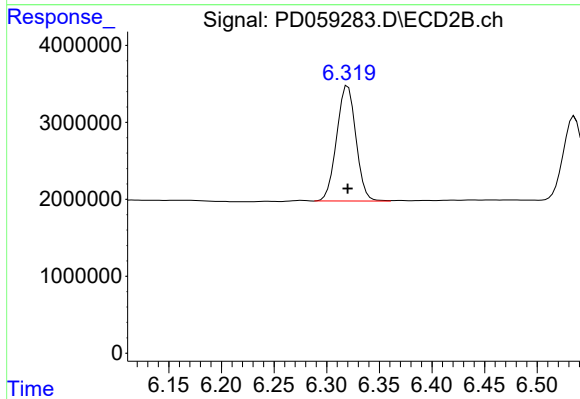

#13 Dieldrin


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 19118933
Conc: 9.57 ng/ml

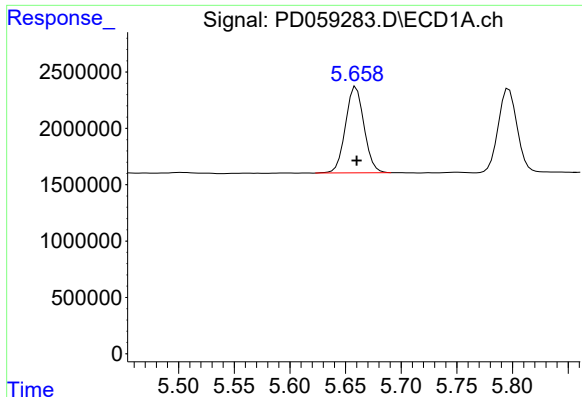

#14 Endrin


R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 8868402
Conc: 9.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

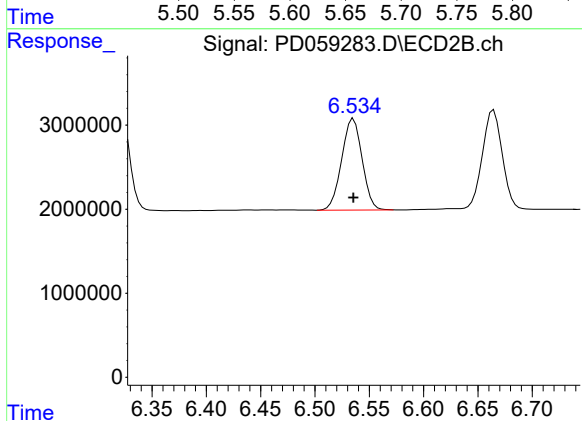


#14 Endrin

R.T.: 6.535 min
Delta R.T.: 0.000 min
Response: 14292590
Conc: 9.23 ng/ml

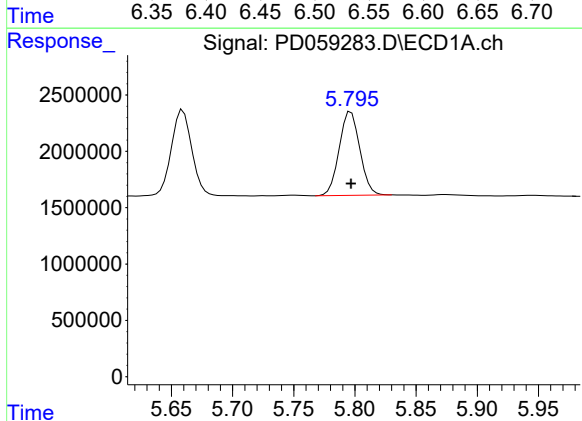


#16 4,4'-DDD

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 8736814
Conc: 9.66 ng/ml

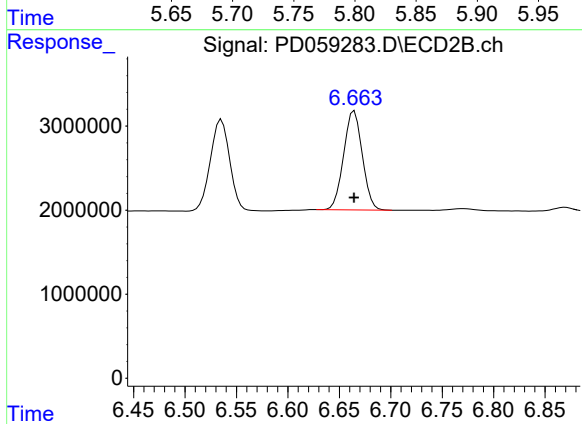

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 14891990
Conc: 9.54 ng/ml

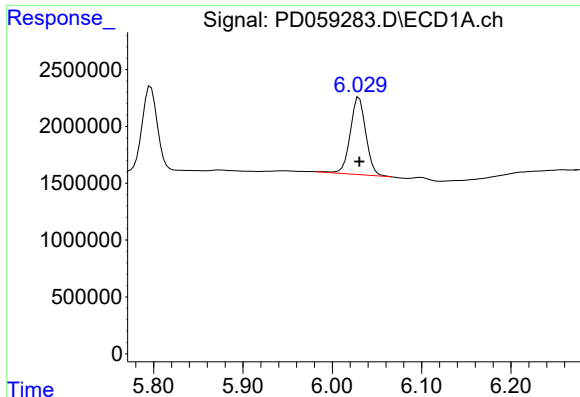

#17 4,4'-DDT


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 8187339
Conc: 8.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

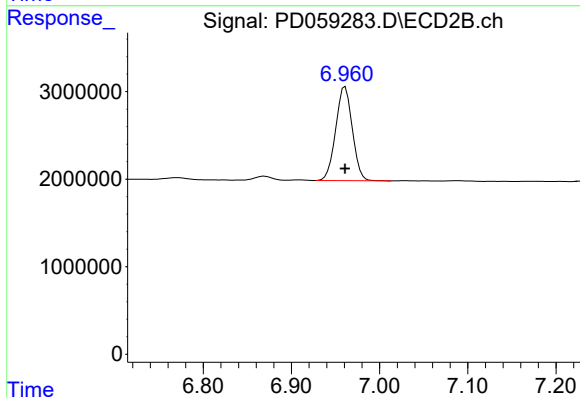


#17 4,4'-DDT

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 14088110
Conc: 8.93 ng/ml

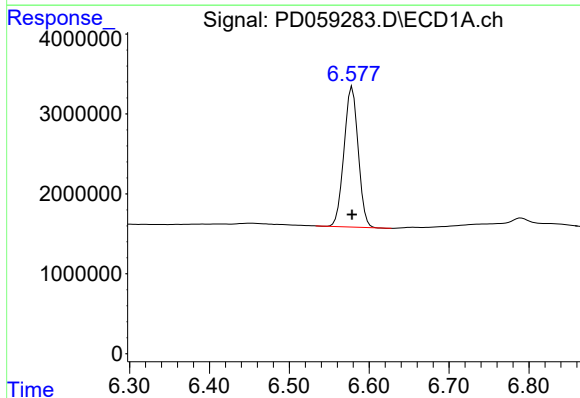


#20 Methoxychlor

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 21667271
Conc: 48.25 ng/ml

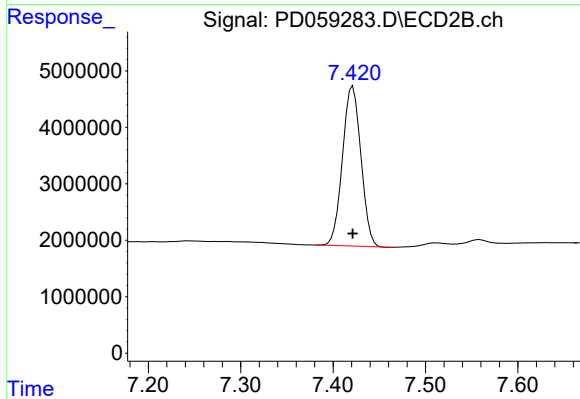

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 39267762
Conc: 45.13 ng/ml

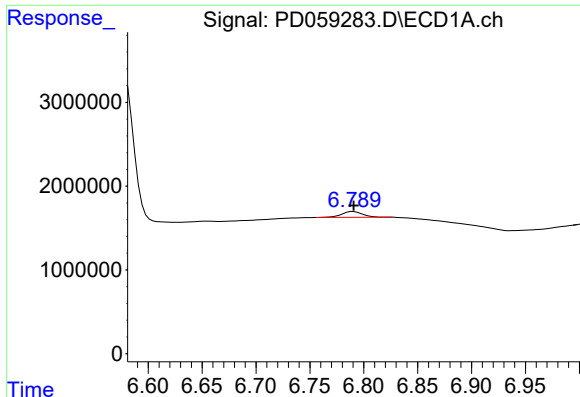

#21 Endrin ketone


R.T.: 6.790 min
Delta R.T.: 0.000 min
Response: 956458
Conc: 13.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

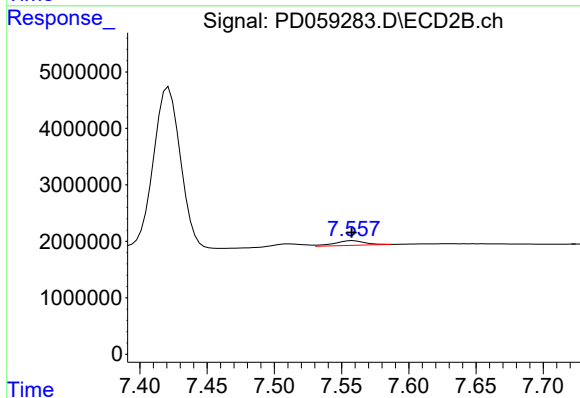


#21 Endrin ketone

R.T.: 7.558 min
Delta R.T.: 0.000 min
Response: 1266173
Conc: 16.82 ng/ml

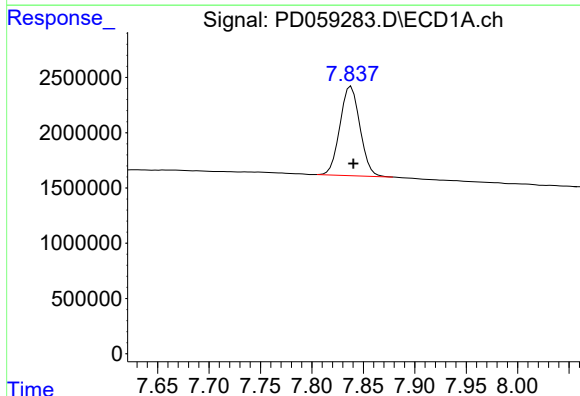

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.002 min
Response: 10927504
Conc: 10.55 ng/ml

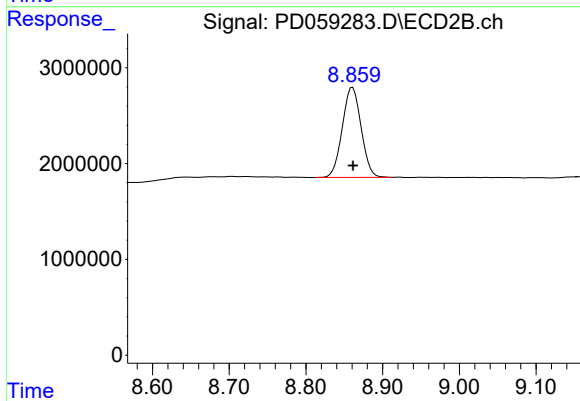

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 16077345
Conc: 10.45 ng/ml