

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
 Data File : PD059287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 11:29
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 11:55:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 11:55:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	19108615	35637294	20.000	20.000
27)	SA Decachlor...	7.840	8.861	41449051	61549256	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.628	4.247	28327579	50701928	20.000	20.000
3)	MA gamma-BHC...	3.899	4.528	27186944	46497598	20.000	20.000
4)	MA Heptachlor	4.177	5.028	24533214	45213592	20.000	20.000
9)	A Endosulfan I	5.171	6.064	21687214	36314782	20.000	20.000
13)	MA Dieldrin	5.409	6.320	48064581	79898212	40.000	40.000
14)	MA Endrin	5.660	6.535	36924480	61948649	40.000	40.000
16)	A 4,4'-DDD	5.797	6.664	36163645	62461680	40.000	40.000
17)	MA 4,4'-DDT	6.030	6.961	36935014	63137097	40.000	40.000
20)	A Methoxychlor	6.578	7.421	89809527	174.0E6	200.000	200.000
21)	B Endrin ke...	6.791	7.558	2826700	3010492	40.000	40.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
Data File : PD059287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 11:29
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 11:55:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 11:55:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

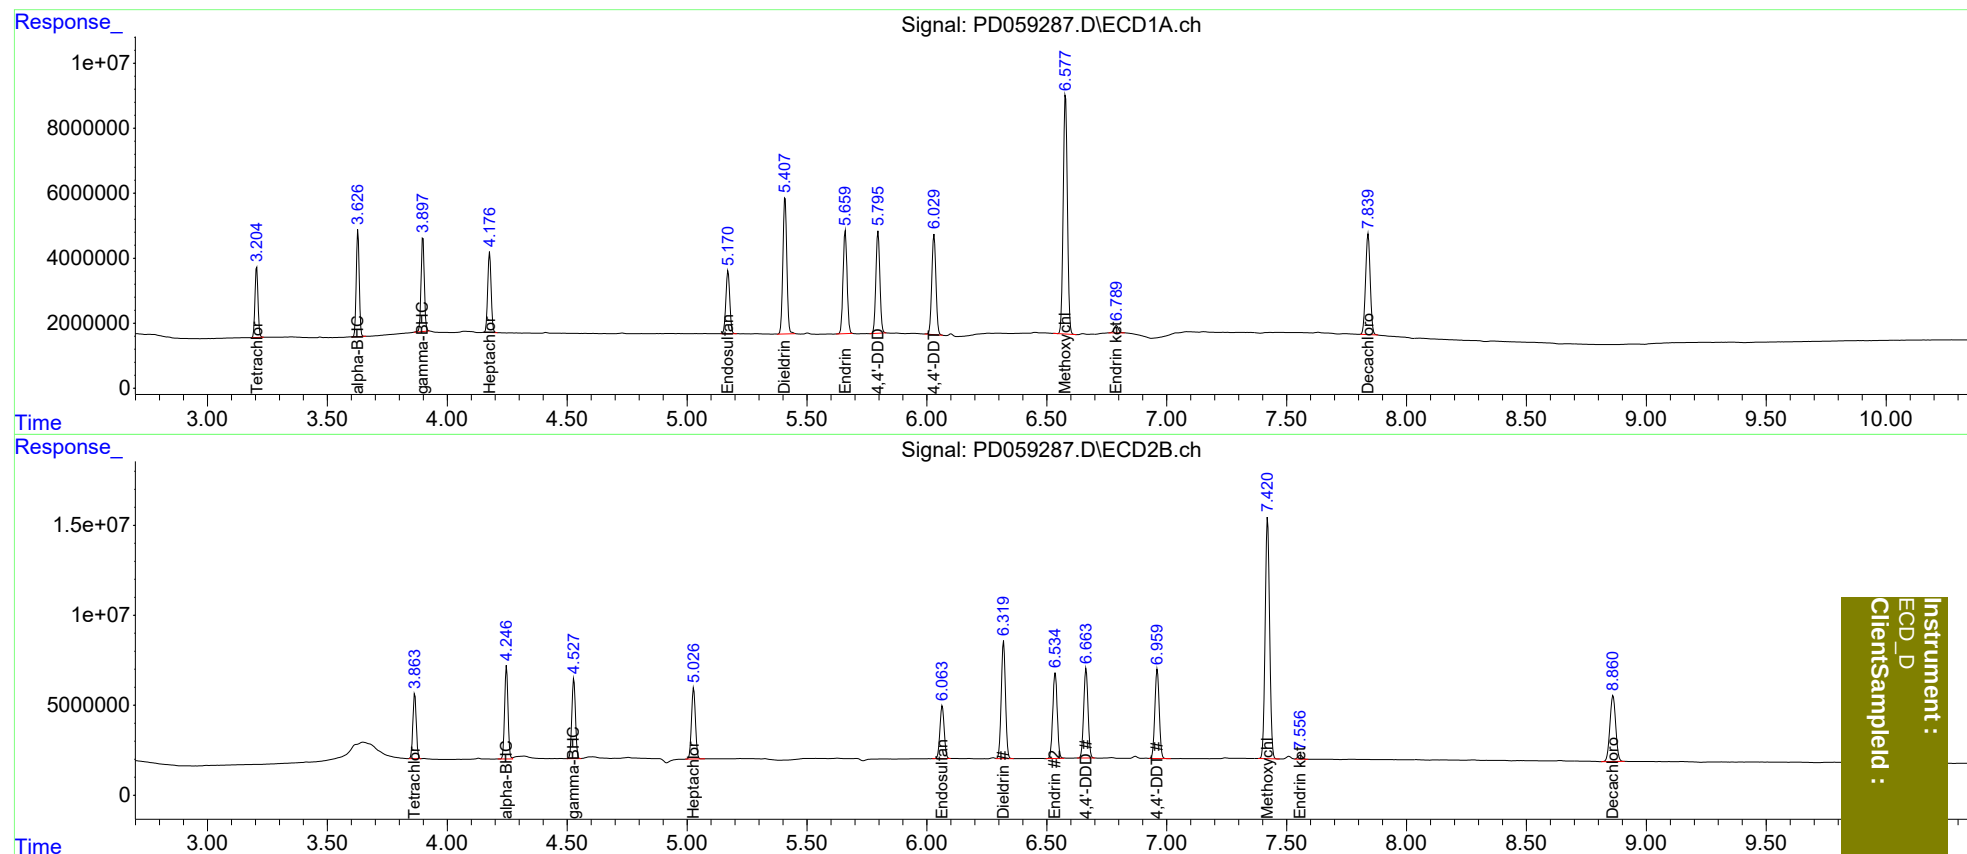


Instrument :
ECD_D
ClientSampled :

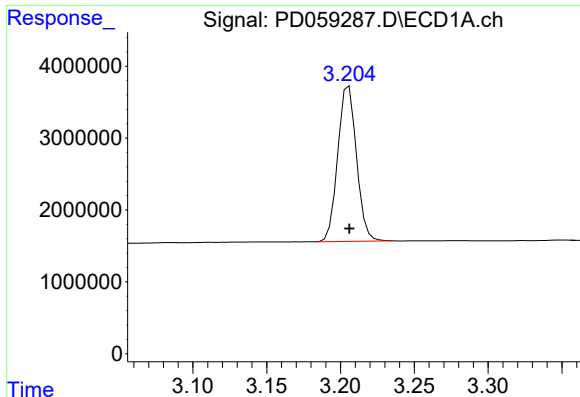

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 19108615
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

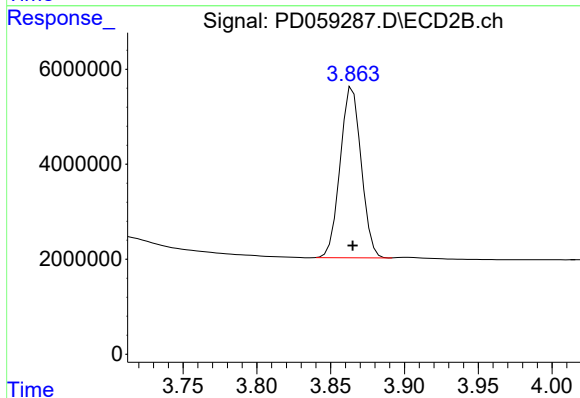


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 35637294
Conc: 20.00 ng/ml

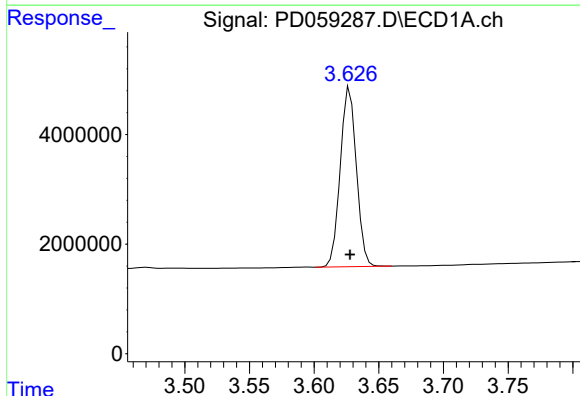


#2 alpha-BHC

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 28327579
Conc: 20.00 ng/ml

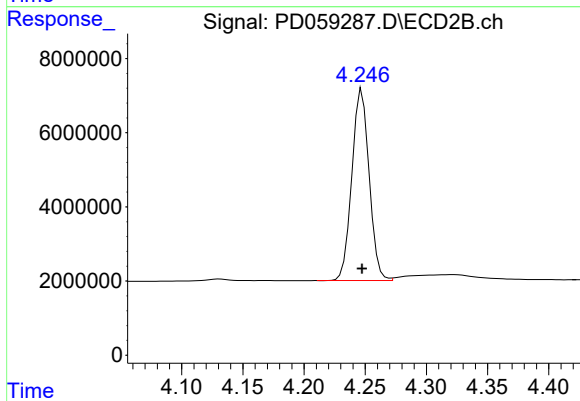

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 50701928
Conc: 20.00 ng/ml

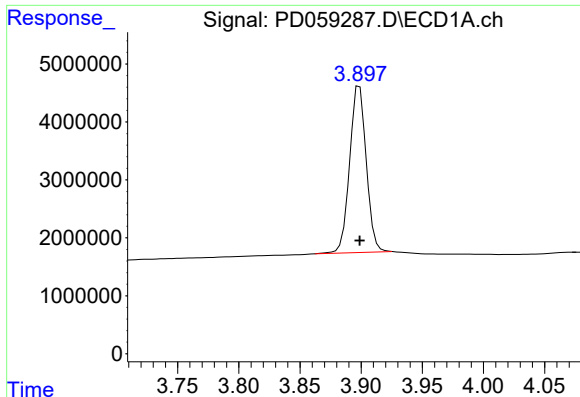

#3 gamma-BHC (Lindane)


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 27186944
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

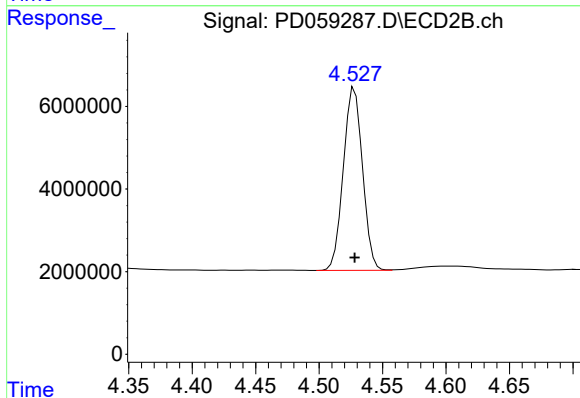


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 46497598
Conc: 20.00 ng/ml

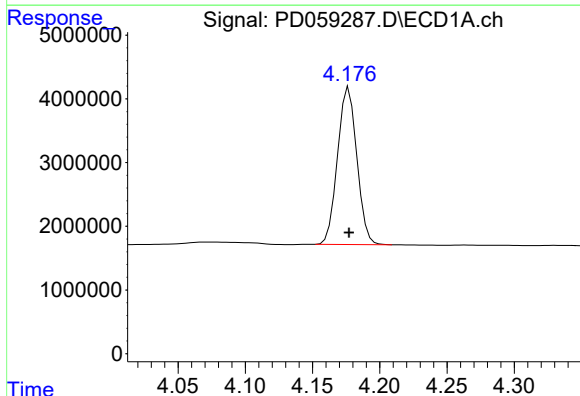


#4 Heptachlor

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 24533214
Conc: 20.00 ng/ml

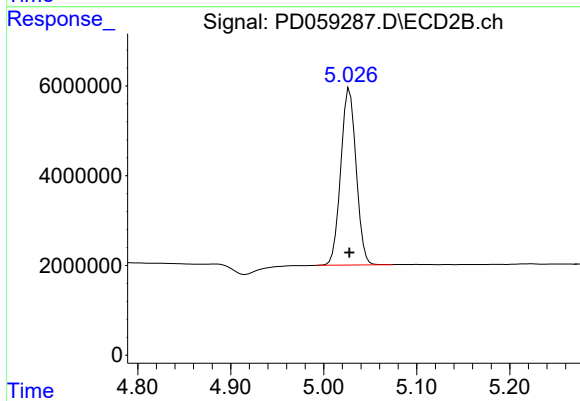

#4 Heptachlor


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 45213592
Conc: 20.00 ng/ml

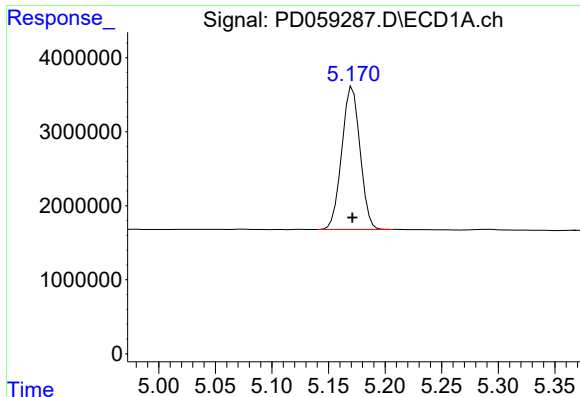

#9 Endosulfan I


R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 21687214
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

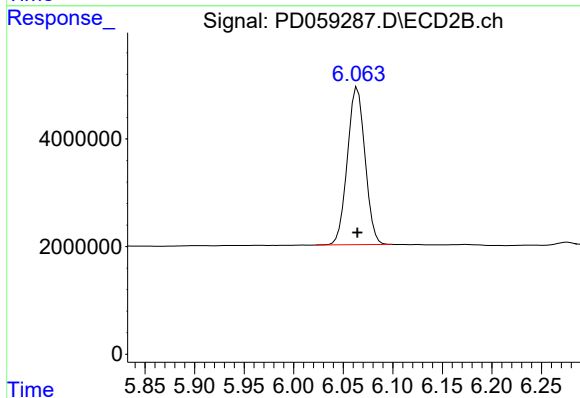


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 36314782
Conc: 20.00 ng/ml

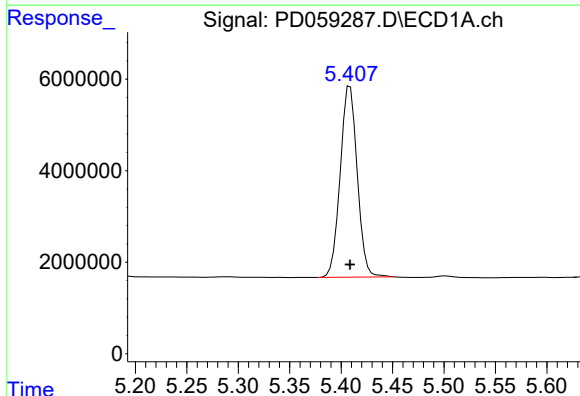


#13 Dieldrin

R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 48064581
Conc: 40.00 ng/ml

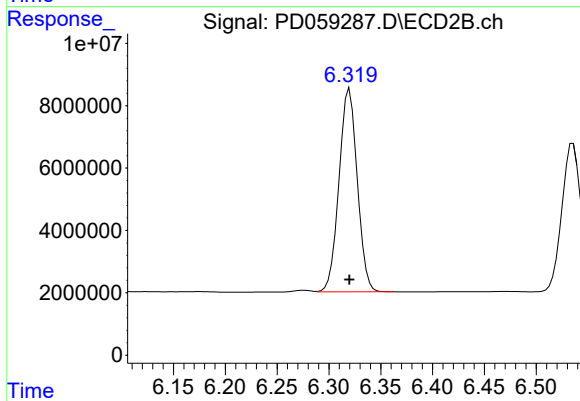

#13 Dieldrin


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 79898212
Conc: 40.00 ng/ml

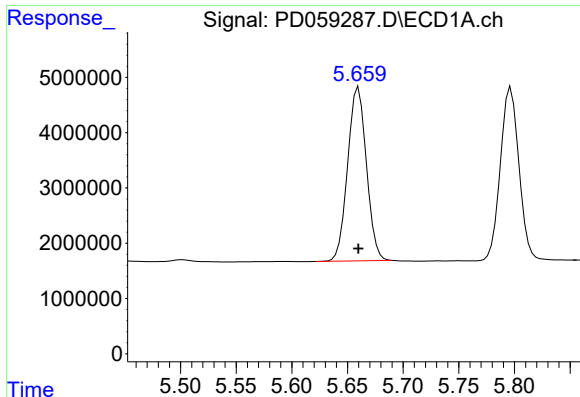

#14 Endrin


R.T.: 5.660 min
Delta R.T.: 0.000 min
Response: 36924480
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

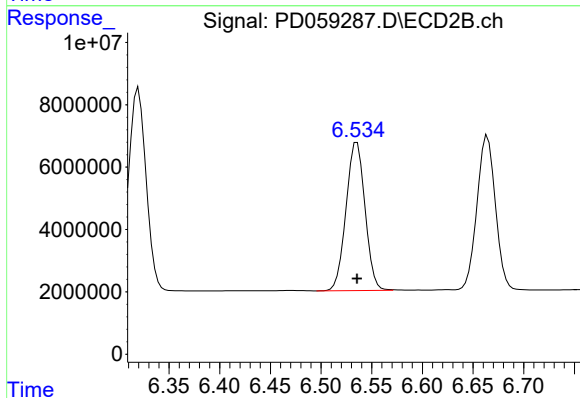


#14 Endrin

R.T.: 6.535 min
Delta R.T.: 0.000 min
Response: 61948649
Conc: 40.00 ng/ml

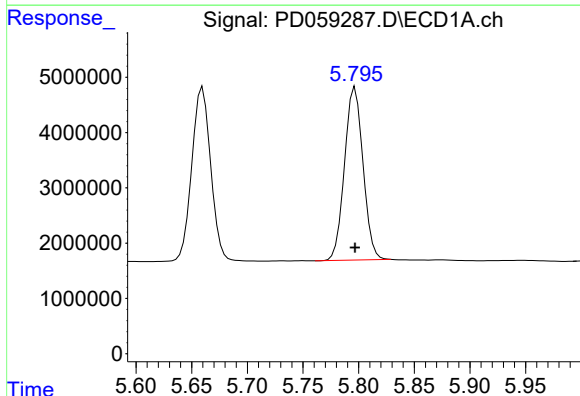


#16 4,4'-DDD

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 36163645
Conc: 40.00 ng/ml

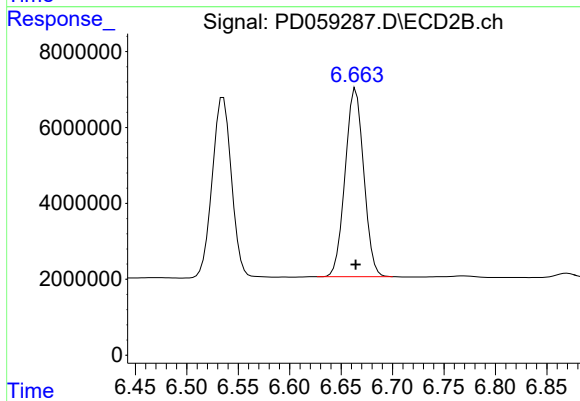

#16 4,4'-DDD


R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 62461680
Conc: 40.00 ng/ml

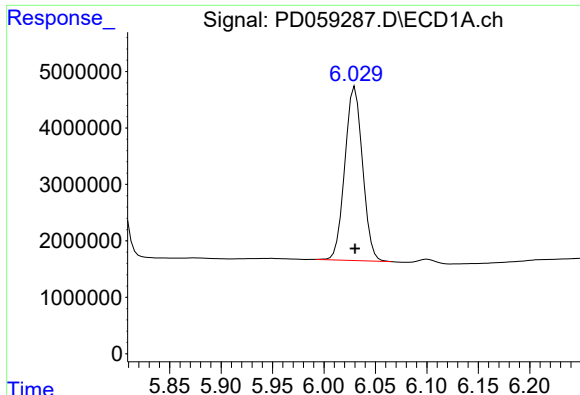

#17 4,4'-DDT


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 36935014
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

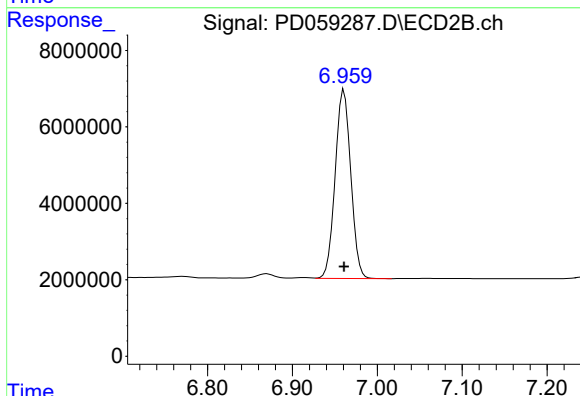


#17 4,4'-DDT

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 63137097
Conc: 40.00 ng/ml

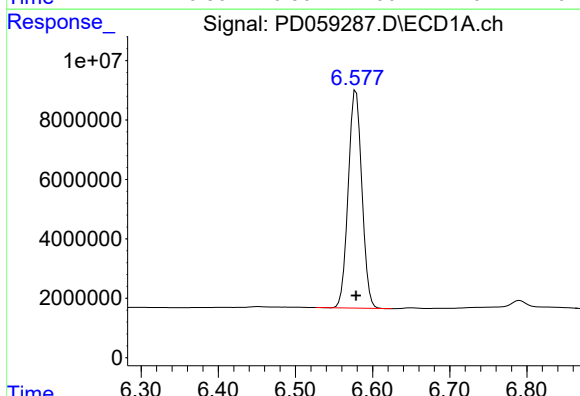


#20 Methoxychlor

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 89809527
Conc: 200.00 ng/ml

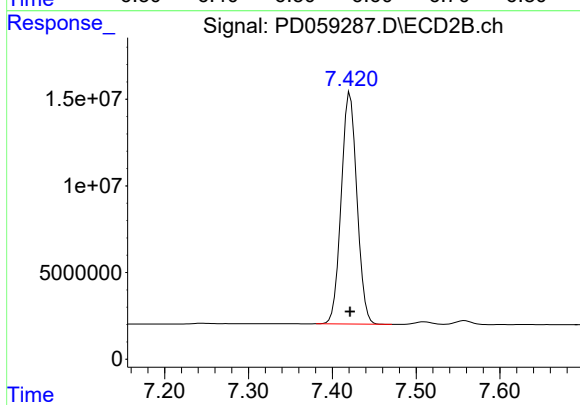

#20 Methoxychlor


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 174021713
Conc: 200.00 ng/ml

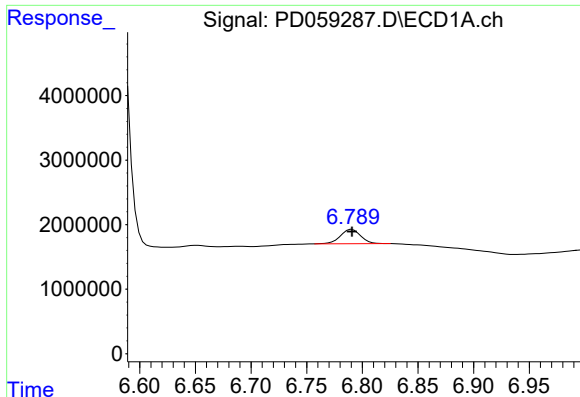

#21 Endrin ketone


R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 2826700
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

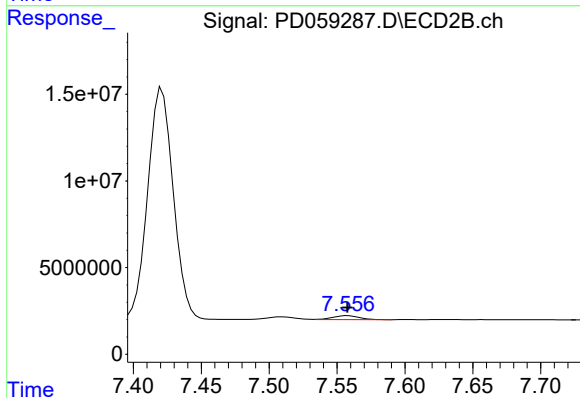


#21 Endrin ketone

R.T.: 7.558 min
Delta R.T.: 0.000 min
Response: 3010492
Conc: 40.00 ng/ml

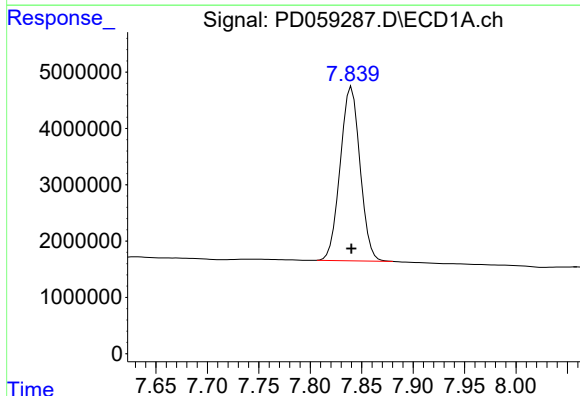

#27 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 41449051
Conc: 40.00 ng/ml

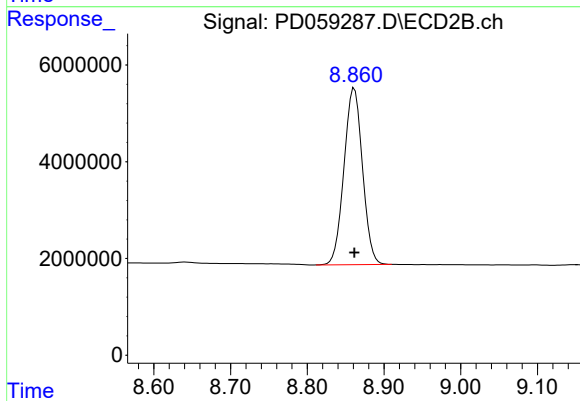

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 61549256
Conc: 40.00 ng/ml