

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
 Data File : PD059295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 13:22
 Operator : DD\AJ
 Sample : L4087-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:17:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:19:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


3) MA	gamma-BHC...	3.907	0.000	880530	0	0.629	N.D.	#
6) B	beta-BHC	0.000	4.665f	0	338679	N.D.	0.324	
8) B	Heptachlo...	0.000	5.710	0	1860659	N.D.	0.936	
9) A	Endosulfan I	0.000	6.086	0	290866	N.D.	0.159	
10) B	trans-Chl...	0.000	5.889f	0	376601	N.D.	0.190	
11) B	cis-Chlor...	0.000	6.086f	0	290866	N.D.	0.146	
19) B	Endosulfa...	0.000	7.122	0	658813	N.D.	0.383	
23)	Toxaphene-2	5.501	0.000	8959191	0	1268.549	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
Data File : PD059295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 13:22
Operator : DD\AJ
Sample : L4087-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:17:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:19:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

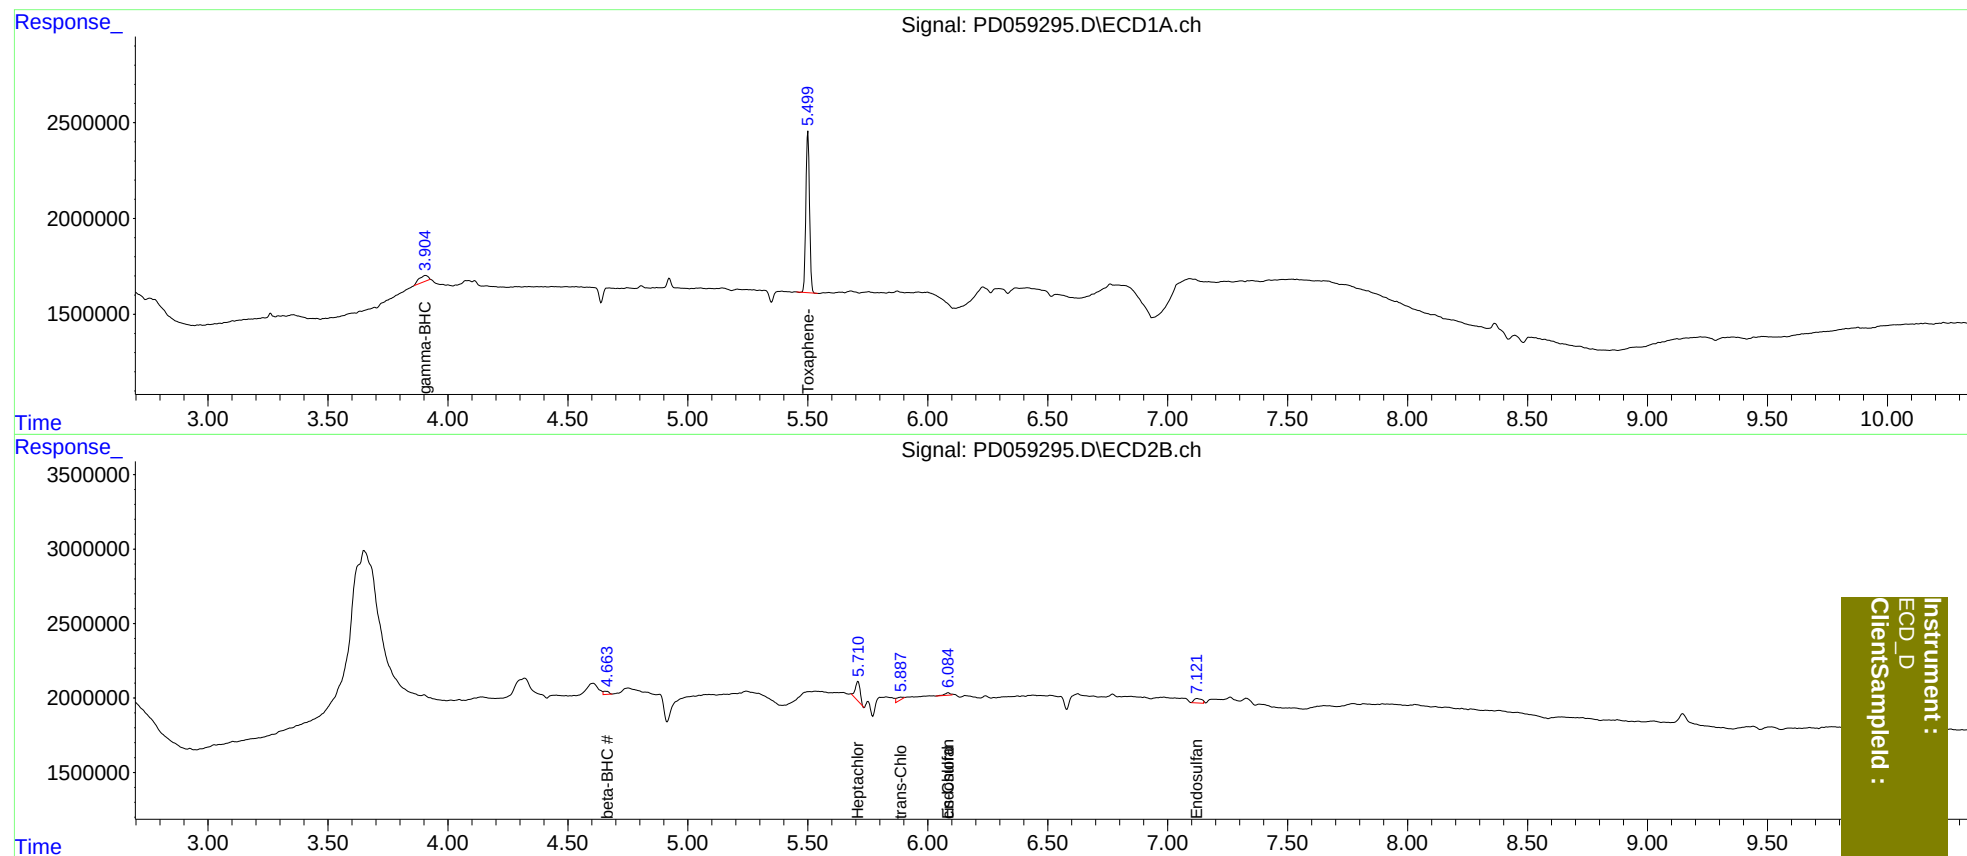


Instrument :
ECD_D
ClientSampled :

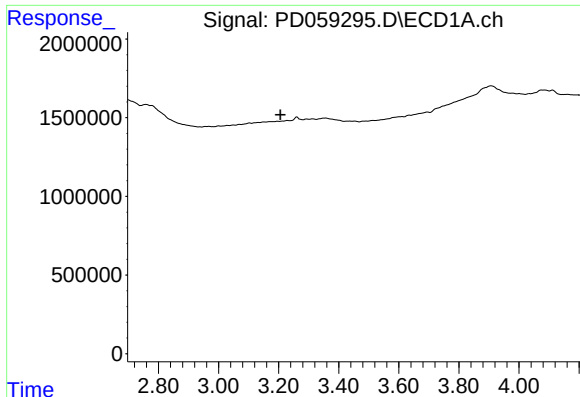

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

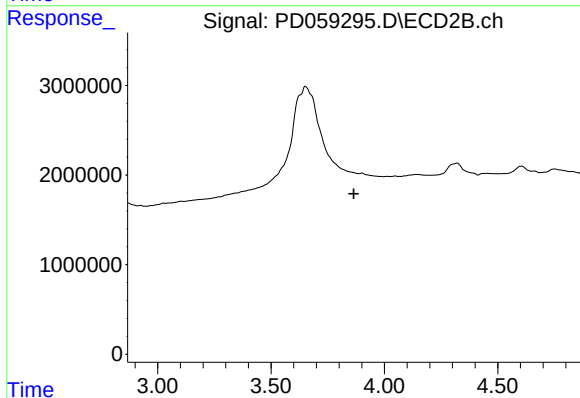


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.865 min
Response: 0
Conc: N.D.

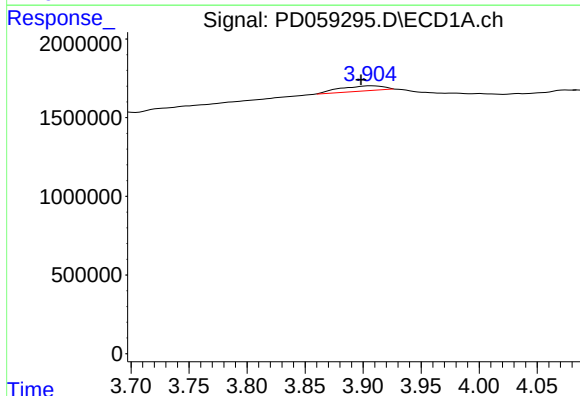


#3 gamma-BHC (Lindane)

R.T.: 3.907 min
Delta R.T.: 0.008 min
Response: 880530
Conc: 0.63 ng/ml

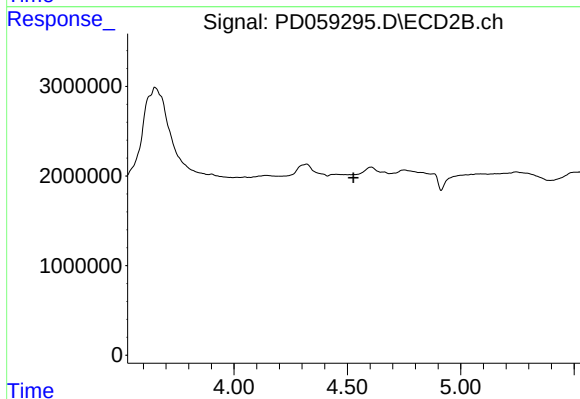

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

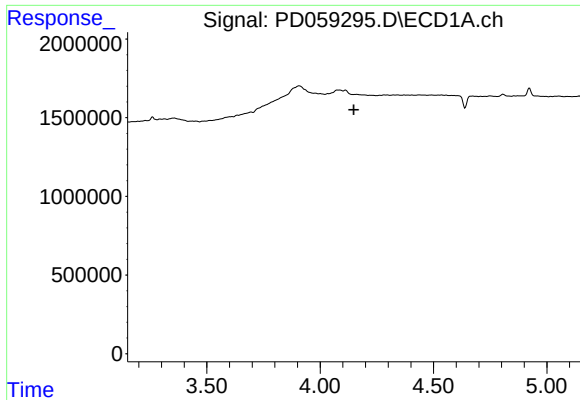

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

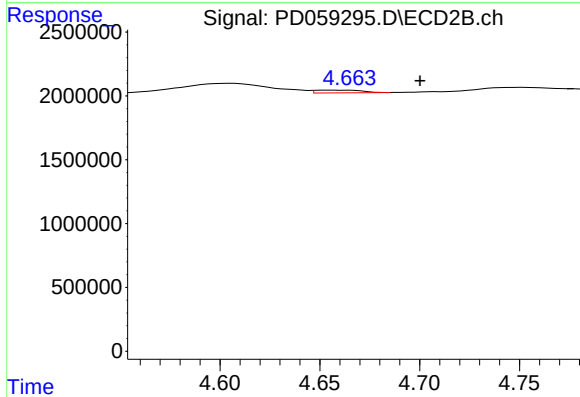


#6 beta-BHC

R.T.: 4.665 min
Delta R.T.: -0.036 min
Response: 338679
Conc: 0.32 ng/ml

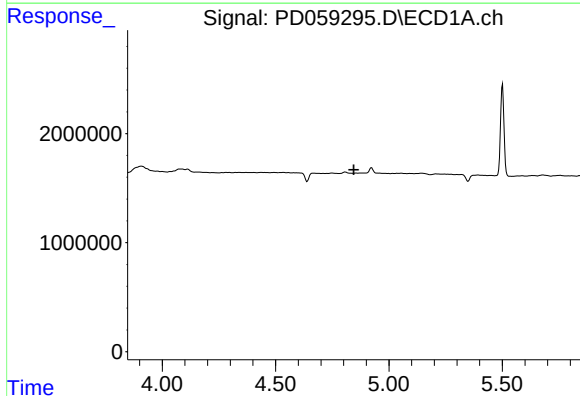


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

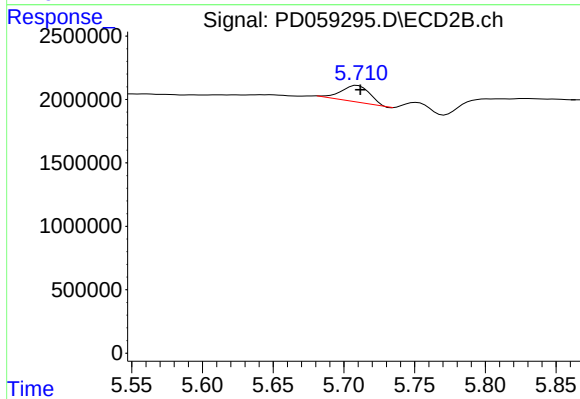

#8 Heptachlor epoxide


R.T.: 5.710 min
Delta R.T.: -0.002 min
Response: 1860659
Conc: 0.94 ng/ml

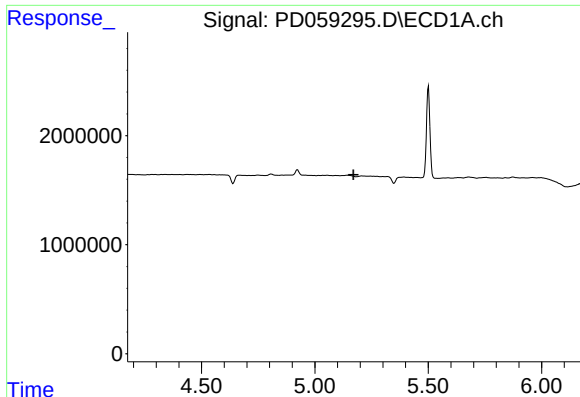

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

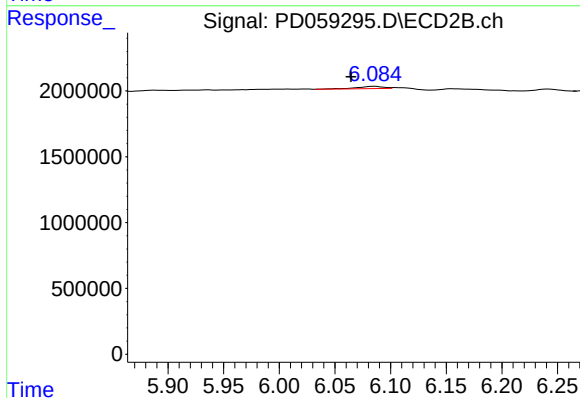


#9 Endosulfan I

R.T.: 6.086 min
Delta R.T.: 0.021 min
Response: 290866
Conc: 0.16 ng/ml

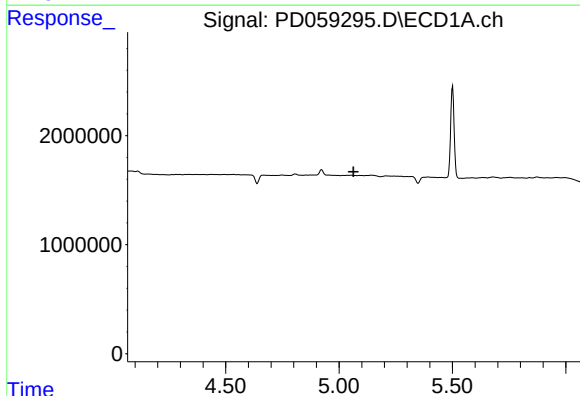


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

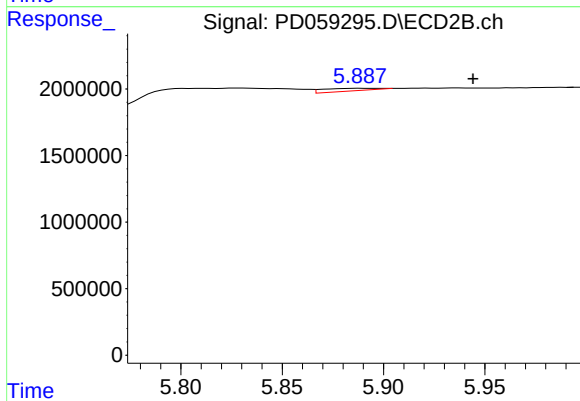

#10 trans-Chlordane


R.T.: 5.889 min
Delta R.T.: -0.055 min
Response: 376601
Conc: 0.19 ng/ml

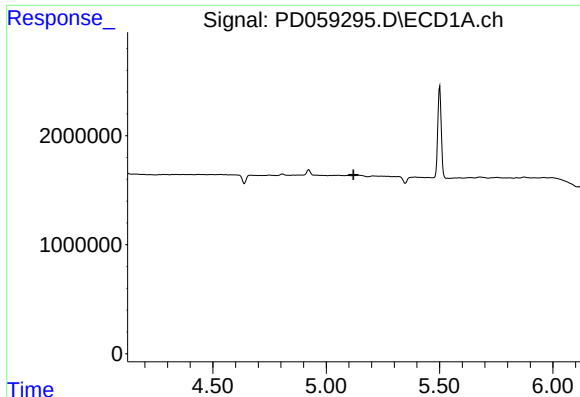

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

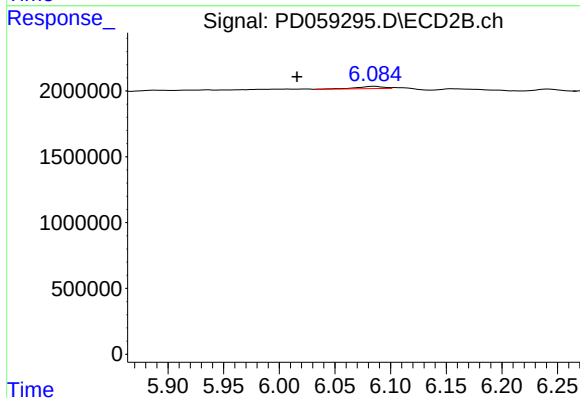


#11 cis-Chlordane

R.T.: 6.086 min
Delta R.T.: 0.070 min
Response: 290866
Conc: 0.15 ng/ml

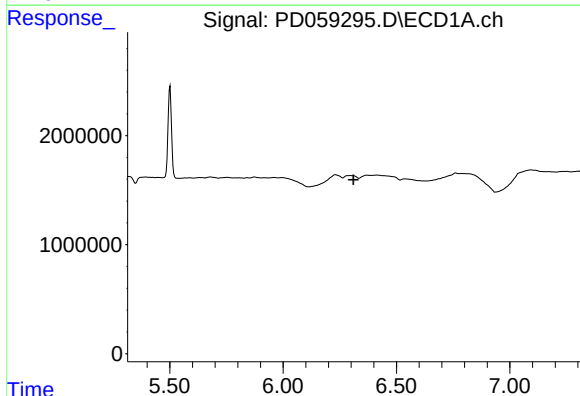


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

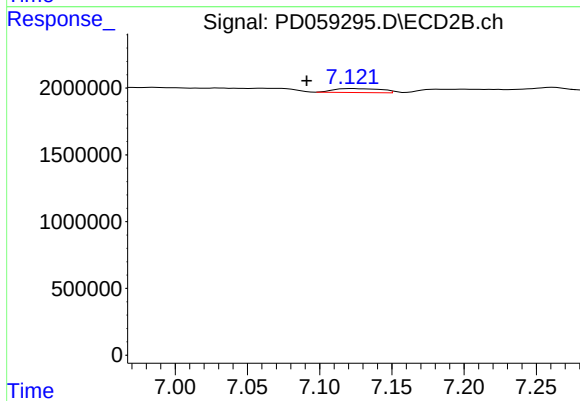

#19 Endosulfan Sulfate


R.T.: 7.122 min
Delta R.T.: 0.031 min
Response: 658813
Conc: 0.38 ng/ml

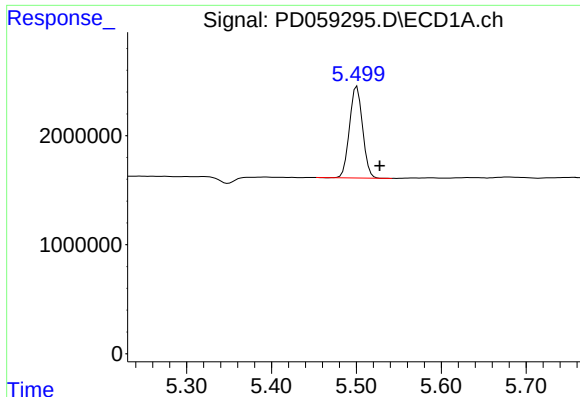

#23 Toxaphene-2


R.T.: 5.501 min
Delta R.T.: -0.027 min
Response: 8959191
Conc: 1268.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

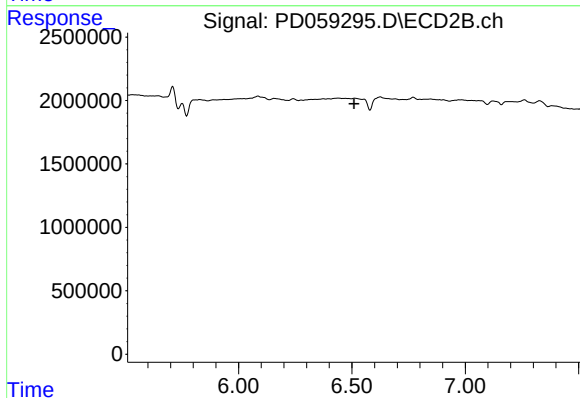


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.510 min
Response: 0
Conc: N.D.

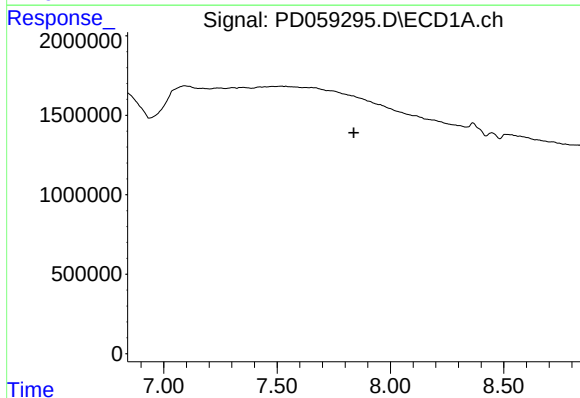

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

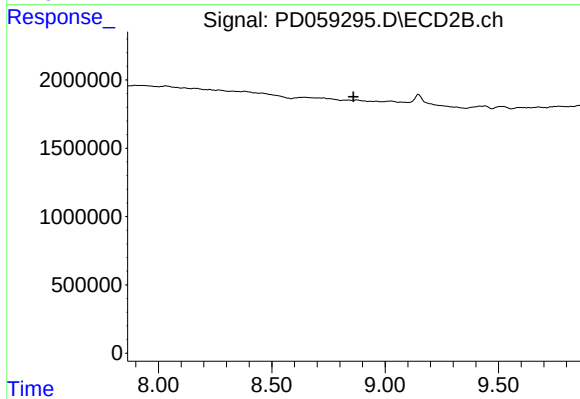

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.861 min
Response: 0
Conc: N.D.