

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
 Data File : PD059309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 17:20
 Operator : DD\AJ
 Sample : PB131853BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:22:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:19:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	19238656	36238531	19.952	20.266
27)	SA Decachlor...	7.840	8.861	38046919	57619071	37.278	39.082
Target Compounds							
3)	MA gamma-BHC...	3.910	0.000	937266	0	0.669	N.D. #
6)	B beta-BHC	0.000	4.651f	0	412244	N.D.	0.394
8)	B Heptachlo...	0.000	5.760f	0	391352	N.D.	0.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
Data File : PD059309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 17:20
Operator : DD\AJ
Sample : PB131853BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:22:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:19:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

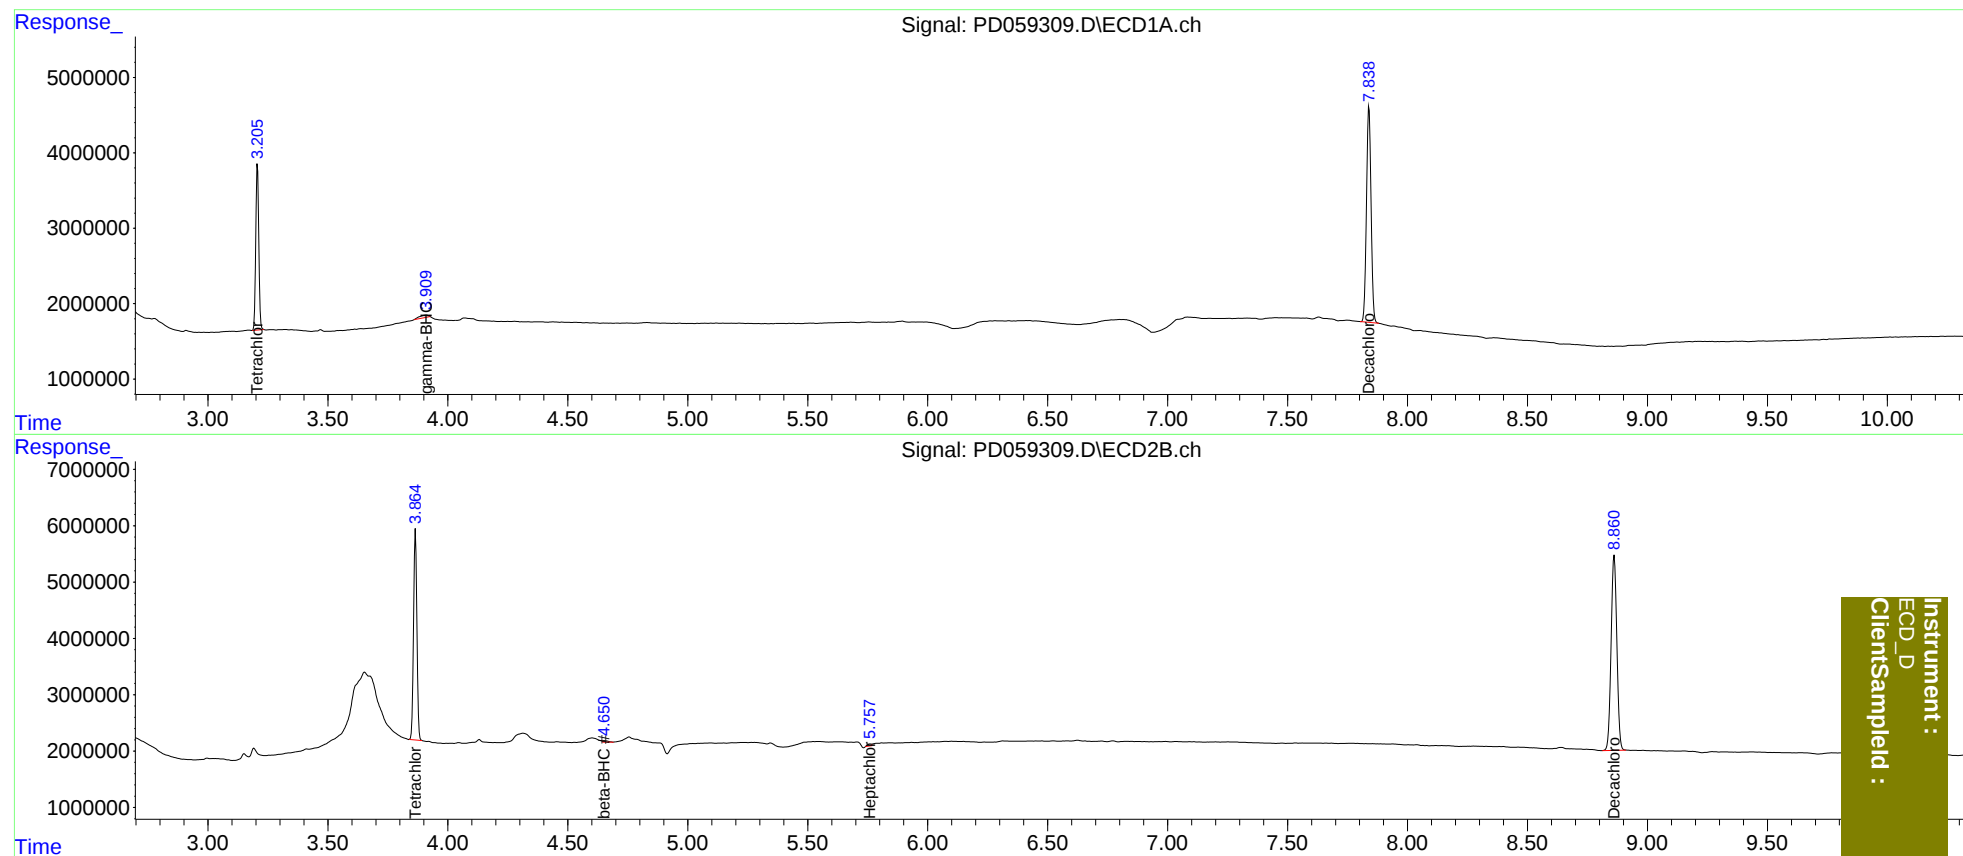


Instrument :
ECD_D
ClientSampleId :

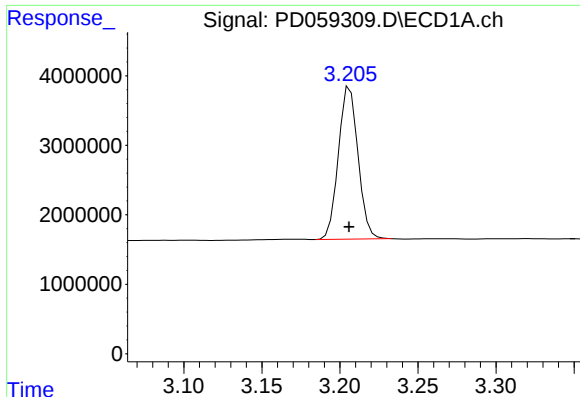

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 19238656
Conc: 19.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

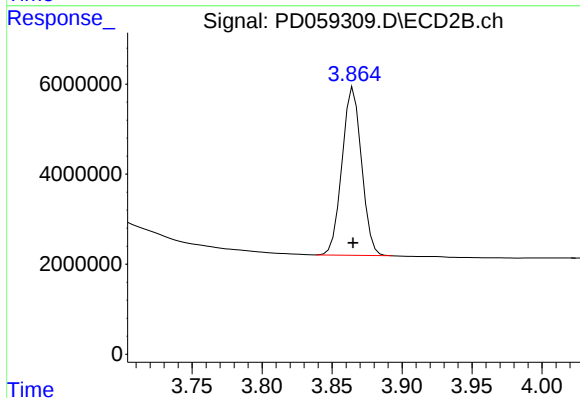


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 36238531
Conc: 20.27 ng/ml

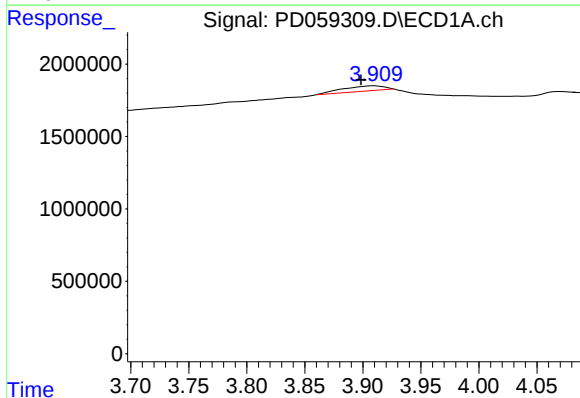


#3 gamma-BHC (Lindane)

R.T.: 3.910 min
Delta R.T.: 0.012 min
Response: 937266
Conc: 0.67 ng/ml

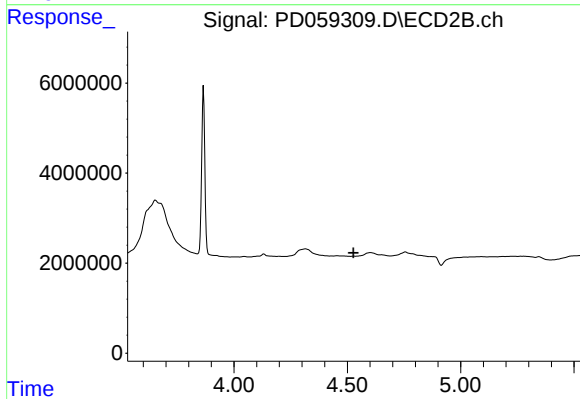

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

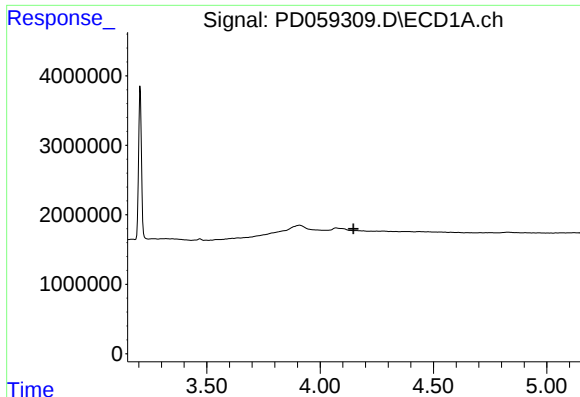

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

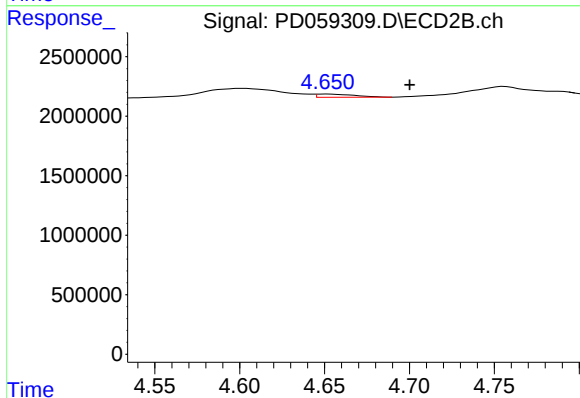


#6 beta-BHC

R.T.: 4.651 min
Delta R.T.: -0.049 min
Response: 412244
Conc: 0.39 ng/ml

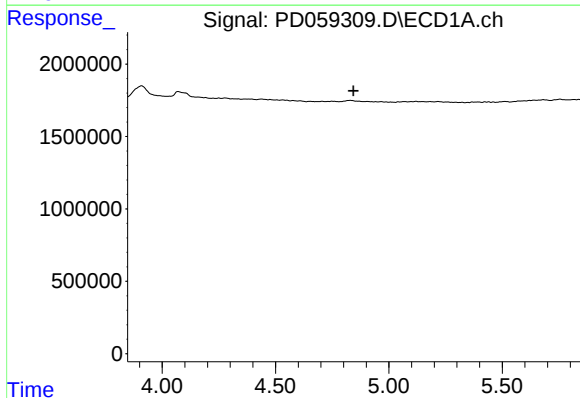


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.844 min
Response: 0
Conc: N.D.

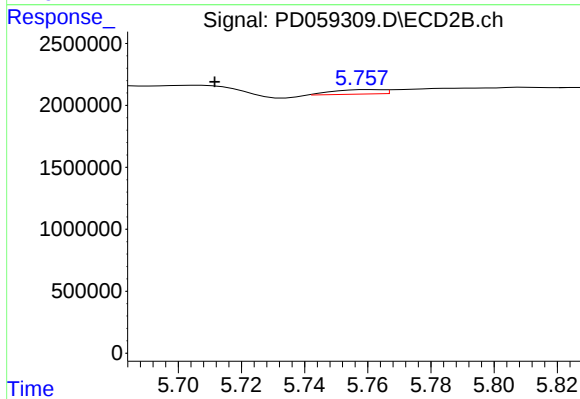

#8 Heptachlor epoxide


R.T.: 5.760 min
Delta R.T.: 0.049 min
Response: 391352
Conc: 0.20 ng/ml

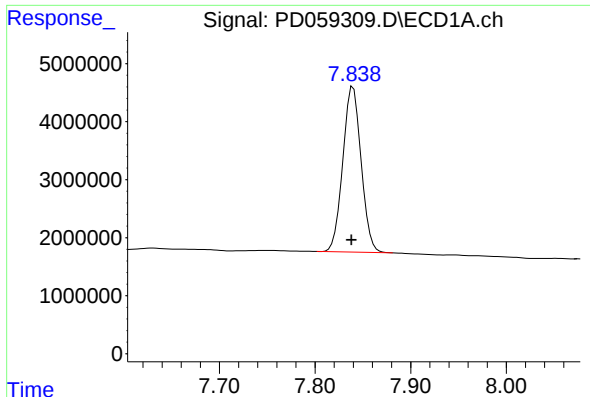

#27 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.002 min
Response: 38046919
Conc: 37.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

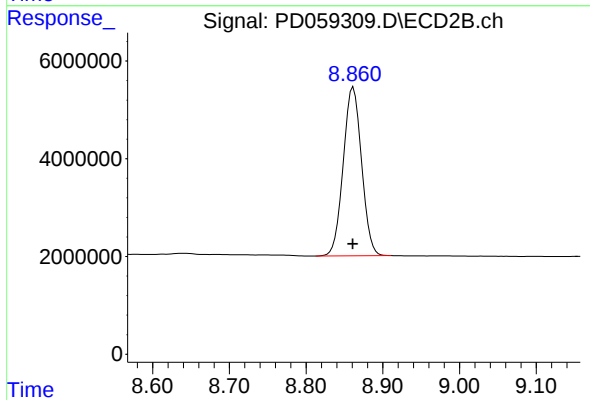

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 57619071
Conc: 39.08 ng/ml