

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
 Data File : PD059319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 19:42
 Operator : DD\AJ
 Sample : MDL-TOX-BL-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:49:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:19:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	19930716	37274745	20.670	20.846
2)	SA Decachlor...	7.839	8.861	38818467	58248794	38.034	39.510
Target Compounds							
3)	MA gamma-BHC...	3.909	0.000	921476	0	0.658	N.D. #
10)	B trans-Chl...	0.000	5.886f	0	119038	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092320\
Data File : PD059319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 19:42
Operator : DD\AJ
Sample : MDL-TOX-BL-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:49:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:19:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

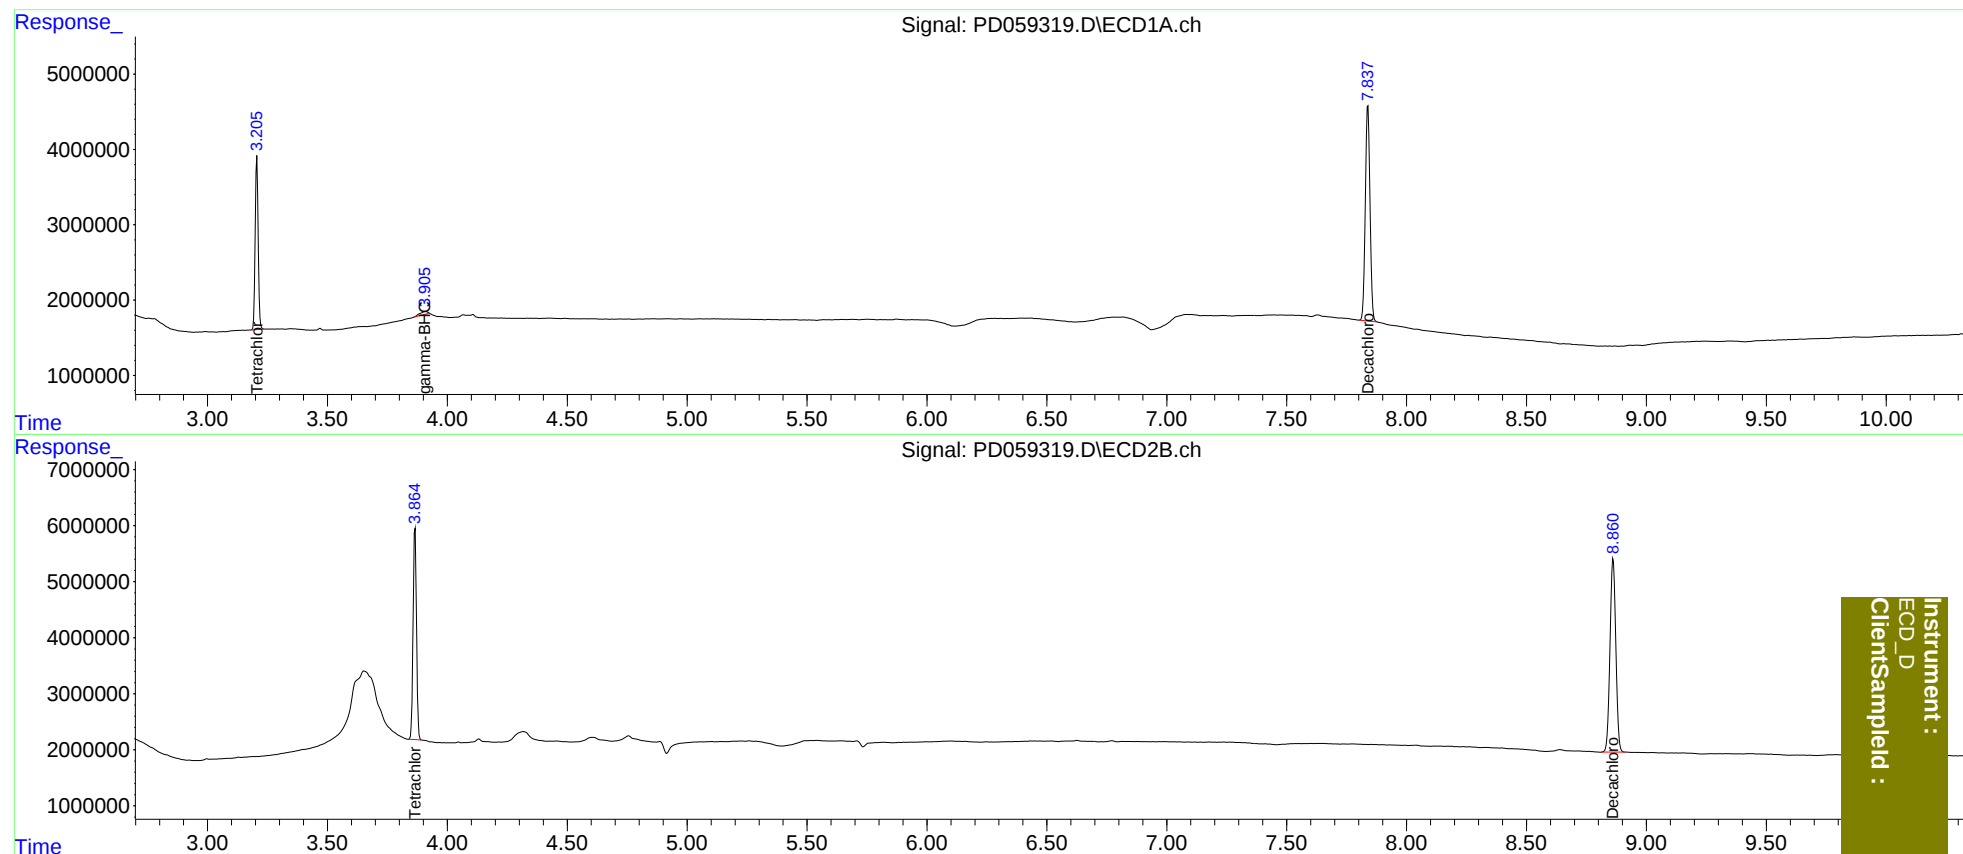


Instrument :
ECD_D
ClientSampleId :

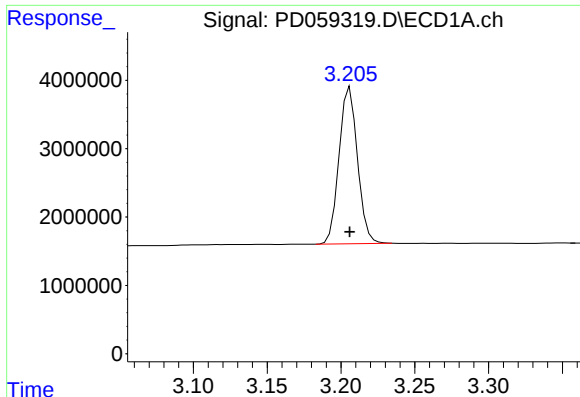

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 19930716
Conc: 20.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

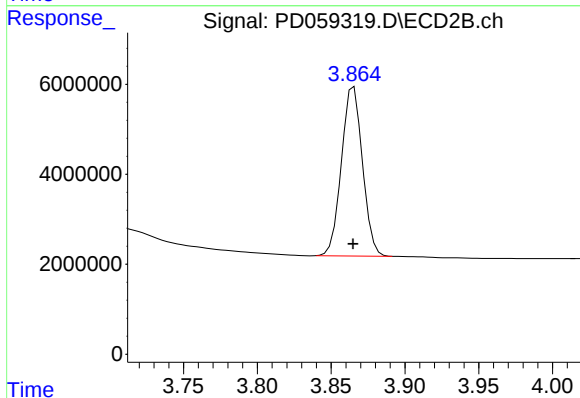


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 37274745
Conc: 20.85 ng/ml

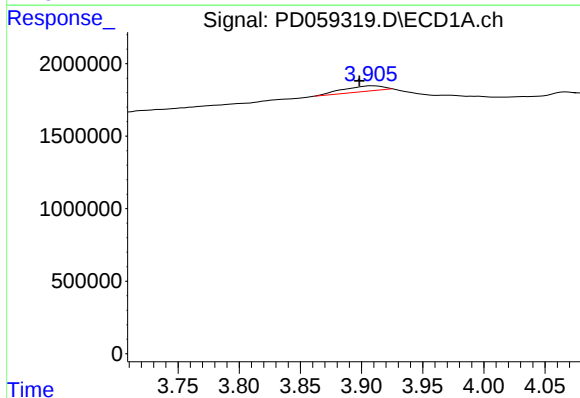


#3 gamma-BHC (Lindane)

R.T.: 3.909 min
Delta R.T.: 0.011 min
Response: 921476
Conc: 0.66 ng/ml

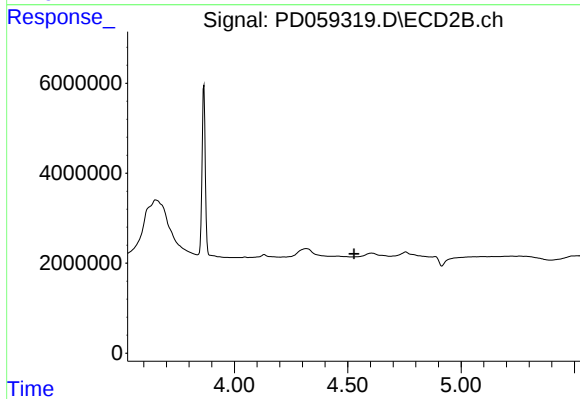

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

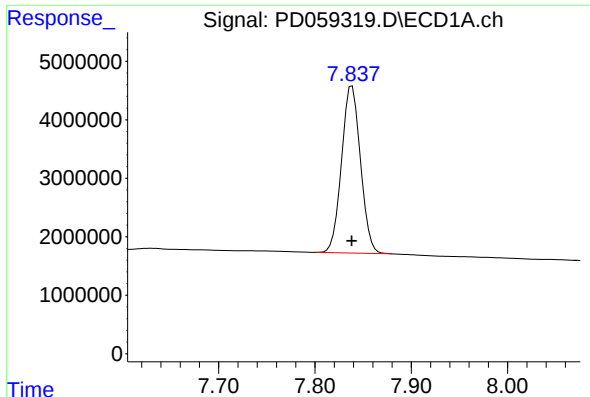

#27 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 38818467
Conc: 38.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

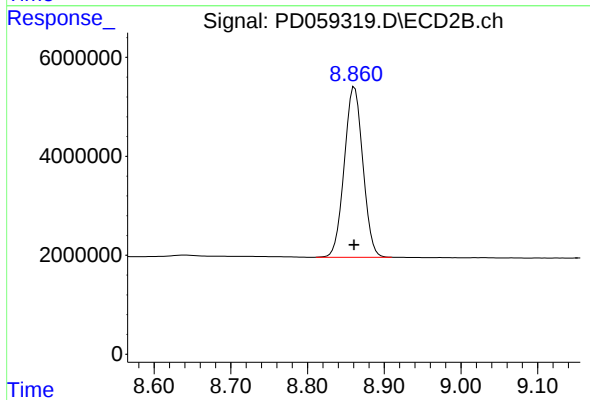

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 58248794
Conc: 39.51 ng/ml