

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
 Data File : PD065825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2021 17:18
 Operator : AR\AJ
 Sample : PB1309087BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB139087BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:33:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	17814492	137.6E6	24.056	23.958
28)	SA Decachlor...	8.235	9.084	33100181	94933952	24.232	24.530
Target Compounds							
6)	B beta-BHC	0.000	4.889f	0	3106267	N.D.	0.840 #
7)	B delta-BHC	0.000	5.095	0	1364703	N.D.	0.190 #
15)	B Endosulfa...	6.321	0.000	871146	0	0.806	N.D. #
19)	B Endosulfa...	6.692	0.000	588693	0	0.516	N.D. #
22)	Mirex	7.387	8.223	981453	4291246	0.813	1.087 #
27)	Chlordane-5	6.321	0.000	871146	0	17.925	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
Data File : PD065825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2021 17:18
Operator : AR\AJ
Sample : PB1309087BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB139087BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:33:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

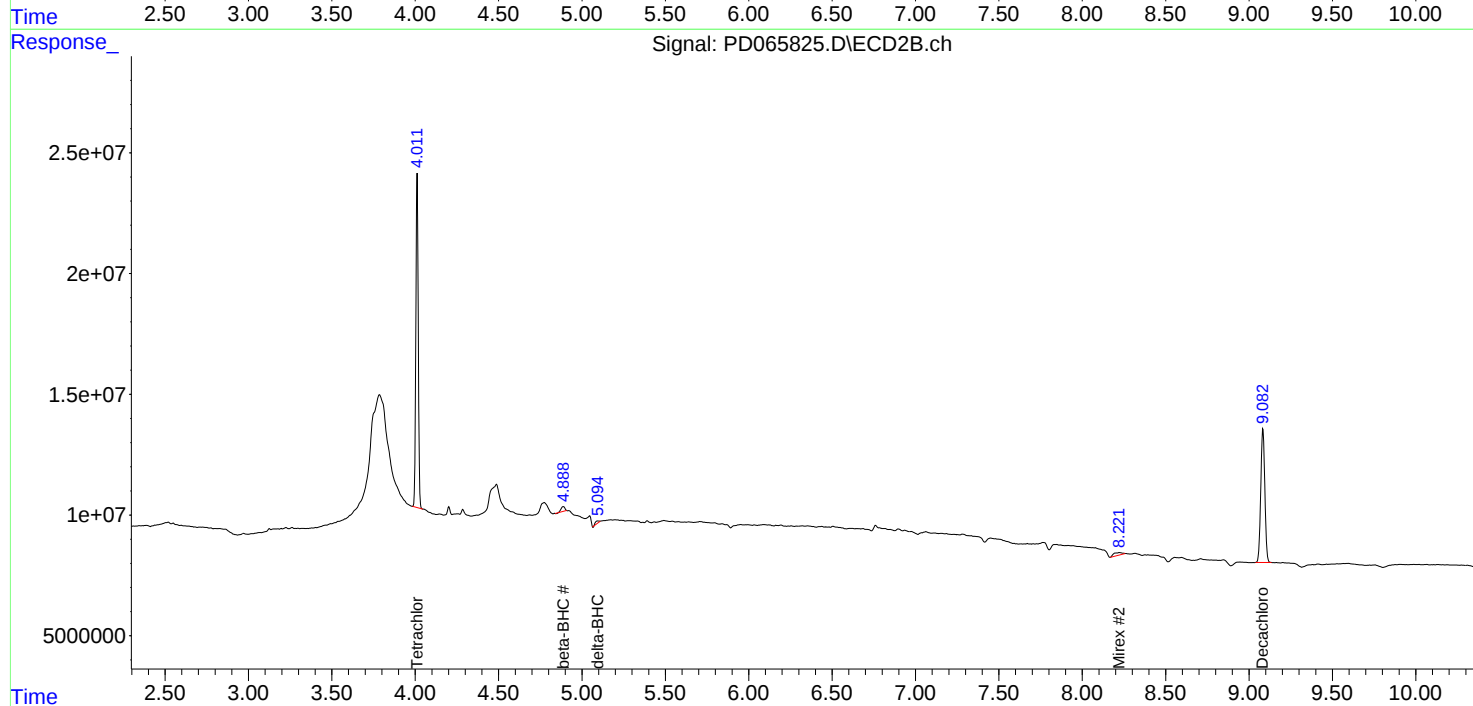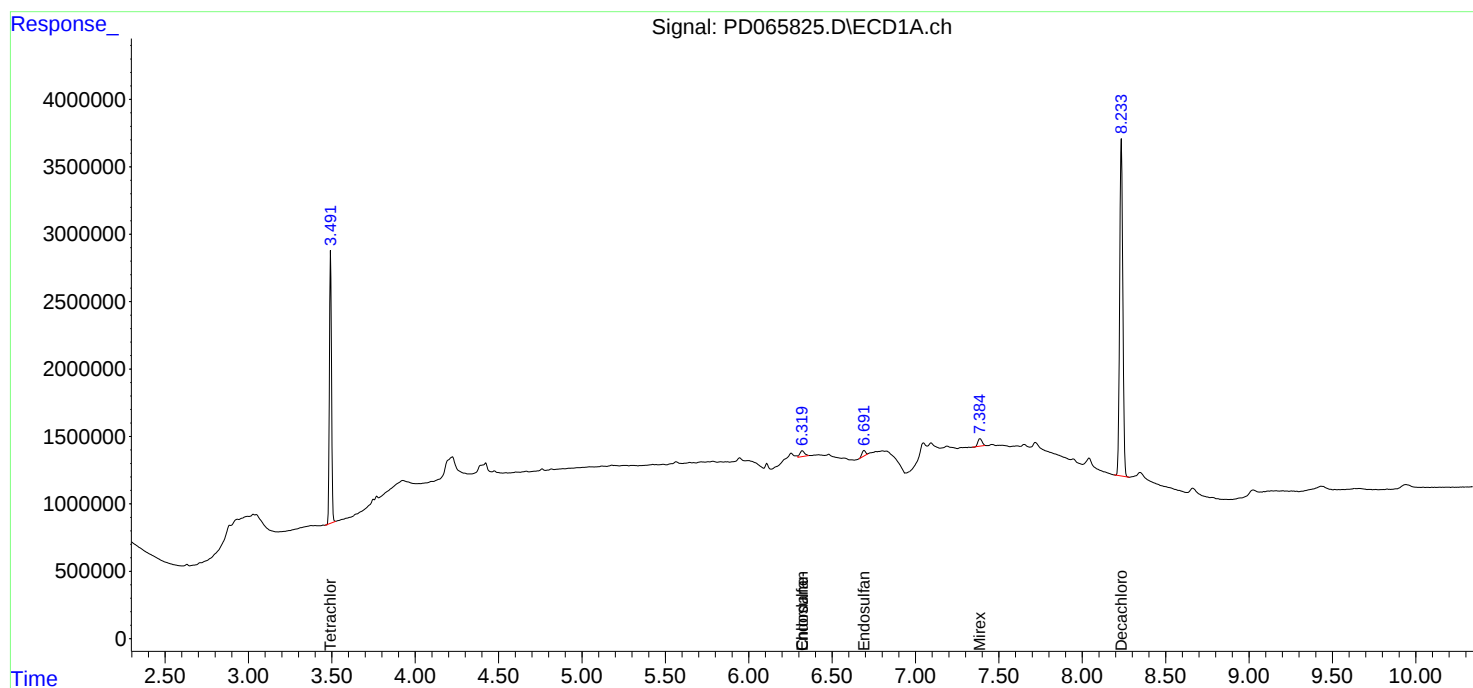


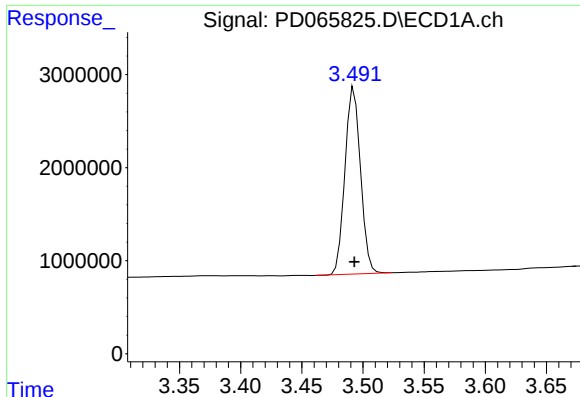

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 17814492
Conc: 24.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB139087BL

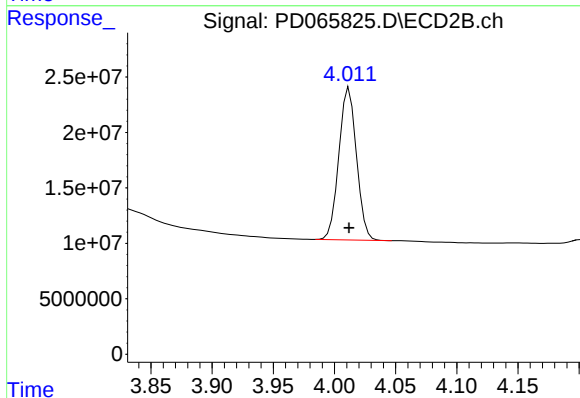


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 137570205
Conc: 23.96 ng/ml

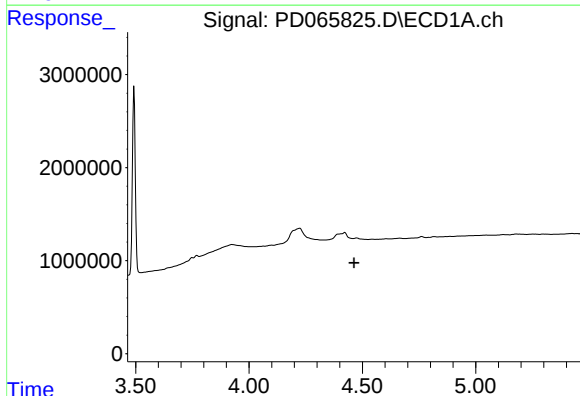


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.464 min
Response: 0
Conc: N.D.

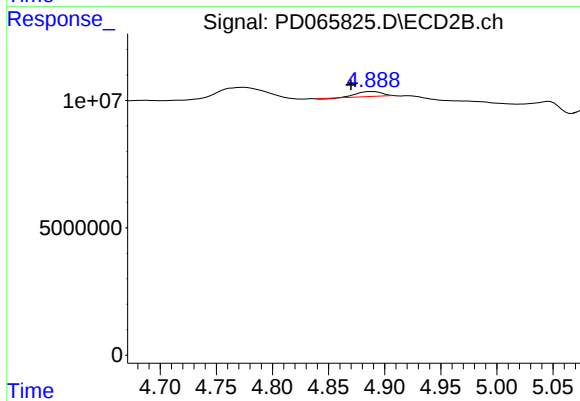

#6 beta-BHC


R.T.: 4.889 min
Delta R.T.: 0.019 min
Response: 3106267
Conc: 0.84 ng/ml

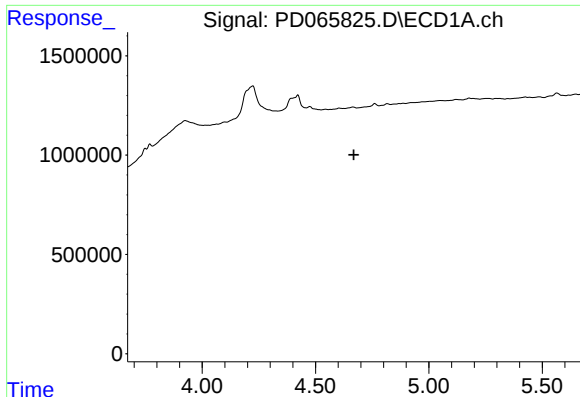

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.668 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB139087BL

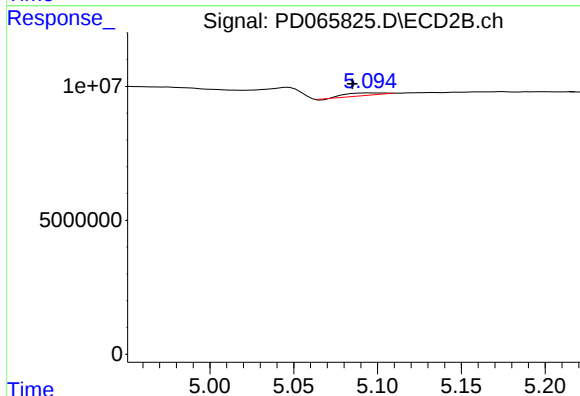


#7 delta-BHC

R.T.: 5.095 min
Delta R.T.: 0.010 min
Response: 1364703
Conc: 0.19 ng/ml

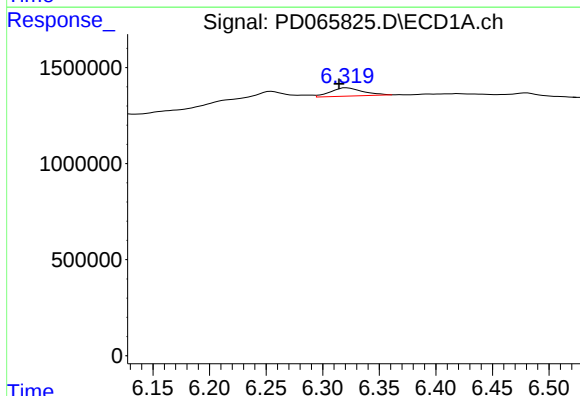


#15 Endosulfan II

R.T.: 6.321 min
Delta R.T.: 0.007 min
Response: 871146
Conc: 0.81 ng/ml

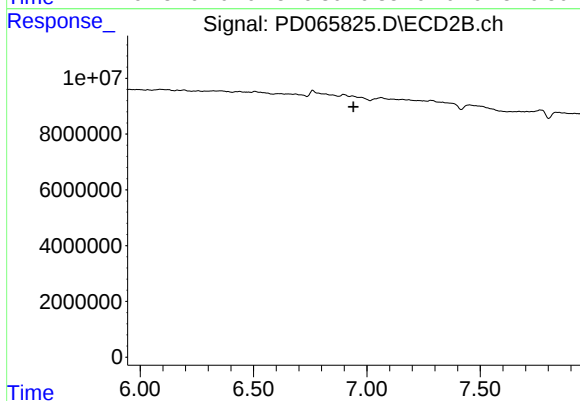

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.941 min
Response: 0
Conc: N.D.

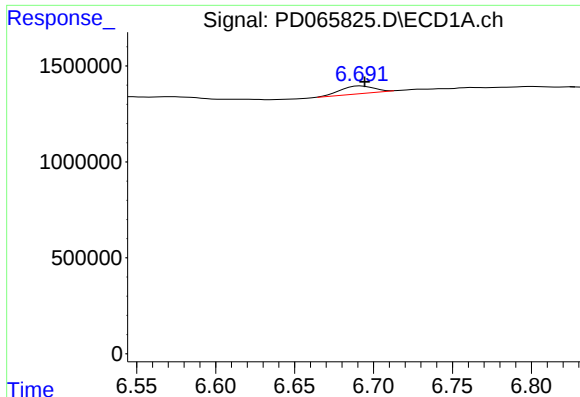

#19 Endosulfan Sulfate


R.T.: 6.692 min
Delta R.T.: -0.002 min
Response: 588693
Conc: 0.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB139087BL

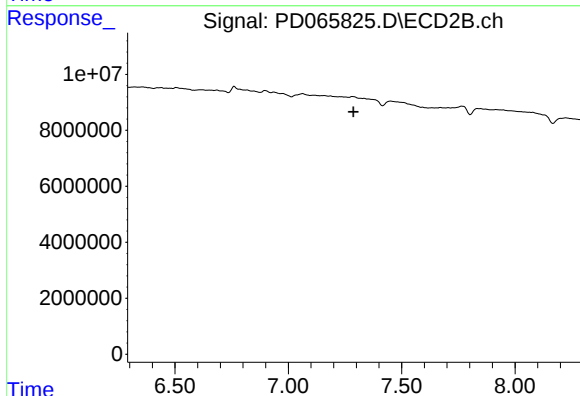


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.288 min
Response: 0
Conc: N.D.

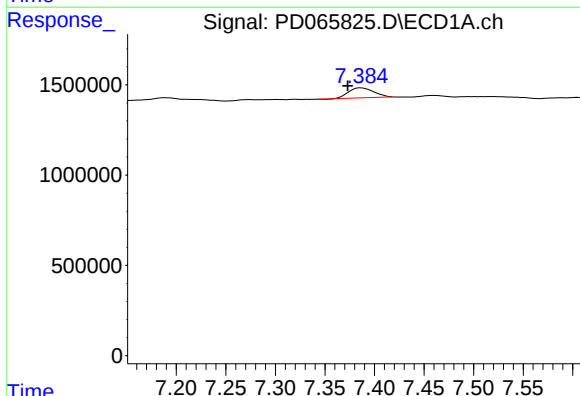


#22 Mirex

R.T.: 7.387 min
Delta R.T.: 0.014 min
Response: 981453
Conc: 0.81 ng/ml

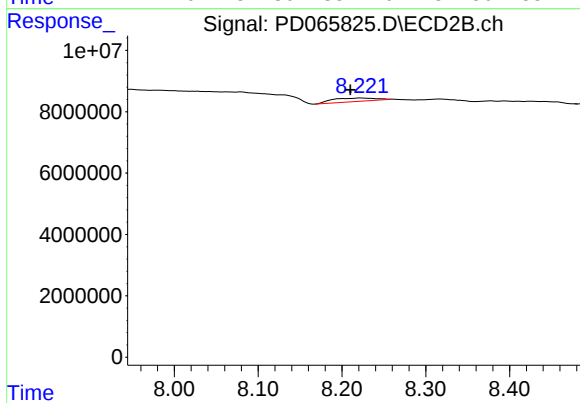

#22 Mirex


R.T.: 8.223 min
Delta R.T.: 0.013 min
Response: 4291246
Conc: 1.09 ng/ml

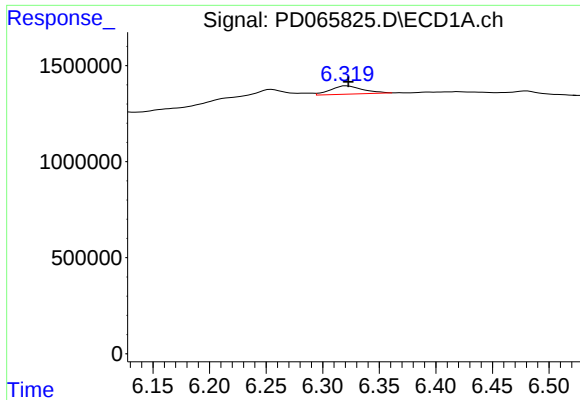

#27 Chlordane-5


R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 871146
Conc: 17.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB139087BL

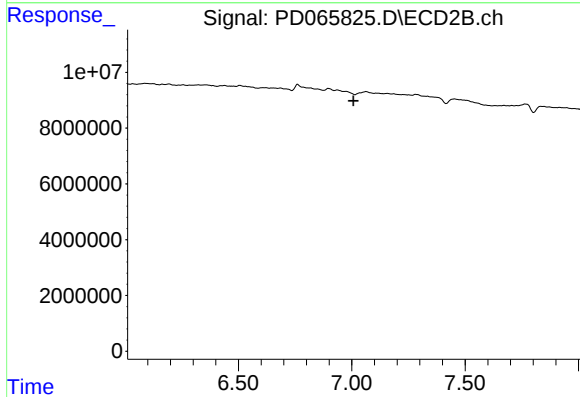


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

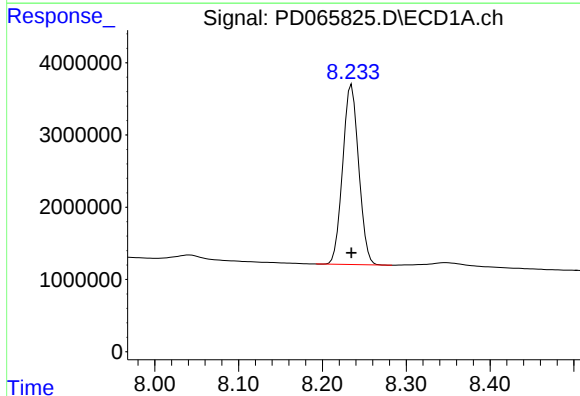

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 33100181
Conc: 24.23 ng/ml

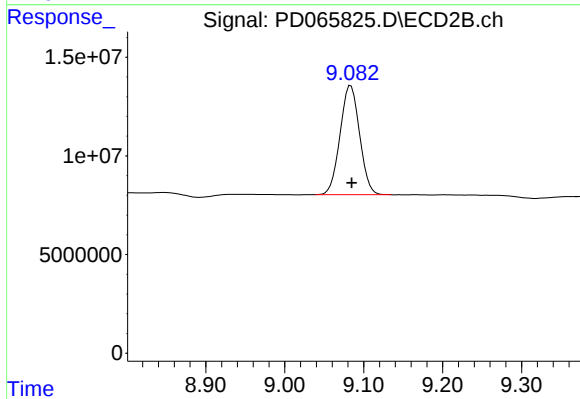

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.001 min
Response: 94933952
Conc: 24.53 ng/ml