

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
 Data File : PD065813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2021 13:25
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 16:09:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.012	41901892	274.3E6	56.582	47.766
28)	SA Decachlor...	8.239	9.087	62850438	184.1E6	46.012	47.581
Target Compounds							
23)	Chlordane-1	4.364	5.008	15191319	105.1E6	453.510	474.829
24)	Chlordane-2	4.865	5.478	18531482	101.1E6	456.310	437.002
25)	Chlordane-3	5.431	6.126	51719495	364.4E6	438.991	444.324
26)	Chlordane-4	5.489	6.199	43531164	425.7E6	440.758	443.798
27)	Chlordane-5	6.326	7.009	20915195	82694913	430.352	444.980



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
Data File : PD065813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2021 13:25
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 16:09:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

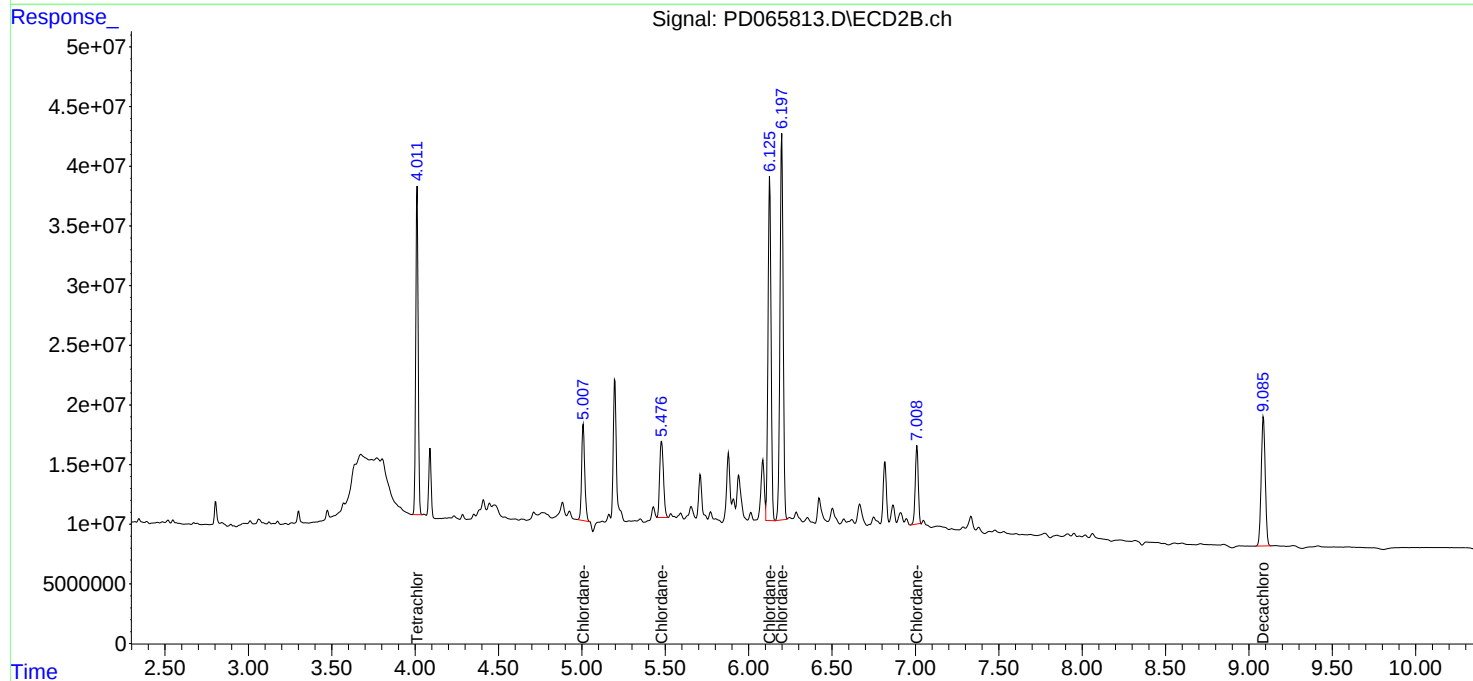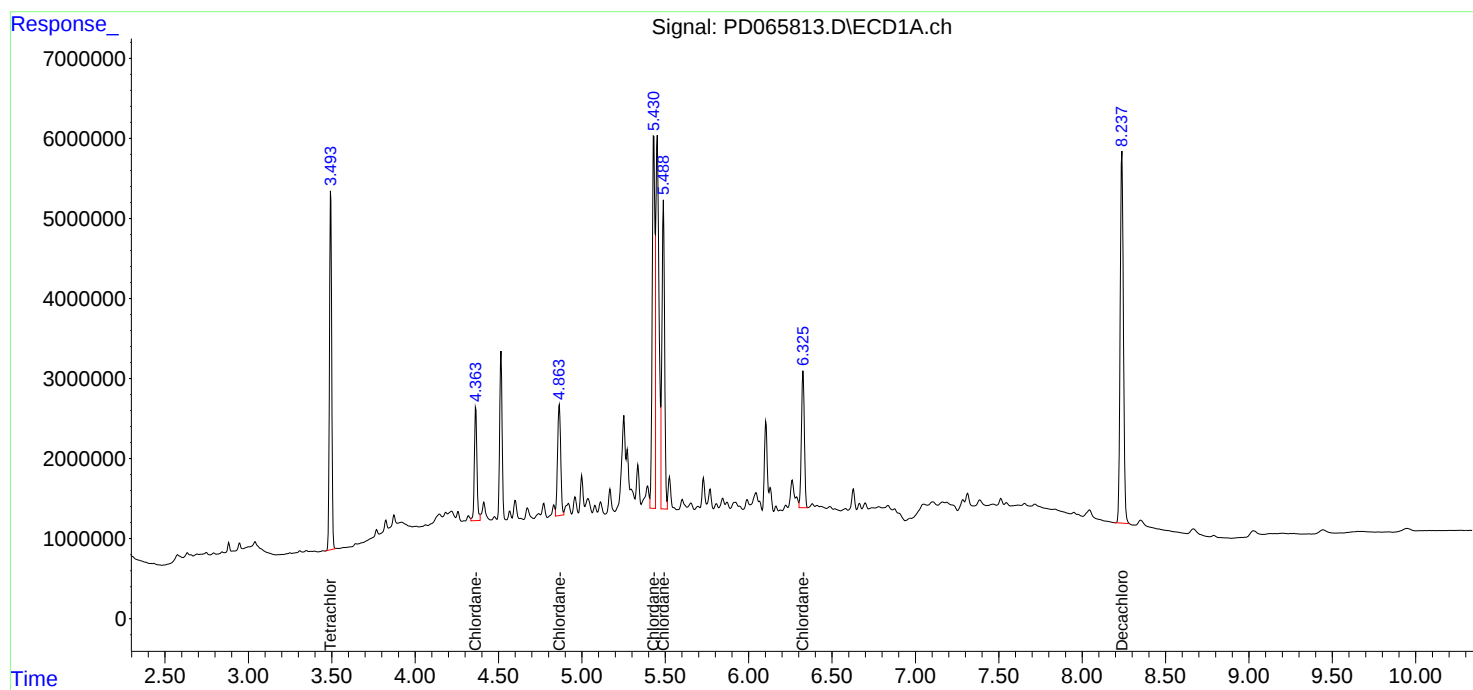


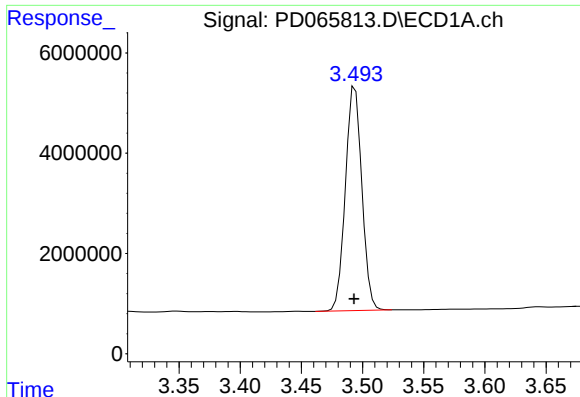

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 41901892
Conc: 56.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

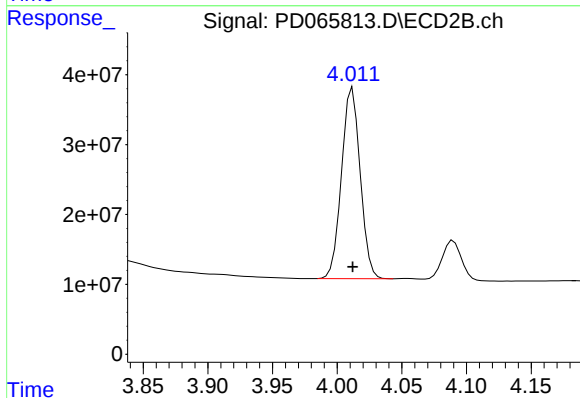


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 274276901
Conc: 47.77 ng/ml

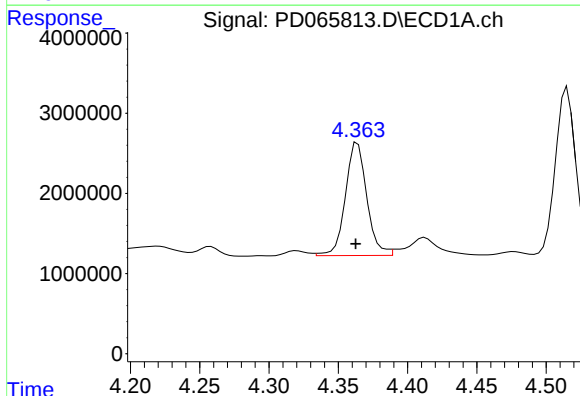


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.001 min
Response: 15191319
Conc: 453.51 ng/ml

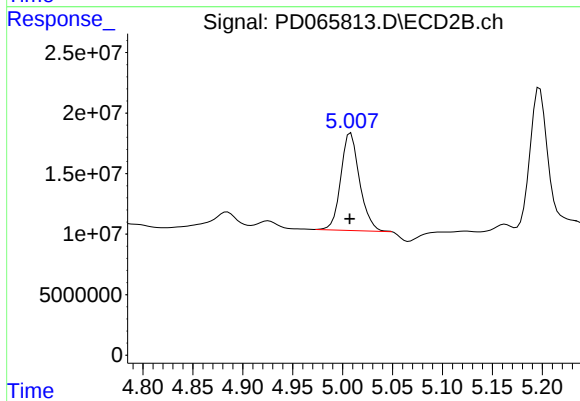

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 105133636
Conc: 474.83 ng/ml

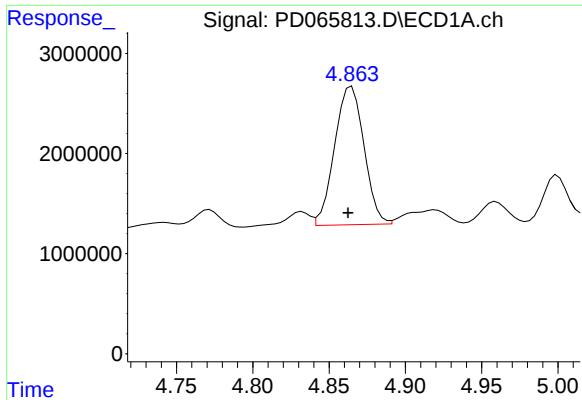

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.002 min
Response: 18531482
Conc: 456.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

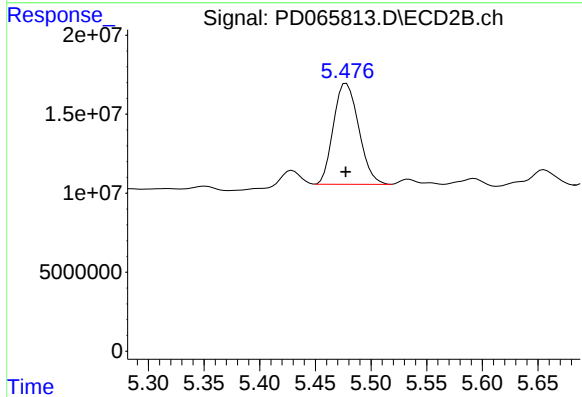


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 101084037
Conc: 437.00 ng/ml

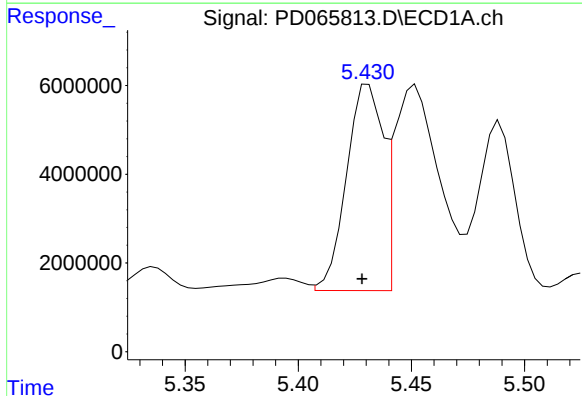


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.003 min
Response: 51719495
Conc: 438.99 ng/ml

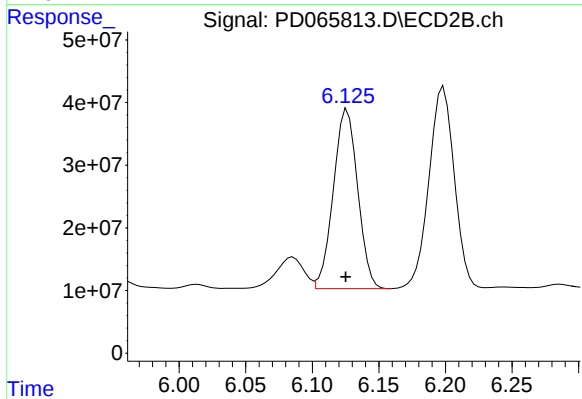

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.001 min
Response: 364370643
Conc: 444.32 ng/ml

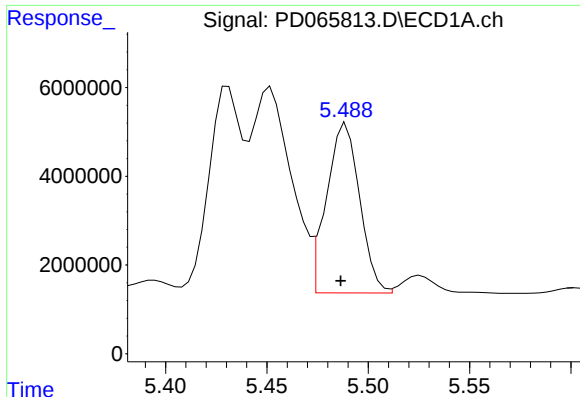

#26 Chlordane-4


R.T.: 5.489 min
Delta R.T.: 0.003 min
Response: 43531164
Conc: 440.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

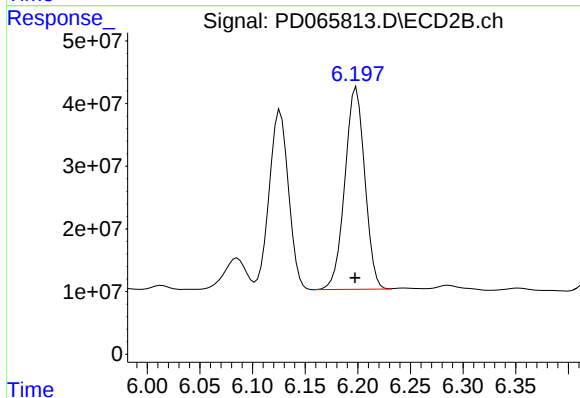


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 425673917
Conc: 443.80 ng/ml

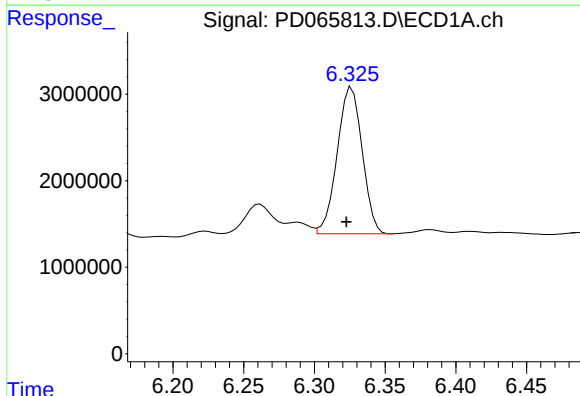


#27 Chlordane-5

R.T.: 6.326 min
Delta R.T.: 0.004 min
Response: 20915195
Conc: 430.35 ng/ml

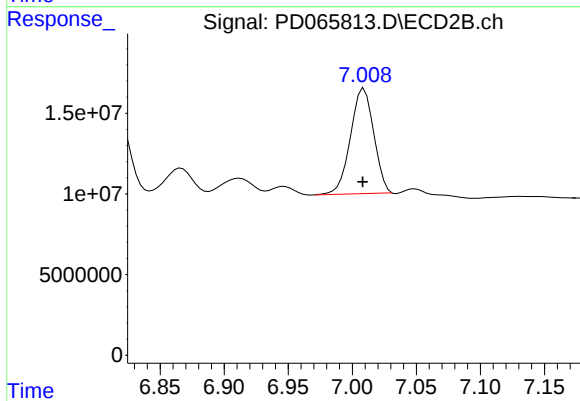

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.001 min
Response: 82694913
Conc: 444.98 ng/ml

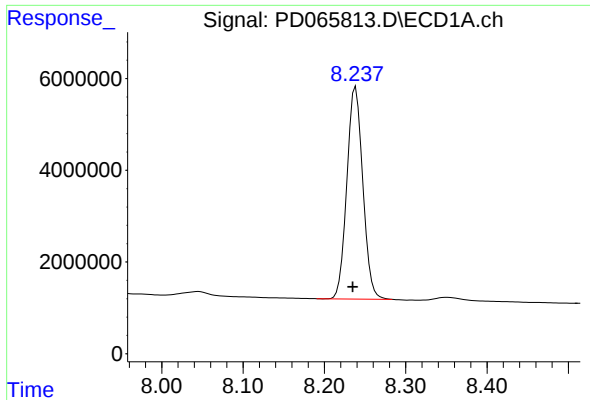

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.004 min
Response: 62850438
Conc: 46.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

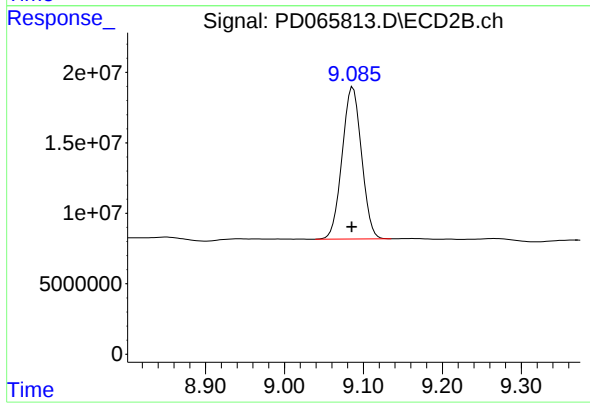

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.002 min
Response: 184146523
Conc: 47.58 ng/ml