

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
 Data File : PD065816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2021 14:17
 Operator : AR\AJ
 Sample : M3702-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 16:21:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	4.012	43924350	135.6E6	59.313	23.618 #
28)	SA Decachlor...	8.236	9.085	35838329	98294976	26.237	25.398
Target Compounds							
23)	Chlordane-1	4.362	5.008	71109272	522.6E6	2122.844	2360.428
24)	Chlordane-2	4.862	5.478	85135424	474.7E6	2096.333	2052.025
25)	Chlordane-3	5.429	6.126	316.4E6	1800.3E6	2685.379	2195.283
26)	Chlordane-4	5.487	6.199	255.3E6	1993.3E6	2584.979	2078.126
27)	Chlordane-5	6.324	7.009	99601623	396.0E6	2049.408	2130.835



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
Data File : PD065816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2021 14:17
Operator : AR\AJ
Sample : M3702-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 16:21:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

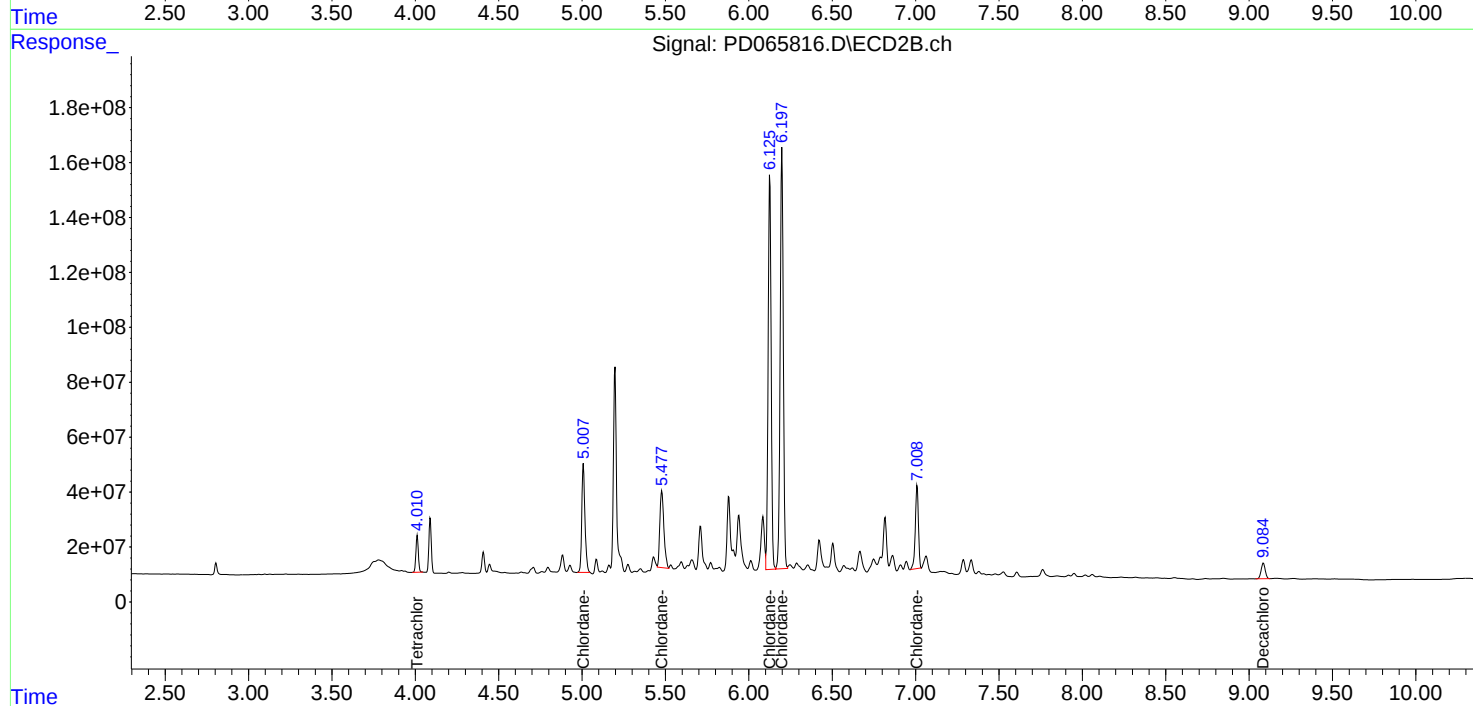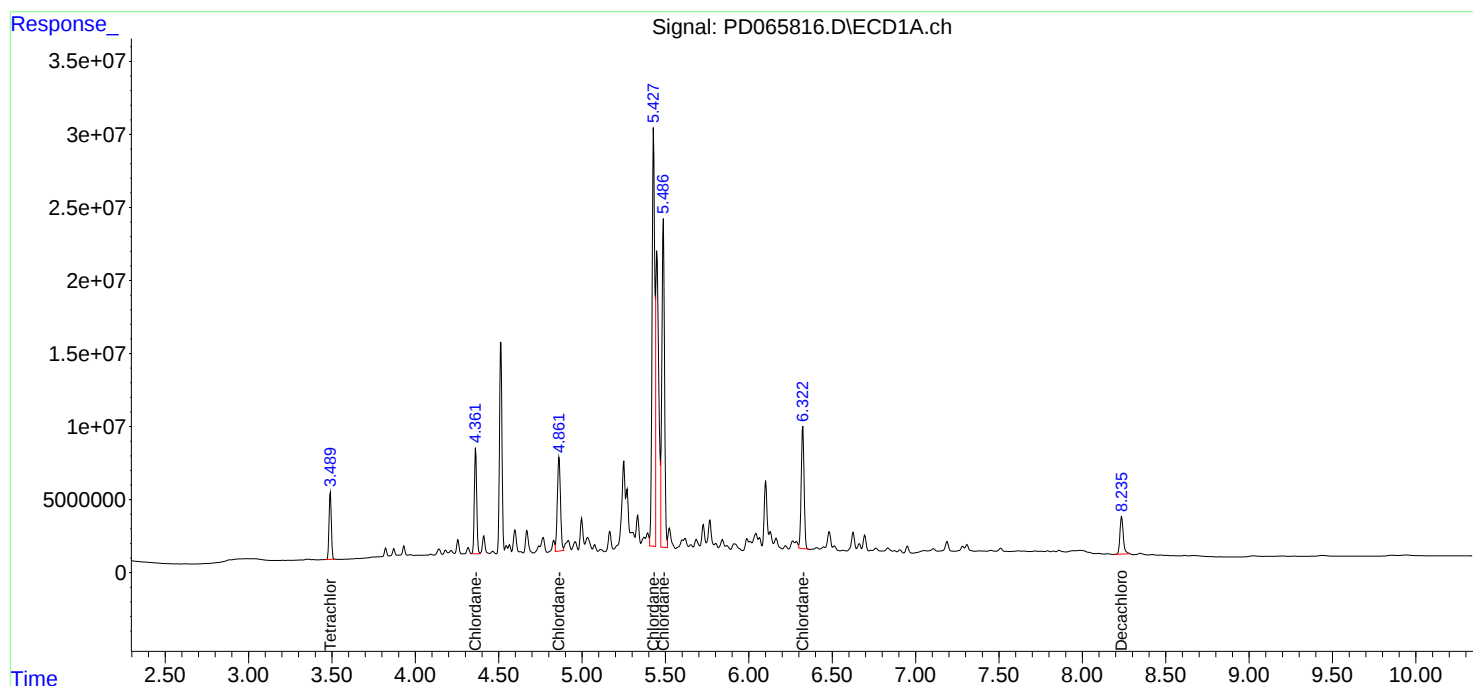


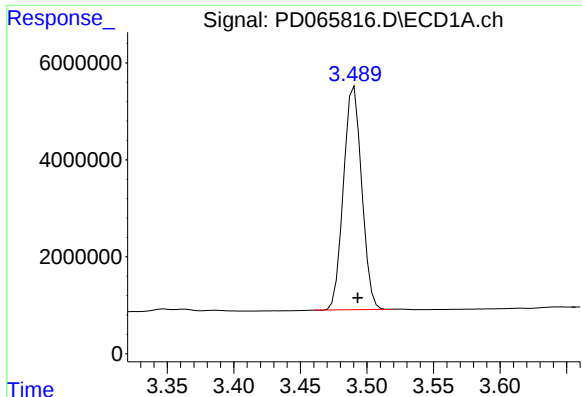

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: -0.003 min
Response: 43924350
Conc: 59.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

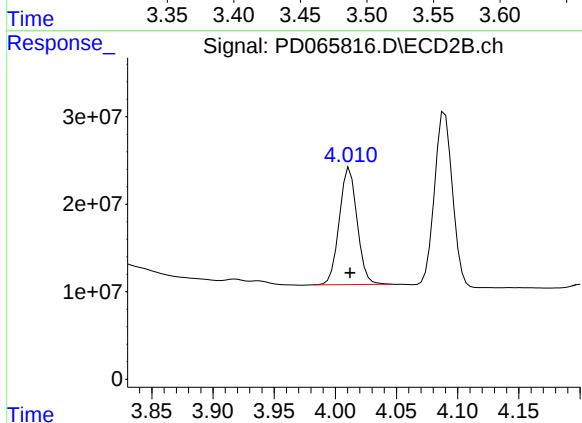


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 135620406
Conc: 23.62 ng/ml

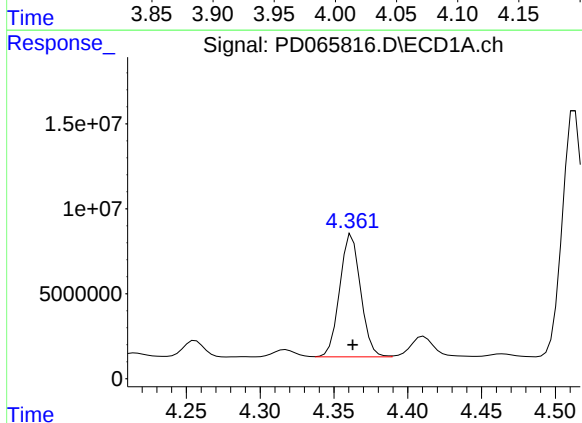


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 71109272
Conc: 2122.84 ng/ml

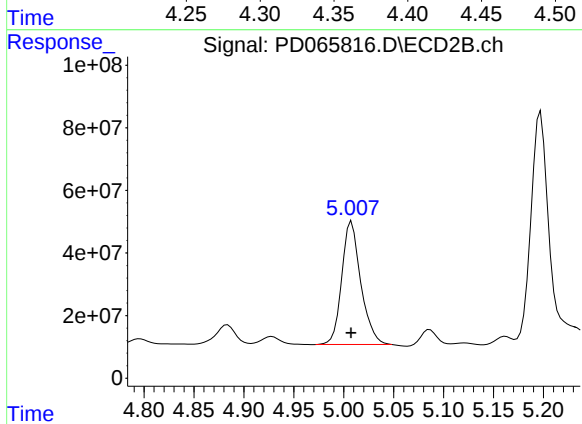

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 522630784
Conc: 2360.43 ng/ml

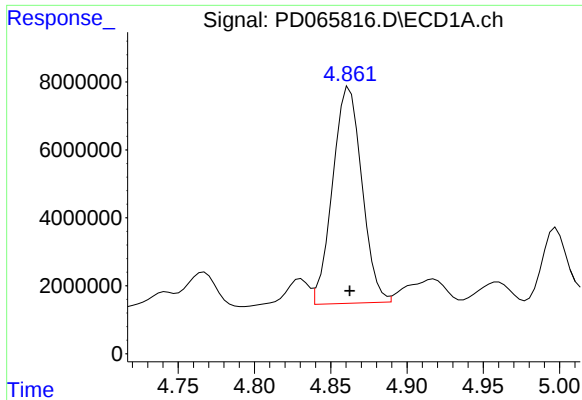

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 85135424
Conc: 2096.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

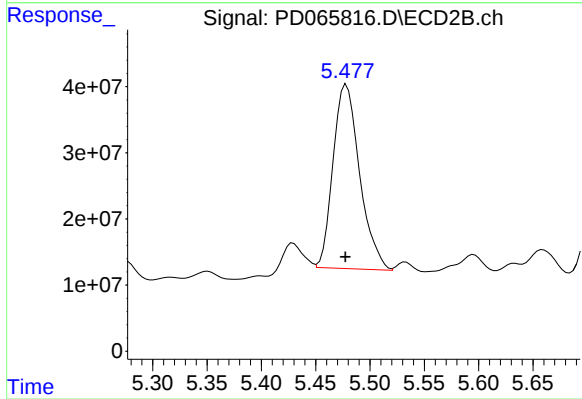


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 474658479
Conc: 2052.02 ng/ml

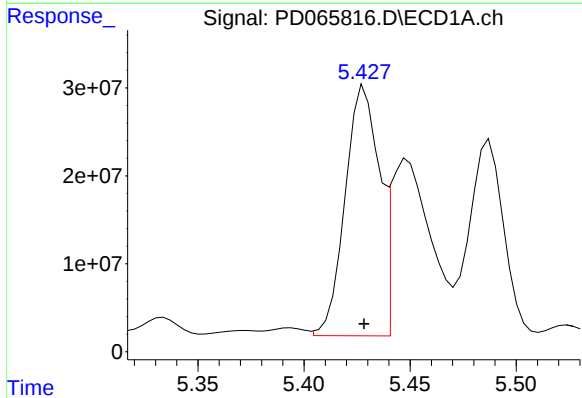


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 316376372
Conc: 2685.38 ng/ml

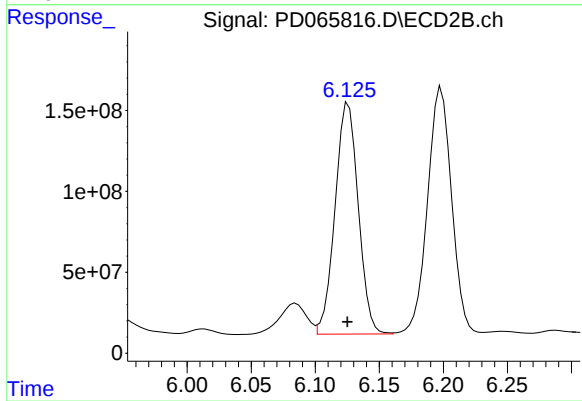

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 1800255859
Conc: 2195.28 ng/ml

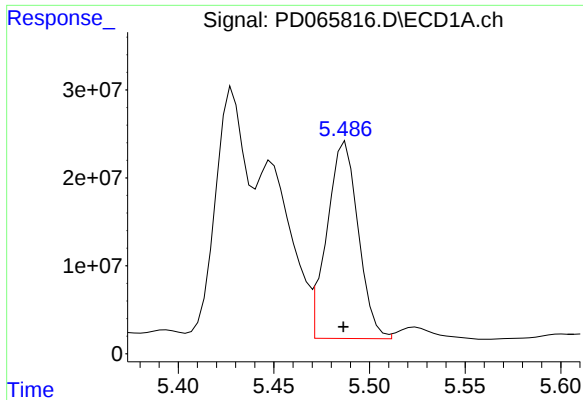

#26 Chlordane-4


R.T.: 5.487 min
Delta R.T.: 0.001 min
Response: 255303921
Conc: 2584.98 ng/m

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

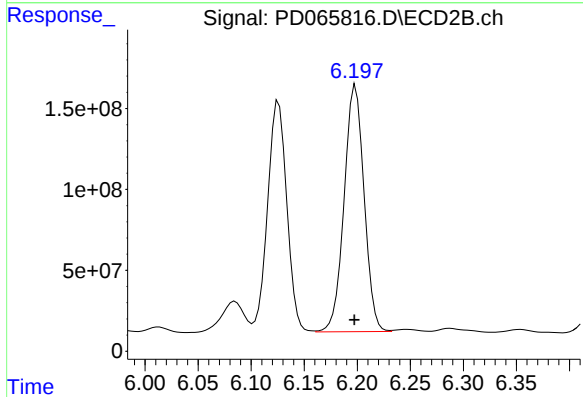


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 1993258154
Conc: 2078.13 ng/ml

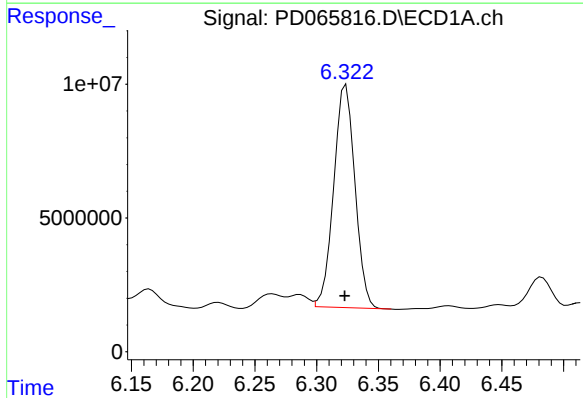


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.001 min
Response: 99601623
Conc: 2049.41 ng/ml

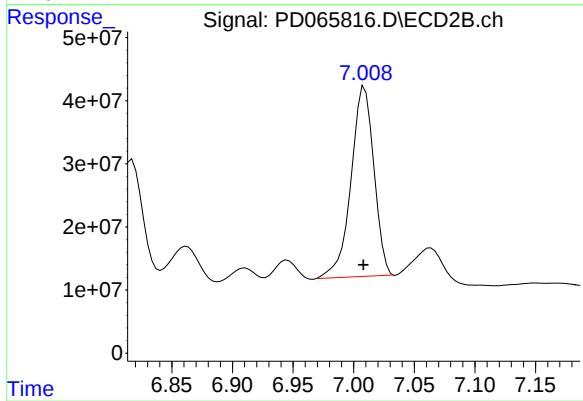

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.001 min
Response: 395993907
Conc: 2130.83 ng/ml

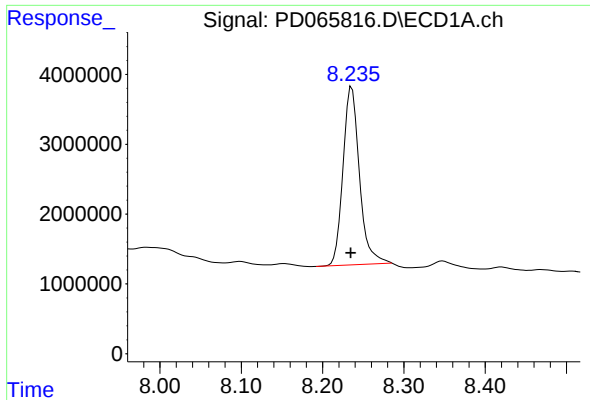

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.001 min
Response: 35838329
Conc: 26.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

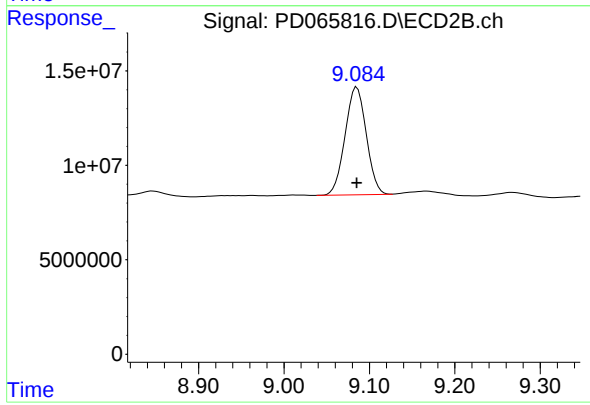

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 98294976
Conc: 25.40 ng/ml