

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
 Data File : PD065831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2021 18:41
 Operator : AR\AJ
 Sample : M3702-11DL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:35:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	4.012	9031559	29068219	12.196	5.062 #
28)	SA Decachlor...	8.235	9.085	8300286	20419985	6.077	5.276
Target Compounds							
23)	Chlordane-1	4.362	5.007	15112398	108.5E6	451.154	490.224
24)	Chlordane-2	4.862	5.478	19718534	107.7E6	485.540	465.806
25)	Chlordane-3	5.428	6.125	60720282	371.2E6	515.389	452.693
26)	Chlordane-4	5.487	6.198	50244276	420.6E6	508.729	438.500
27)	Chlordane-5	6.323	7.009	20112847	78499468	413.843	422.404



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
Data File : PD065831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2021 18:41
Operator : AR\AJ
Sample : M3702-11DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:35:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

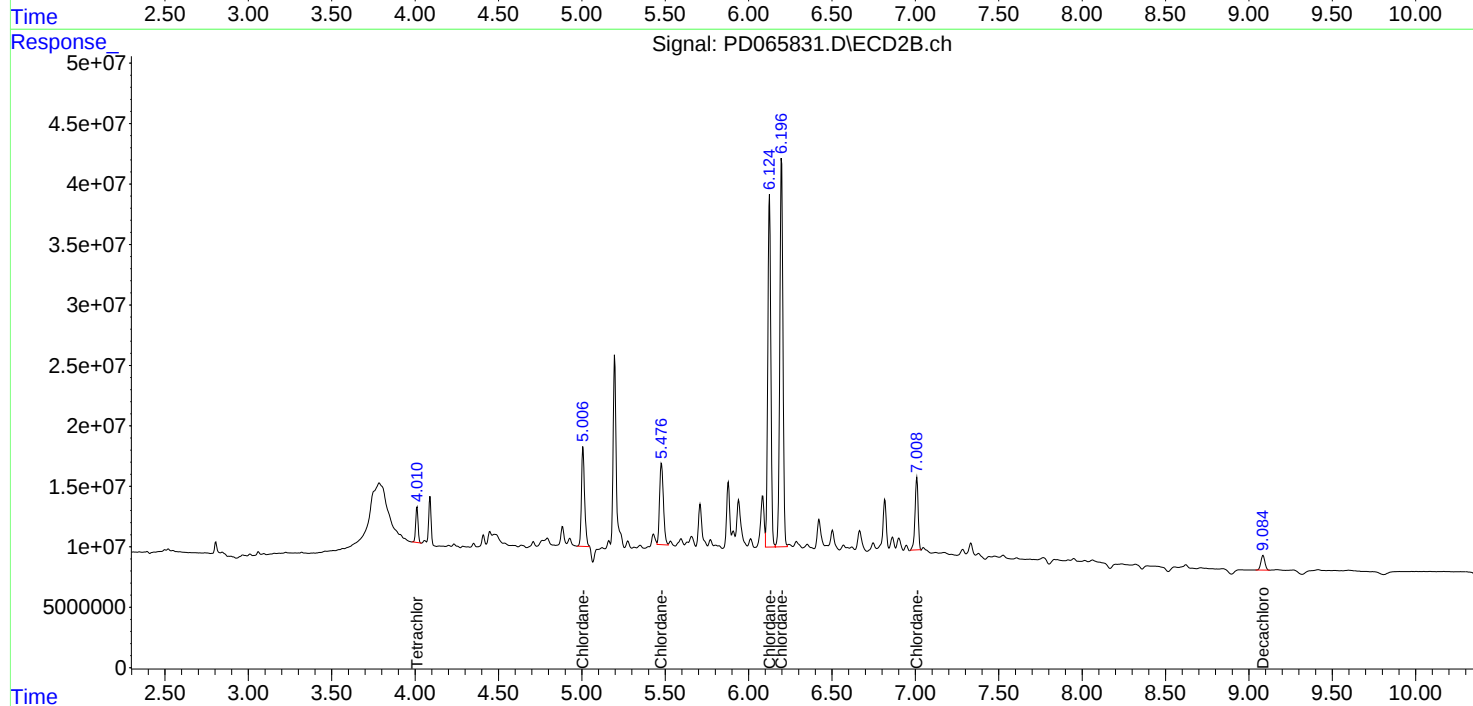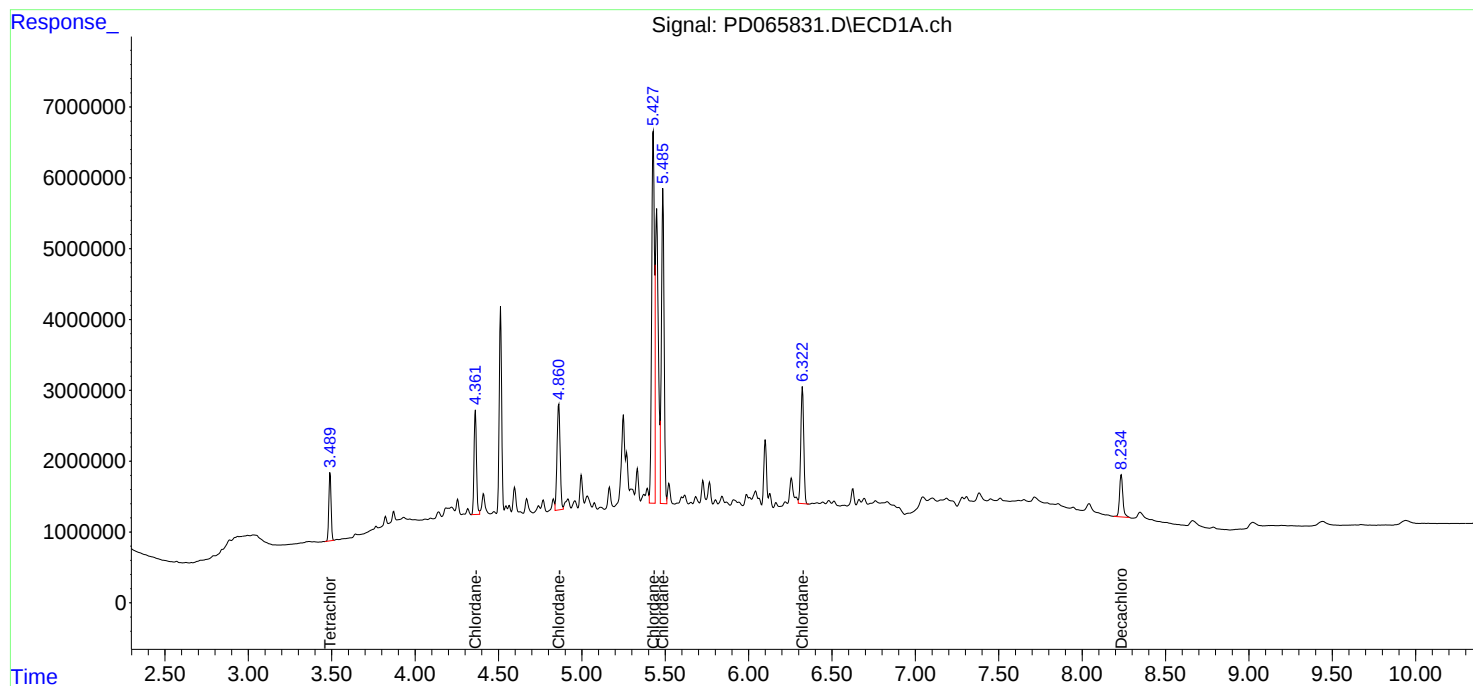


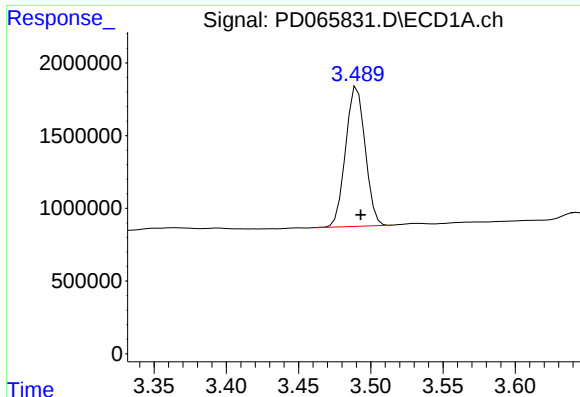

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: -0.002 min
Response: 9031559
Conc: 12.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

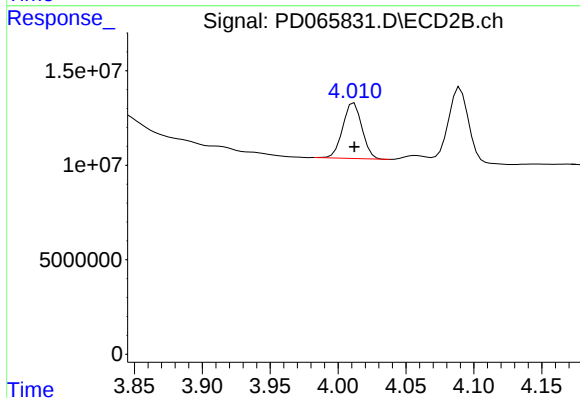


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 29068219
Conc: 5.06 ng/ml

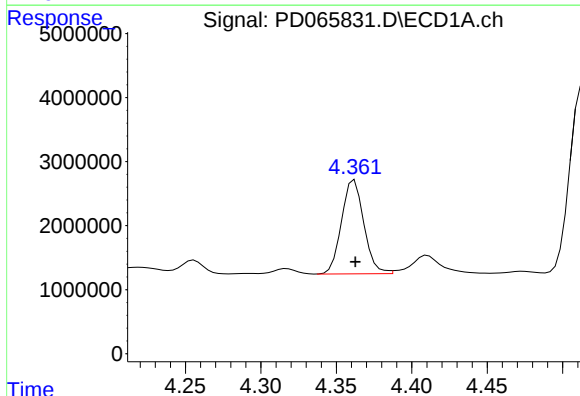


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 15112398
Conc: 451.15 ng/ml

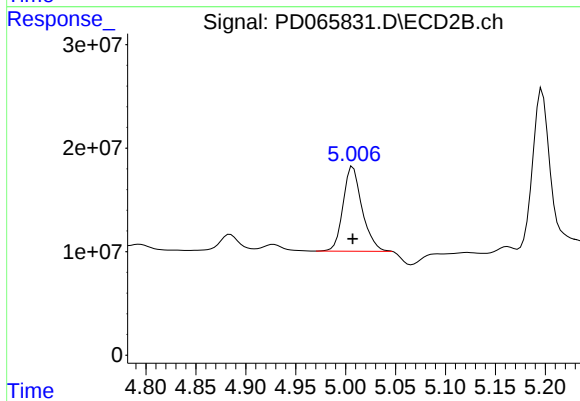

#23 Chlordane-1


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 108542217
Conc: 490.22 ng/ml

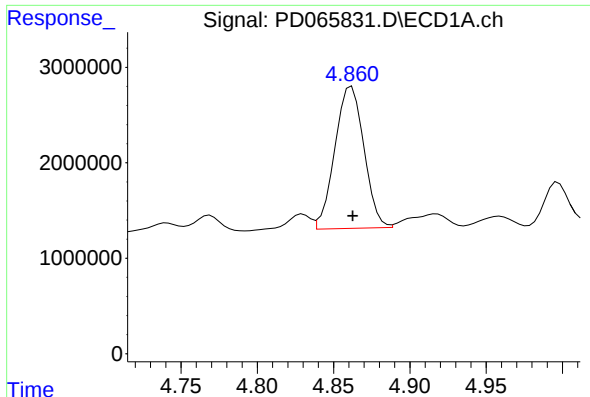

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 19718534
Conc: 485.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

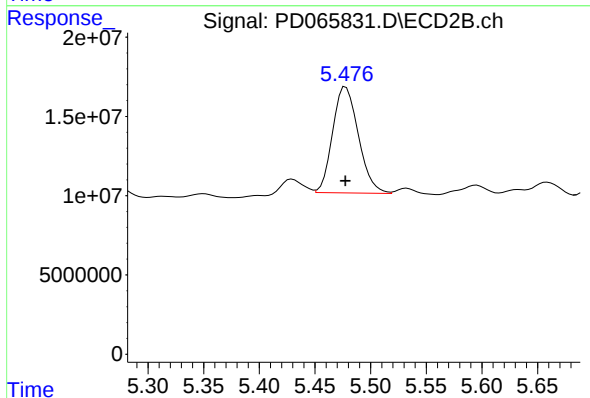


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 107746555
Conc: 465.81 ng/ml

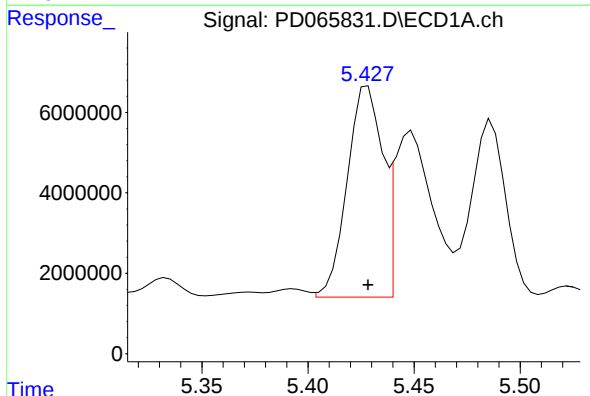


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 60720282
Conc: 515.39 ng/ml

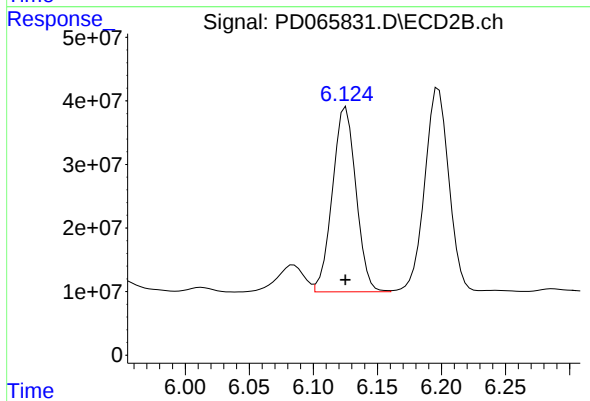

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 371234043
Conc: 452.69 ng/ml

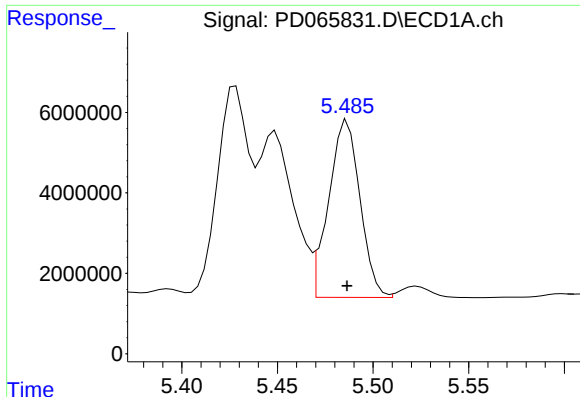

#26 Chlordane-4


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 50244276
Conc: 508.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

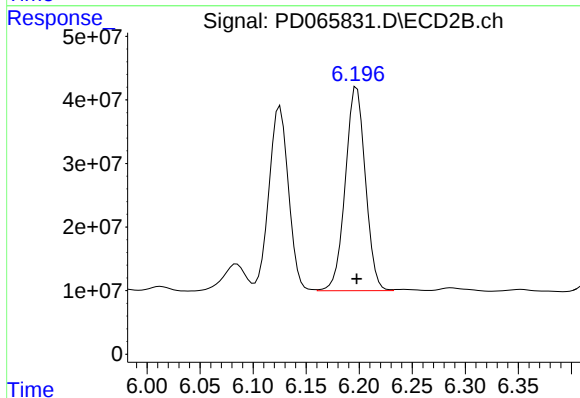


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 420591898
Conc: 438.50 ng/ml

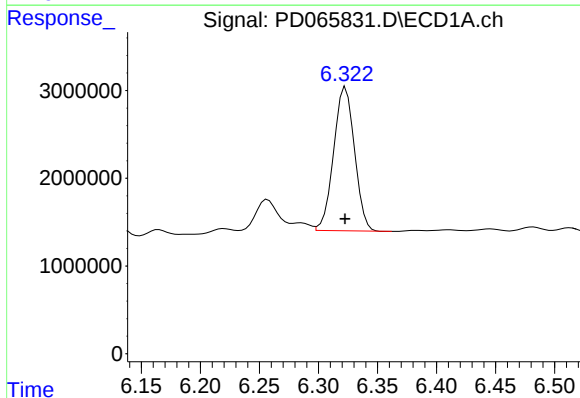


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 20112847
Conc: 413.84 ng/ml

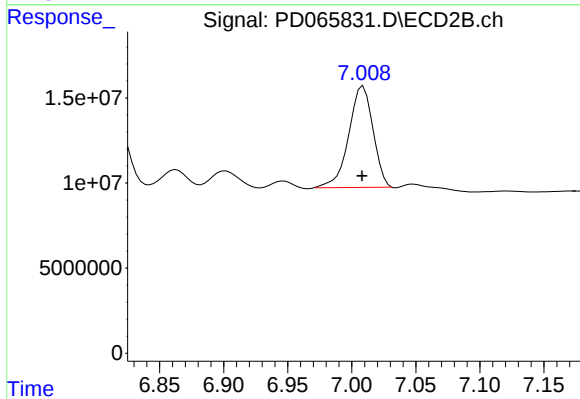

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 78499468
Conc: 422.40 ng/ml

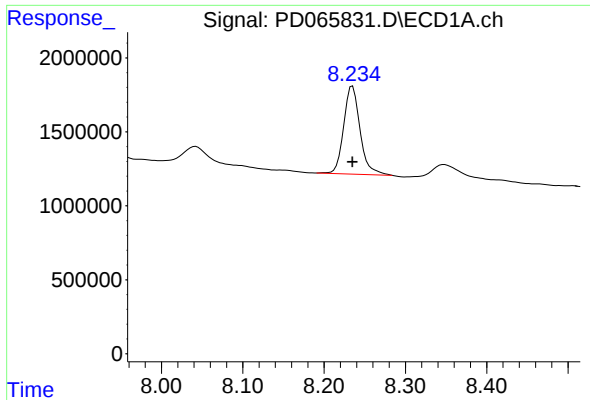

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 8300286
Conc: 6.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

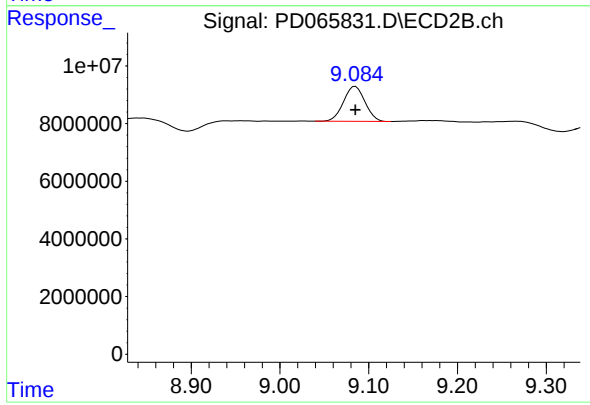

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 20419985
Conc: 5.28 ng/ml