

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
 Data File : PD065836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2021 19:50
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:37:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 23 12:18:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	42643232	266.6E6	57.583	46.430
28)	SA Decachlor...	8.235	9.085	62184045	180.3E6	45.524	46.575
Target Compounds							
23)	Chlordane-1	4.362	5.008	14274532	98878201	426.141	446.577
24)	Chlordane-2	4.862	5.478	18662507	98143964	459.536	424.292
25)	Chlordane-3	5.429	6.125	52273279	355.6E6	443.692	433.570
26)	Chlordane-4	5.487	6.198	43716042	414.6E6	442.630	432.208
27)	Chlordane-5	6.324	7.009	20767420	82446325	427.312	443.642



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092321\
Data File : PD065836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2021 19:50
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:37:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092221.M
Quant Title : GC Extractables
QLast Update : Thu Sep 23 12:18:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

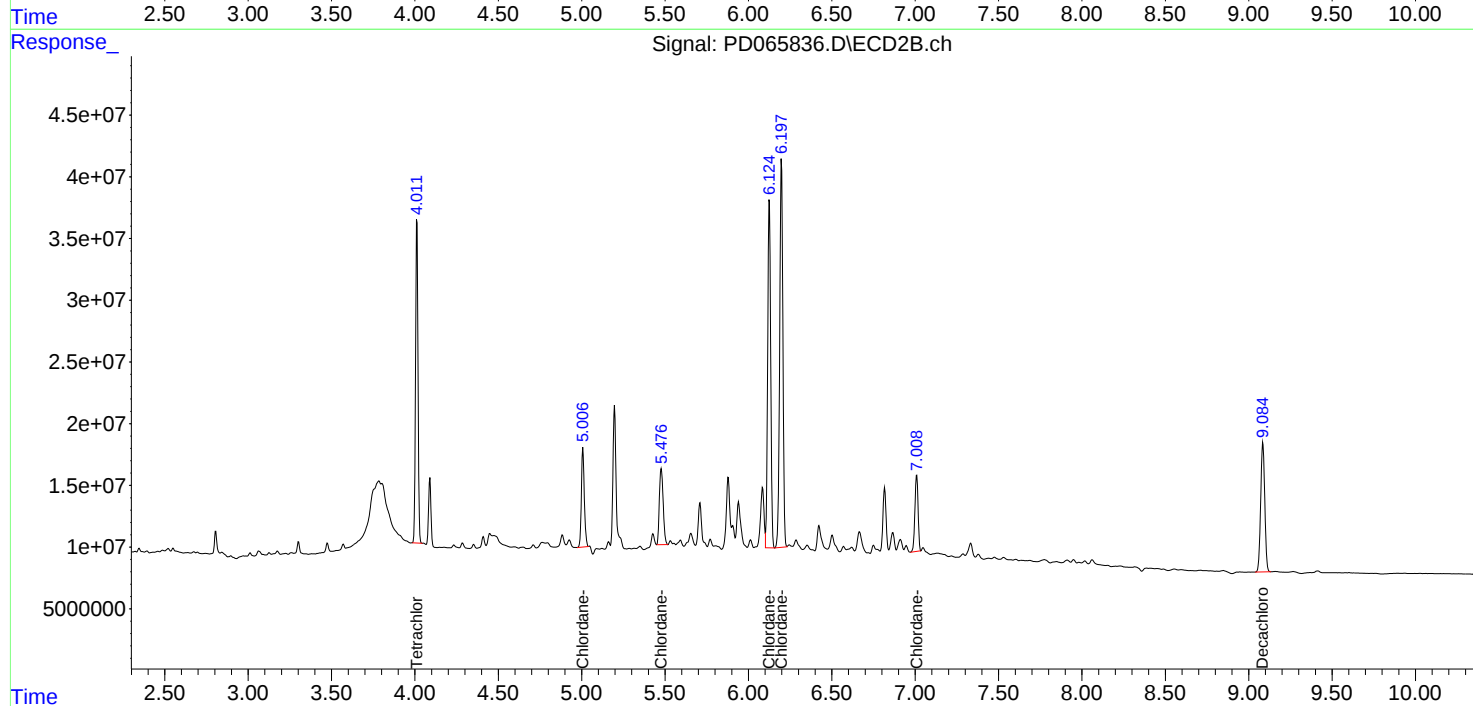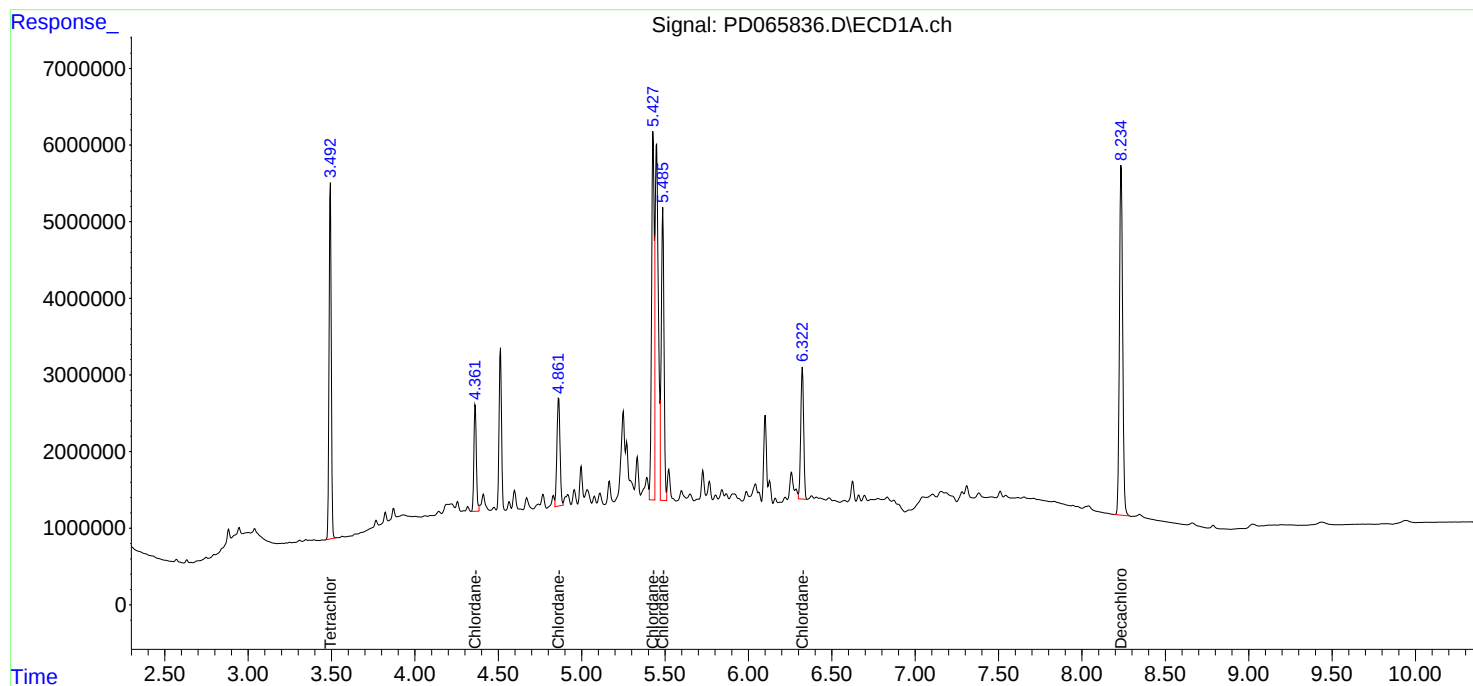


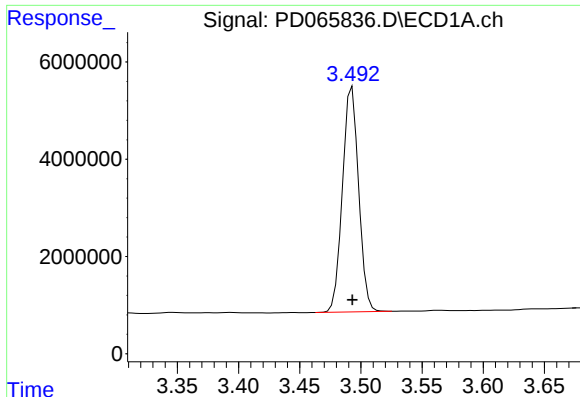

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.000 min
Response: 42643232
Conc: 57.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

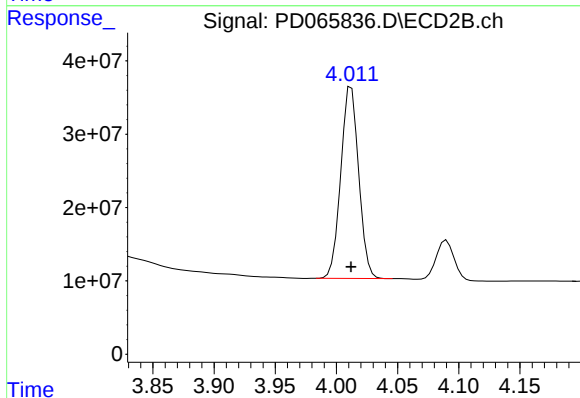


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 266607982
Conc: 46.43 ng/ml

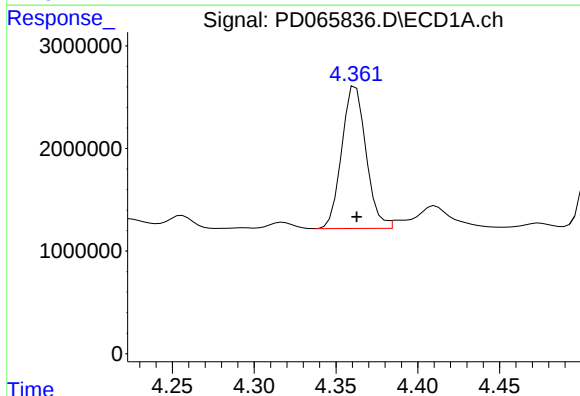


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 14274532
Conc: 426.14 ng/ml

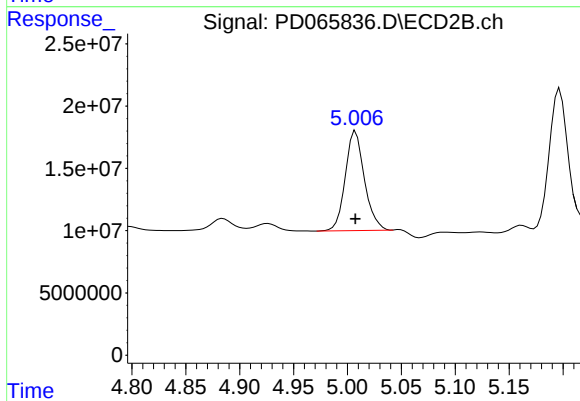

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 98878201
Conc: 446.58 ng/ml

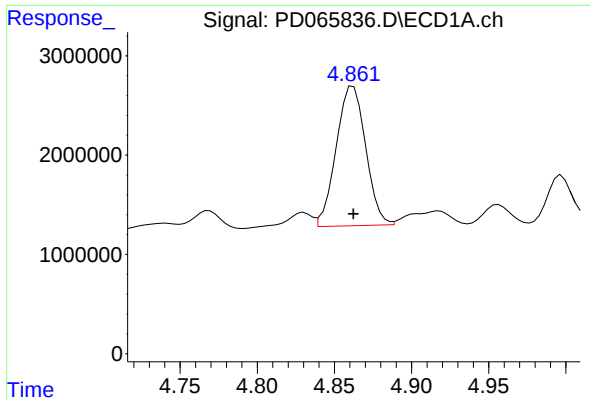

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 18662507
Conc: 459.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

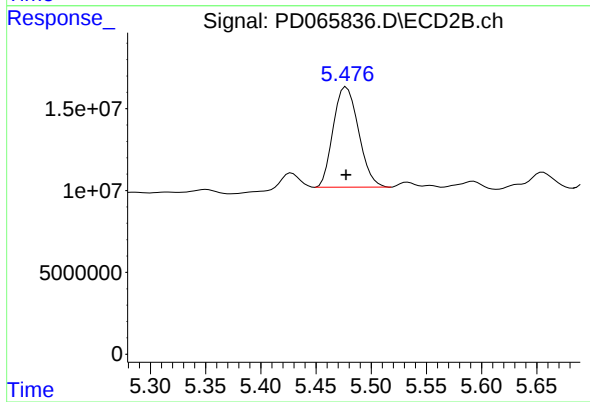


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 98143964
Conc: 424.29 ng/ml

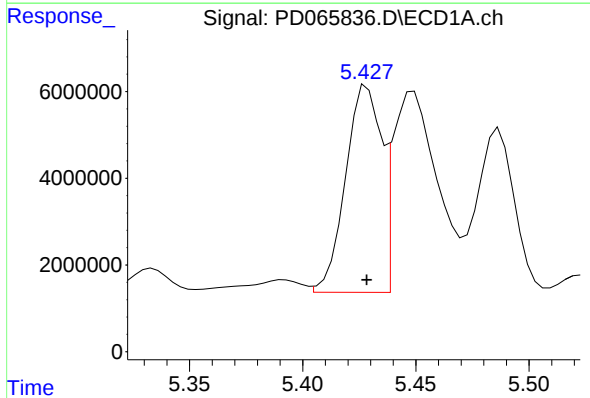


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 52273279
Conc: 443.69 ng/ml

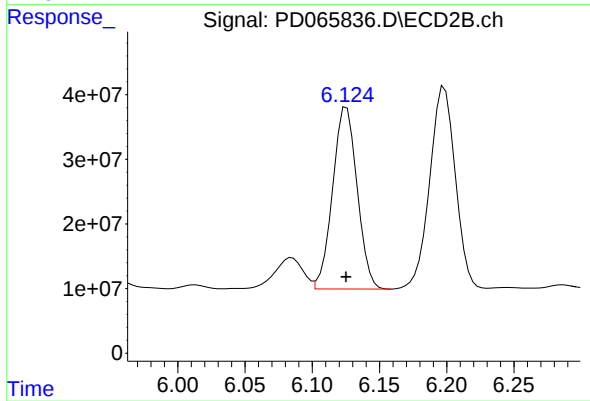

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 355551648
Conc: 433.57 ng/ml

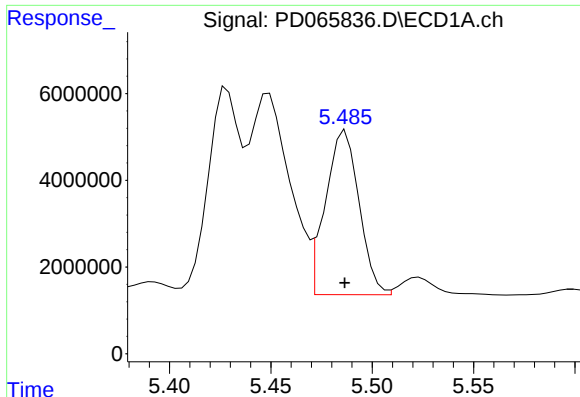

#26 Chlordane-4


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 43716042
Conc: 442.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

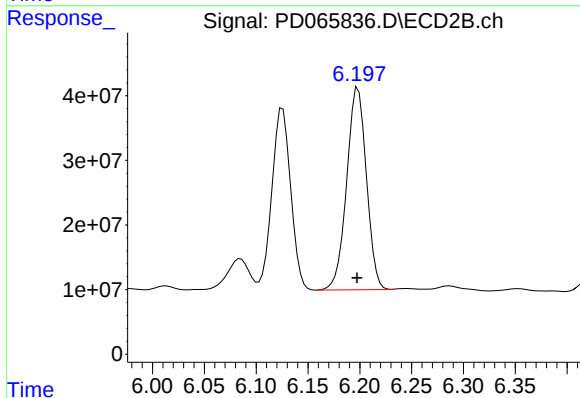


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 414557366
Conc: 432.21 ng/ml

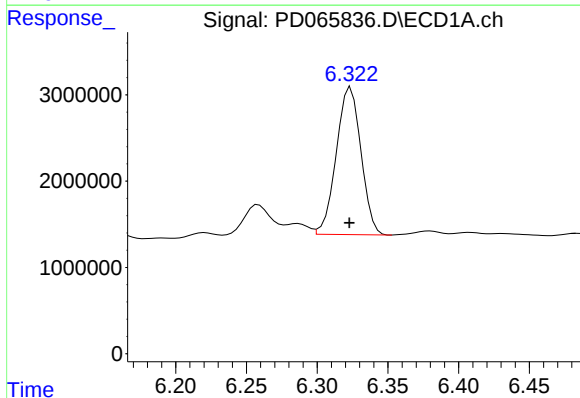


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.001 min
Response: 20767420
Conc: 427.31 ng/ml

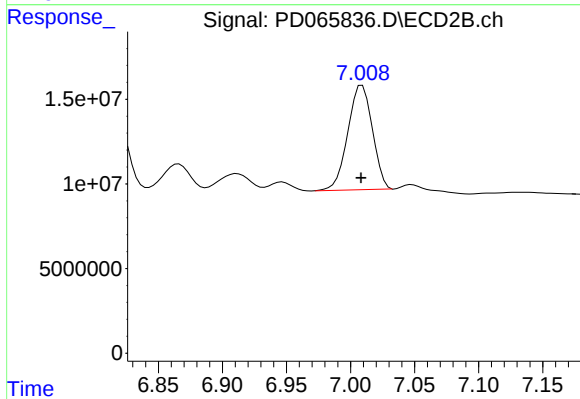

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.001 min
Response: 82446325
Conc: 443.64 ng/ml

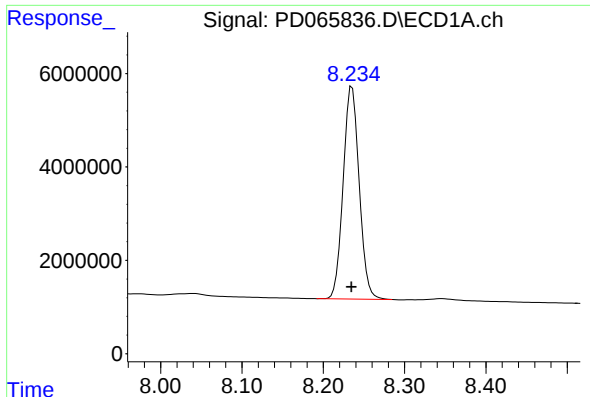

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 62184045
Conc: 45.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

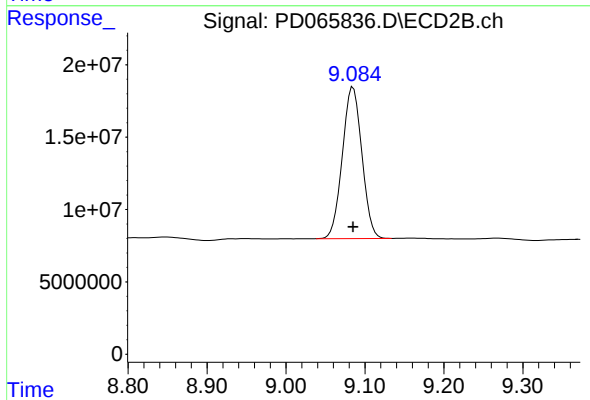

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 180252432
Conc: 46.57 ng/ml