

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
 Data File : PD071983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 11:28
 Operator : AR\AJ
 Sample : PB147818BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS818

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/23/2022
 Supervised By :Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 23:54:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.811	3.563	44728513	629.0E6	17.151	19.196
27)	SA Decachlor...	8.001	9.093	90690028	357.7E6	34.559	37.422
Target Compounds							
2)	A alpha-BHC	3.320	4.030	17051633	231.6E6	4.421	5.250
3)	MA gamma-BHC...	3.654	4.366	17287006	206.3E6	4.682	5.547
4)	MA Heptachlor	4.000	4.944	17184425	160.9E6	4.515	5.958 #
5)	MB Aldrin	4.283	5.286	17384622	137.4E6	4.884	6.358 #
6)	B beta-BHC	3.952	4.573	8250511	82825083	5.194	5.787
7)	B delta-BHC	4.186	4.820	14396275	142.1E6	4.120	5.407m#
8)	B Heptachlo...	4.790	5.718	16295049	107.0E6	4.999	6.329 #
9)	A Endosulfan I	5.164	6.106	15107716	93197510	4.794	5.934
10)	B trans-Chl...	5.043	5.973	16576751	101.7E6	4.896	6.009
11)	B cis-Chlor...	5.108	6.050	16501759	99566447	4.948	6.109
12)	B 4,4'-DDE	5.299	6.224	29531404	178.7E6	9.628	12.246 #
13)	MA Dieldrin	5.431	6.383	31348779	189.0E6	9.053	11.810 #
14)	MA Endrin	5.708	6.616	28263670	147.2E6	9.437	11.191
15)	B Endosulfa...	6.003	6.842	27580409	152.5E6	10.376	12.650
16)	A 4,4'-DDD	5.856	6.748	24961260	144.7E6	9.483	11.826
17)	MA 4,4'-DDT	6.110	7.060	24976389	141.6E6	9.175	11.738 #
18)	B Endrin al...	6.184	6.974	22075035	114.6E6	9.543	11.237
19)	B Endosulfa...	6.408	7.206	25745142	129.6E6	9.664	11.412
20)	A Methoxychlor	6.689	7.536	72290747	327.9E6	50.331	59.755
21)	B Endrin ke...	6.916	7.698	33075636	155.1E6	11.053m	12.534

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092322\
Data File : PD071983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 11:28
Operator : AR\AJ
Sample : PB147818BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 23:54:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

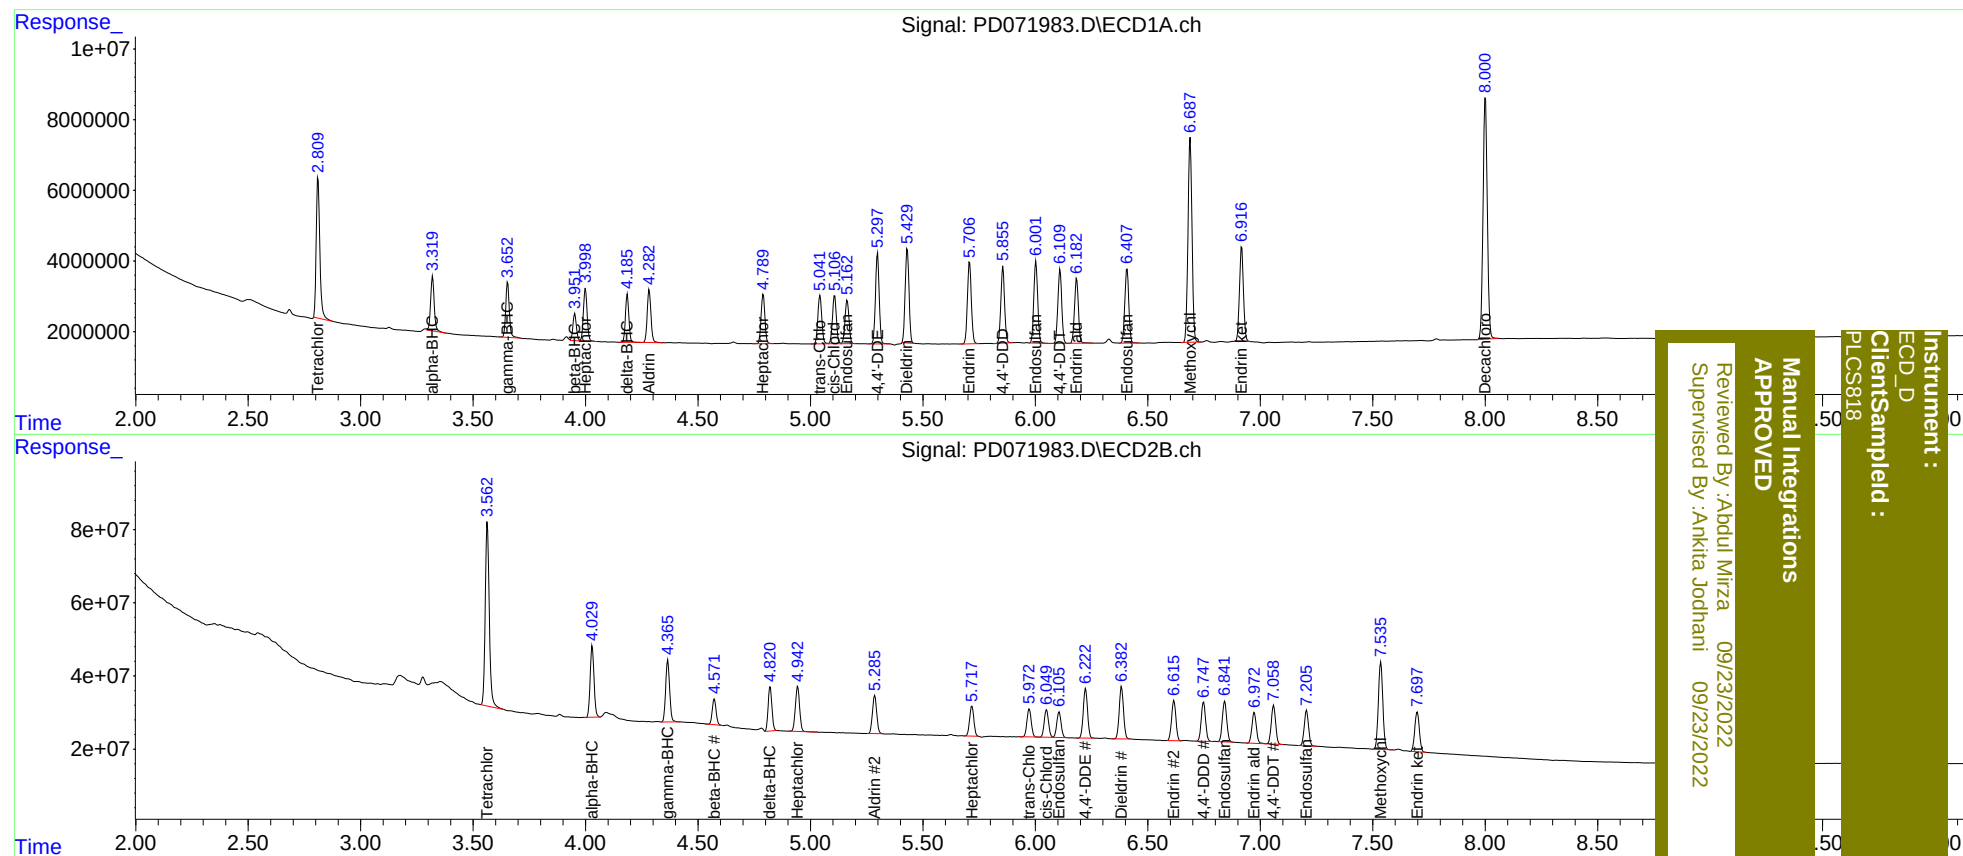

Reviewed By: Abdul Mirza 09/23/2022
Supervised By: Ankita Jodhani 09/23/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS818